

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031758.D
 Acq On : 26 Jul 2023 10:54
 Operator : SY/MD
 Sample : 03754-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

Signal : TIC: VV031758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	235556	261630	15.88%	2.165%
2	1.532	147	153	165	rVB	220556	257500	15.63%	2.131%
3	2.059	308	317	346	rVB	402089	608223	36.92%	5.033%
4	2.680	508	510	512	rBV3	1393	869	0.05%	0.007%
5	2.796	544	546	550	rBV4	1219	840	0.05%	0.007%
6	2.818	550	553	557	rBV5	1461	1265	0.08%	0.010%
7	2.963	595	598	600	rBV4	806	442	0.03%	0.004%
8	2.989	603	606	609	rVV4	1313	948	0.06%	0.008%
9	3.005	609	611	613	rVV3	1298	428	0.03%	0.004%
10	3.014	613	614	617	rVV3	867	333	0.02%	0.003%
11	3.037	619	621	624	rVB3	1975	994	0.06%	0.008%
12	3.069	629	631	633	rBV3	884	377	0.02%	0.003%
13	3.185	664	667	669	rBV4	1214	660	0.04%	0.005%
14	3.211	673	675	678	rVB3	994	516	0.03%	0.004%
15	3.230	678	681	684	rBV5	2022	1355	0.08%	0.011%
16	3.256	688	689	691	rBV2	778	373	0.02%	0.003%
17	3.294	697	701	702	rBV2	1358	756	0.05%	0.006%
18	3.342	713	716	720	rBV5	1086	980	0.06%	0.008%
19	3.362	720	722	724	rBV2	1253	627	0.04%	0.005%
20	3.381	727	728	729	rBV	721	240	0.01%	0.002%
21	3.564	781	785	789	rVB7	1396	1048	0.06%	0.009%
22	3.590	789	793	797	rBV4	1711	1423	0.09%	0.012%
23	3.648	808	811	815	rVB5	1551	840	0.05%	0.007%
24	3.664	815	816	818	rBV2	1084	501	0.03%	0.004%
25	3.728	833	836	839	rBV3	693	472	0.03%	0.004%
26	3.748	839	842	844	rBV5	1329	918	0.06%	0.008%
27	3.793	846	856	886	rBV	127024	375948	22.82%	3.111%
28	4.256	986	1000	1024	rVB	286043	730330	44.34%	6.043%
29	4.574	1096	1099	1100	rBV2	1707	1076	0.07%	0.009%
30	4.857	1185	1187	1190	rVB3	1403	672	0.04%	0.006%
31	4.902	1198	1201	1203	rBV3	1539	1119	0.07%	0.009%
32	4.960	1203	1219	1243	rBV2	610334	1647268	100.00%	13.631%
33	5.471	1375	1378	1381	rBV4	1451	1171	0.07%	0.010%
34	5.538	1386	1399	1421	rBV	390937	821828	49.89%	6.801%
35	5.992	1529	1540	1559	rBV2	395796	811749	49.28%	6.717%
36	6.384	1660	1662	1663	rBV2	1012	357	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031758.D
 Acq On : 26 Jul 2023 10:54
 Operator : SY/MD
 Sample : 03754-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.506	1698	1700	1704	rBV5	1750	1022	0.06%	0.008%
38	6.526	1704	1706	1709	rBV4	1131	565	0.03%	0.005%
39	6.702	1759	1761	1762	rBV	1019	331	0.02%	0.003%
40	6.831	1799	1801	1807	rVB5	1595	1497	0.09%	0.012%
41	6.870	1810	1813	1814	rBV2	1465	691	0.04%	0.006%
42	6.879	1814	1816	1818	rBV3	908	338	0.02%	0.003%
43	6.918	1818	1828	1853	rBV	167659	333843	20.27%	2.763%
44	7.249	1920	1931	1957	rBV	578854	1042600	63.29%	8.627%
45	7.516	2011	2014	2016	rBV3	1699	894	0.05%	0.007%
46	7.558	2018	2027	2050	rBV	128059	237503	14.42%	1.965%
47	8.030	2164	2174	2207	rBV	398466	807832	49.04%	6.685%
48	8.445	2299	2303	2308	rBV7	1751	1930	0.12%	0.016%
49	8.725	2387	2390	2393	rBV4	1482	838	0.05%	0.007%
50	8.789	2399	2410	2432	rBV	643992	1082749	65.73%	8.960%
51	9.326	2574	2577	2580	rBV4	2143	1494	0.09%	0.012%
52	9.345	2580	2583	2584	rVV3	1008	626	0.04%	0.005%
53	9.371	2588	2591	2593	rBV4	1451	879	0.05%	0.007%
54	9.464	2618	2620	2622	rBV3	1001	332	0.02%	0.003%
55	9.593	2658	2660	2662	rVB3	1223	379	0.02%	0.003%
56	9.638	2672	2674	2675	rBV2	1028	371	0.02%	0.003%
57	9.718	2697	2699	2701	rBV3	957	437	0.03%	0.004%
58	9.731	2701	2703	2706	rVV4	984	581	0.04%	0.005%
59	9.773	2710	2716	2719	rBV7	1198	1389	0.08%	0.011%
60	9.837	2733	2736	2740	rBV5	1394	1220	0.07%	0.010%
61	9.873	2744	2747	2748	rBV2	1500	878	0.05%	0.007%
62	9.927	2762	2764	2767	rBV4	974	556	0.03%	0.005%
63	9.950	2769	2771	2772	rBV2	1145	372	0.02%	0.003%
64	10.040	2797	2799	2803	rVB5	1457	718	0.04%	0.006%
65	10.159	2824	2836	2859	rBV	565621	900353	54.66%	7.450%
66	10.426	2916	2919	2921	rBV3	1325	858	0.05%	0.007%
67	10.532	2948	2952	2955	rBV6	2086	2032	0.12%	0.017%
68	10.603	2971	2974	2975	rBV2	1604	914	0.06%	0.008%
69	10.670	2992	2995	2996	rBV3	961	563	0.03%	0.005%
70	10.696	3002	3003	3006	rBV3	1018	631	0.04%	0.005%
71	10.731	3012	3014	3016	rBV3	879	286	0.02%	0.002%
72	10.757	3020	3022	3026	rBV3	763	480	0.03%	0.004%
73	10.844	3043	3049	3050	rBV5	1410	1182	0.07%	0.010%
74	10.902	3065	3067	3068	rBV2	509	270	0.02%	0.002%
75	10.911	3068	3070	3072	rVV3	906	415	0.03%	0.003%
76	10.927	3073	3075	3078	rVB4	1651	857	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031758.D
 Acq On : 26 Jul 2023 10:54
 Operator : SY/MD
 Sample : 03754-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	10.972	3087	3089	3090	rBV	765	263	0.02%	0.002%
78	11.082	3122	3123	3126	rBV3	1193	670	0.04%	0.006%
79	11.191	3145	3157	3185	rBV	626491	988195	59.99%	8.177%
80	11.471	3241	3244	3245	rBV3	1052	596	0.04%	0.005%
81	11.564	3262	3273	3291	rBV	698762	1107761	67.25%	9.167%
82	11.882	3369	3372	3373	rBV3	1790	1083	0.07%	0.009%
83	11.908	3378	3380	3382	rBV2	1050	484	0.03%	0.004%
84	11.988	3402	3405	3408	rBV5	1298	964	0.06%	0.008%
85	12.066	3427	3429	3432	rBV4	1655	750	0.05%	0.006%
86	12.410	3532	3536	3538	rBV4	1312	1086	0.07%	0.009%
87	12.532	3569	3574	3577	rBV5	1907	1686	0.10%	0.014%
88	12.754	3641	3643	3645	rBV2	1155	556	0.03%	0.005%
89	12.943	3700	3702	3704	rBV3	1722	823	0.05%	0.007%
90	13.024	3725	3727	3728	rBV2	1098	346	0.02%	0.003%
91	13.159	3768	3769	3772	rBV2	1188	447	0.03%	0.004%
92	13.178	3772	3775	3778	rBV3	1502	1002	0.06%	0.008%
93	13.310	3814	3816	3818	rBV3	1183	495	0.03%	0.004%
94	13.336	3821	3824	3826	rBV3	1561	1002	0.06%	0.008%
95	13.435	3851	3855	3857	rBV5	2518	1959	0.12%	0.016%
96	13.580	3896	3900	3901	rBV3	1602	1213	0.07%	0.010%
97	13.641	3915	3919	3923	rBV6	1996	1968	0.12%	0.016%
98	13.905	3999	4001	4003	rBV3	1520	482	0.03%	0.004%
99	14.033	4038	4041	4044	rBV4	2206	1812	0.11%	0.015%
100	14.332	4130	4134	4136	rBV6	1600	1335	0.08%	0.011%




Sum of corrected areas: 12084760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031758.D
Acq On : 26 Jul 2023 10:54
Operator : SY/MD
Sample : 03754-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

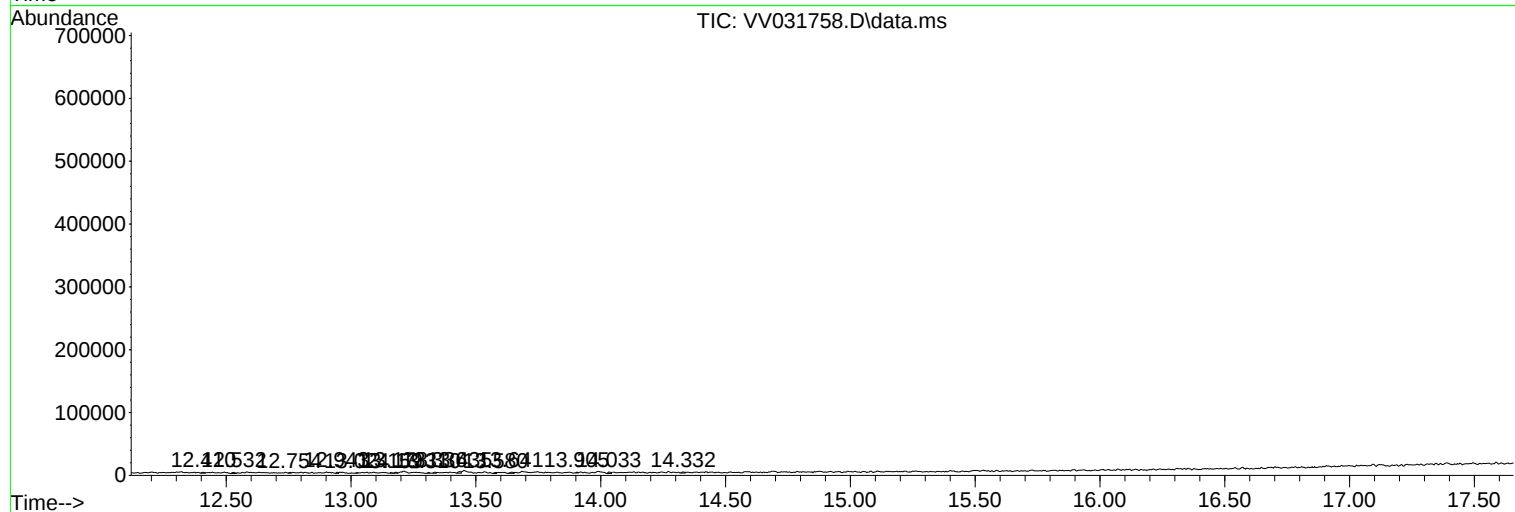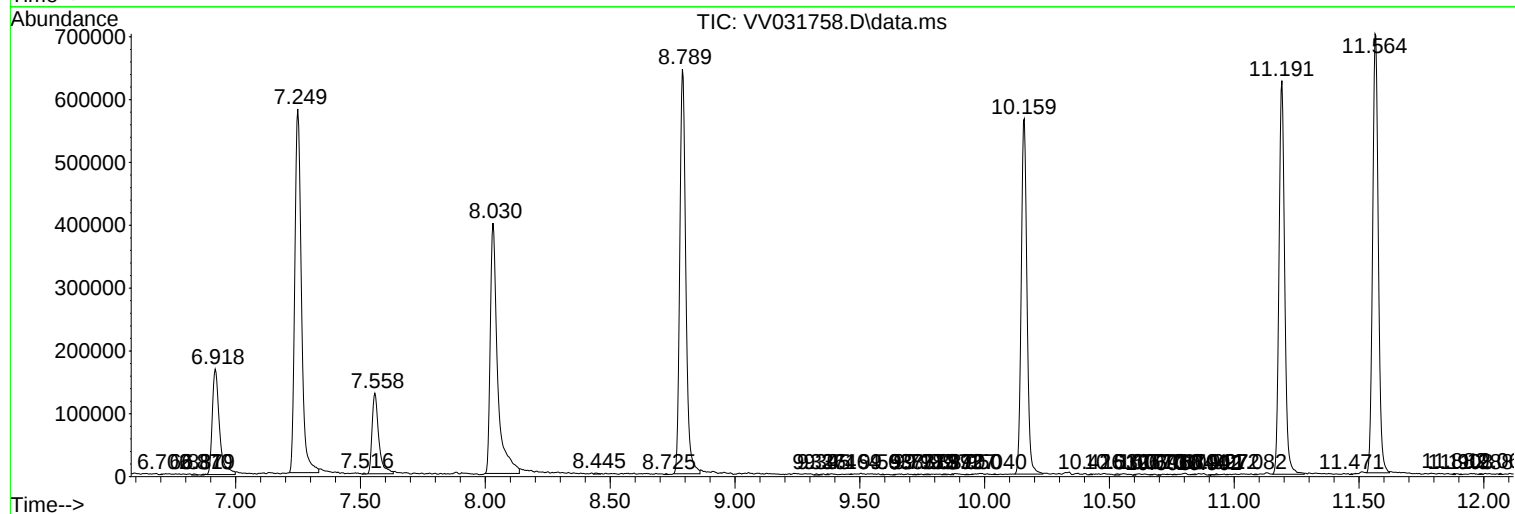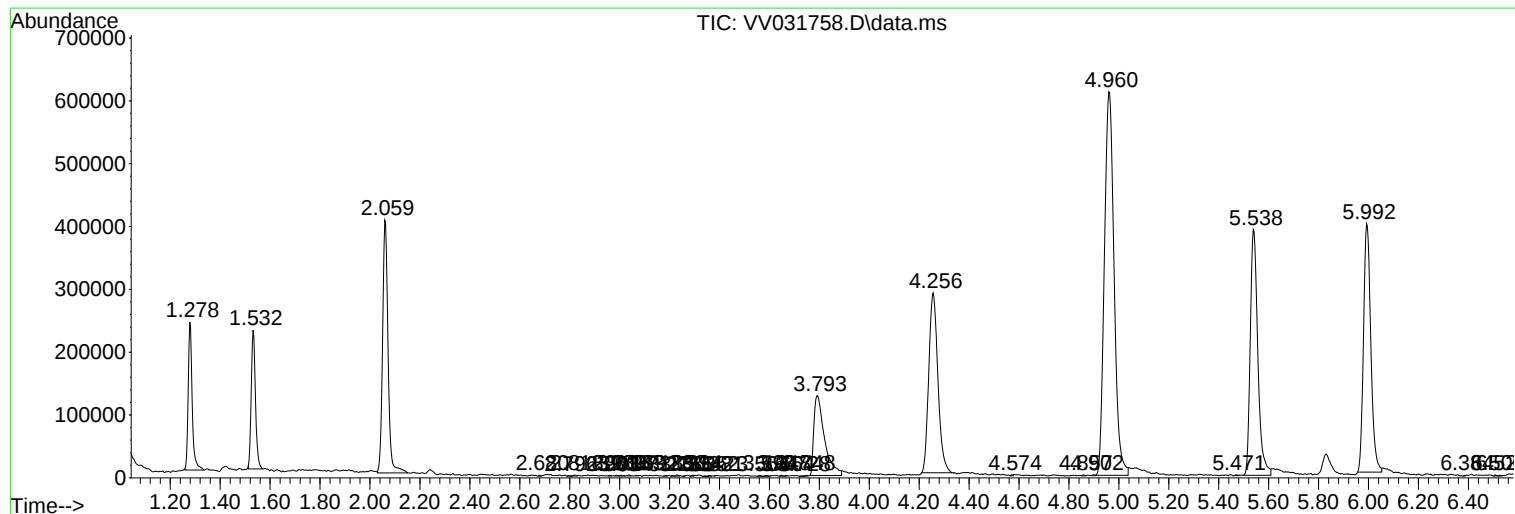

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031758.D
Acq On : 26 Jul 2023 10:54
Operator : SY/MD
Sample : 03754-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031758.D
Acq On : 26 Jul 2023 10:54
Operator : SY/MD
Sample : 03754-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------