

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031768.D
 Acq On : 26 Jul 2023 14:49
 Operator : SY/MD
 Sample : 03754-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	218247	237248	14.60%	1.954%
2	1.532	146	153	168	rVB	207843	252739	15.56%	2.081%
3	2.060	307	317	331	rBV	374000	555176	34.17%	4.571%
4	2.198	358	360	363	rVB3	1699	818	0.05%	0.007%
5	2.230	368	370	375	rVV6	1431	1149	0.07%	0.009%
6	2.281	384	386	389	rVB4	1497	616	0.04%	0.005%
7	2.452	429	439	441	rBV7	2890	3274	0.20%	0.027%
8	2.561	468	473	474	rBV3	1423	1133	0.07%	0.009%
9	2.670	505	507	511	rVB5	1437	1009	0.06%	0.008%
10	2.693	511	514	515	rBV3	1197	618	0.04%	0.005%
11	2.822	551	554	557	rVB2	1168	689	0.04%	0.006%
12	2.844	557	561	564	rVB3	1161	746	0.05%	0.006%
13	2.870	564	569	570	rBV5	1718	1363	0.08%	0.011%
14	2.915	581	583	587	rVB4	905	594	0.04%	0.005%
15	2.950	590	594	595	rBV2	876	678	0.04%	0.006%
16	2.966	595	599	602	rVV5	717	678	0.04%	0.006%
17	2.986	602	605	607	rVV4	1168	788	0.05%	0.006%
18	3.059	627	628	632	rVB2	927	556	0.03%	0.005%
19	3.082	632	635	637	rBV2	795	575	0.04%	0.005%
20	3.114	642	645	647	rBV3	830	593	0.04%	0.005%
21	3.127	647	649	652	rVV3	978	593	0.04%	0.005%
22	3.191	665	669	672	rVV3	971	748	0.05%	0.006%
23	3.429	740	743	746	rBV4	739	598	0.04%	0.005%
24	3.465	749	754	756	rVV3	1053	653	0.04%	0.005%
25	3.484	756	760	764	rVB3	588	608	0.04%	0.005%
26	3.522	770	772	777	rVB4	857	638	0.04%	0.005%
27	3.613	795	800	801	rBV4	811	644	0.04%	0.005%
28	3.641	801	809	812	rBV5	2591	4222	0.26%	0.035%
29	3.793	845	856	885	rBV2	145427	401747	24.73%	3.308%
30	4.092	945	949	950	rBV4	2157	1196	0.07%	0.010%
31	4.256	985	1000	1024	rBV	290449	739218	45.50%	6.087%
32	4.526	1082	1084	1089	rBV6	1184	1121	0.07%	0.009%
33	4.776	1160	1162	1165	rVB4	1557	699	0.04%	0.006%
34	4.963	1203	1220	1249	rBV2	604795	1624637	100.00%	13.377%
35	5.542	1387	1400	1424	rBV	395136	823553	50.69%	6.781%
36	5.831	1479	1490	1508	rBV3	33476	76225	4.69%	0.628%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031768.D
 Acq On : 26 Jul 2023 14:49
 Operator : SY/MD
 Sample : 03754-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	5.995	1529	1541	1558	rBV	394933	802934	49.42%	6.611%
38	6.506	1698	1700	1705	rVB5	2108	1662	0.10%	0.014%
39	6.555	1714	1715	1719	rBV4	1630	1202	0.07%	0.010%
40	6.648	1742	1744	1746	rVB3	1577	677	0.04%	0.006%
41	6.683	1754	1755	1757	rBV2	1395	737	0.05%	0.006%
42	6.786	1785	1787	1790	rVB4	2143	888	0.05%	0.007%
43	6.918	1816	1828	1849	rBV	163864	323477	19.91%	2.664%
44	7.249	1919	1931	1964	rBV	569929	1040188	64.03%	8.565%
45	7.558	2018	2027	2051	rBV	123839	228182	14.05%	1.879%
46	7.796	2097	2101	2105	rVV7	1681	1382	0.09%	0.011%
47	7.825	2108	2110	2114	rVB4	1401	799	0.05%	0.007%
48	7.956	2148	2151	2153	rVB3	1269	668	0.04%	0.006%
49	8.030	2164	2174	2209	rBV	429259	865271	53.26%	7.125%
50	8.567	2339	2341	2343	rBV3	1539	835	0.05%	0.007%
51	8.789	2399	2410	2431	rBV	645840	1087355	66.93%	8.953%
52	9.021	2479	2482	2486	rBV6	1847	1355	0.08%	0.011%
53	9.178	2526	2531	2534	rVB7	1695	1468	0.09%	0.012%
54	9.246	2550	2552	2556	rBV4	1009	843	0.05%	0.007%
55	9.275	2559	2561	2564	rVV3	1343	695	0.04%	0.006%
56	9.442	2610	2613	2616	rVB5	1545	1229	0.08%	0.010%
57	9.461	2616	2619	2621	rBV4	1716	1146	0.07%	0.009%
58	9.500	2628	2631	2633	rBV3	1021	648	0.04%	0.005%
59	9.548	2644	2646	2650	rVB5	1504	844	0.05%	0.007%
60	9.818	2728	2730	2733	rBV4	1092	648	0.04%	0.005%
61	9.886	2749	2751	2755	rVV5	1624	1138	0.07%	0.009%
62	9.982	2779	2781	2783	rBV3	931	570	0.04%	0.005%
63	10.075	2808	2810	2814	rVB4	1611	949	0.06%	0.008%
64	10.159	2824	2836	2864	rBV	577737	911810	56.12%	7.508%
65	10.329	2884	2889	2902	rVB7	6661	9298	0.57%	0.077%
66	10.445	2922	2925	2928	rBV5	1076	774	0.05%	0.006%
67	10.548	2955	2957	2959	rVB3	1966	796	0.05%	0.007%
68	10.567	2960	2963	2964	rBV3	1942	1055	0.06%	0.009%
69	10.683	2998	2999	3001	rBV2	1042	552	0.03%	0.005%
70	10.738	3014	3016	3024	rVB9	2130	1782	0.11%	0.015%
71	11.027	3104	3106	3110	rVB4	1372	784	0.05%	0.006%
72	11.191	3146	3157	3176	rBV	632812	976350	60.10%	8.039%
73	11.358	3207	3209	3214	rVB5	2050	1104	0.07%	0.009%
74	11.567	3263	3274	3297	rVB	697424	1090373	67.11%	8.978%
75	11.754	3329	3332	3337	rBV6	1857	1260	0.08%	0.010%
76	11.947	3390	3392	3394	rBV3	2691	1633	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031768.D
 Acq On : 26 Jul 2023 14:49
 Operator : SY/MD
 Sample : 03754-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.021	3413	3415	3417	rBV3	1667	831	0.05%	0.007%
78	12.120	3444	3446	3450	rVB4	2217	950	0.06%	0.008%
79	12.197	3467	3470	3472	rBV4	2214	1704	0.10%	0.014%
80	12.770	3645	3648	3650	rBV3	989	665	0.04%	0.005%
81	12.831	3664	3667	3673	rVB7	1865	1345	0.08%	0.011%
82	12.924	3694	3696	3698	rBV3	1196	729	0.04%	0.006%
83	12.947	3700	3703	3707	rVB5	1765	1426	0.09%	0.012%
84	12.966	3707	3709	3711	rBV3	1136	637	0.04%	0.005%
85	13.094	3747	3749	3752	rBV4	1538	890	0.05%	0.007%
86	13.139	3761	3763	3767	rVB5	1710	838	0.05%	0.007%
87	13.159	3767	3769	3774	rBV6	1134	886	0.05%	0.007%
88	13.184	3774	3777	3780	rBV5	1804	1211	0.07%	0.010%
89	13.262	3798	3801	3805	rBV5	1995	1720	0.11%	0.014%
90	13.403	3843	3845	3846	rBV2	1810	769	0.05%	0.006%
91	13.590	3901	3903	3905	rBV3	1580	834	0.05%	0.007%
92	13.647	3918	3921	3923	rBV3	2121	1395	0.09%	0.011%
93	13.873	3986	3991	4000	rVB6	12838	17061	1.05%	0.140%
94	13.988	4025	4027	4030	rBV4	2235	1176	0.07%	0.010%
95	14.104	4061	4063	4065	rBV2	1087	633	0.04%	0.005%
96	14.287	4118	4120	4122	rBV2	1542	885	0.05%	0.007%
97	14.477	4177	4179	4183	rBV4	1553	1196	0.07%	0.010%
98	14.741	4258	4261	4263	rBV4	1489	837	0.05%	0.007%
99	14.757	4263	4266	4269	rBV4	2385	1481	0.09%	0.012%
100	14.876	4301	4303	4306	rBV4	1887	1069	0.07%	0.009%




Sum of corrected areas: 12144669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031768.D
Acq On : 26 Jul 2023 14:49
Operator : SY/MD
Sample : 03754-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

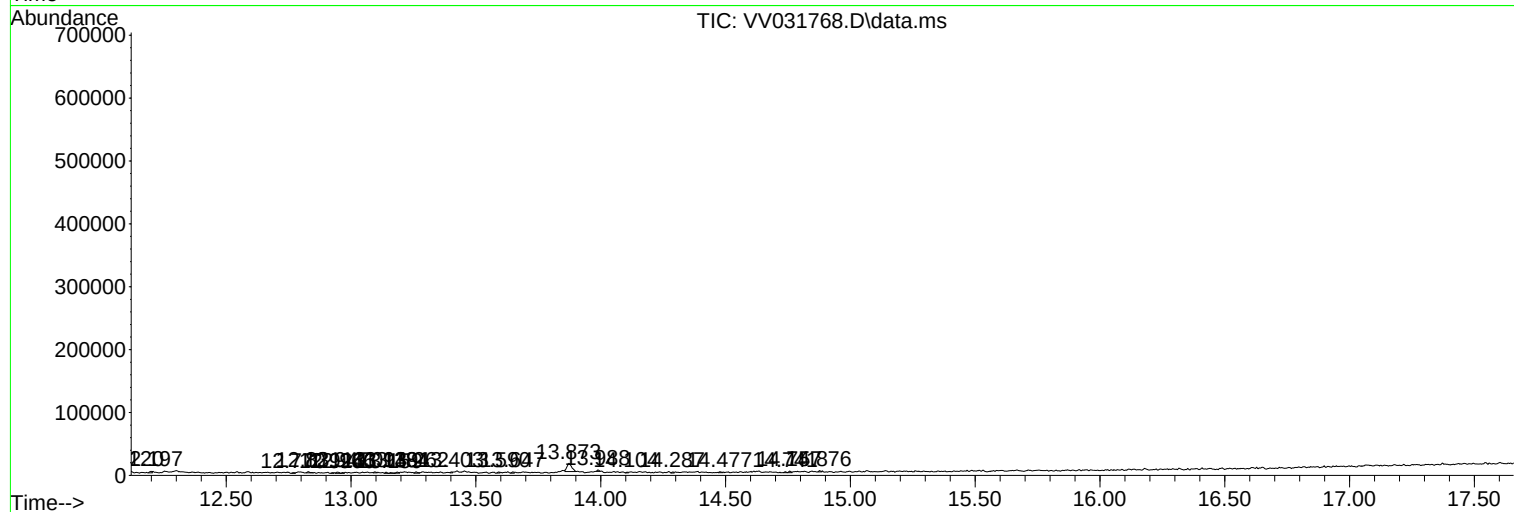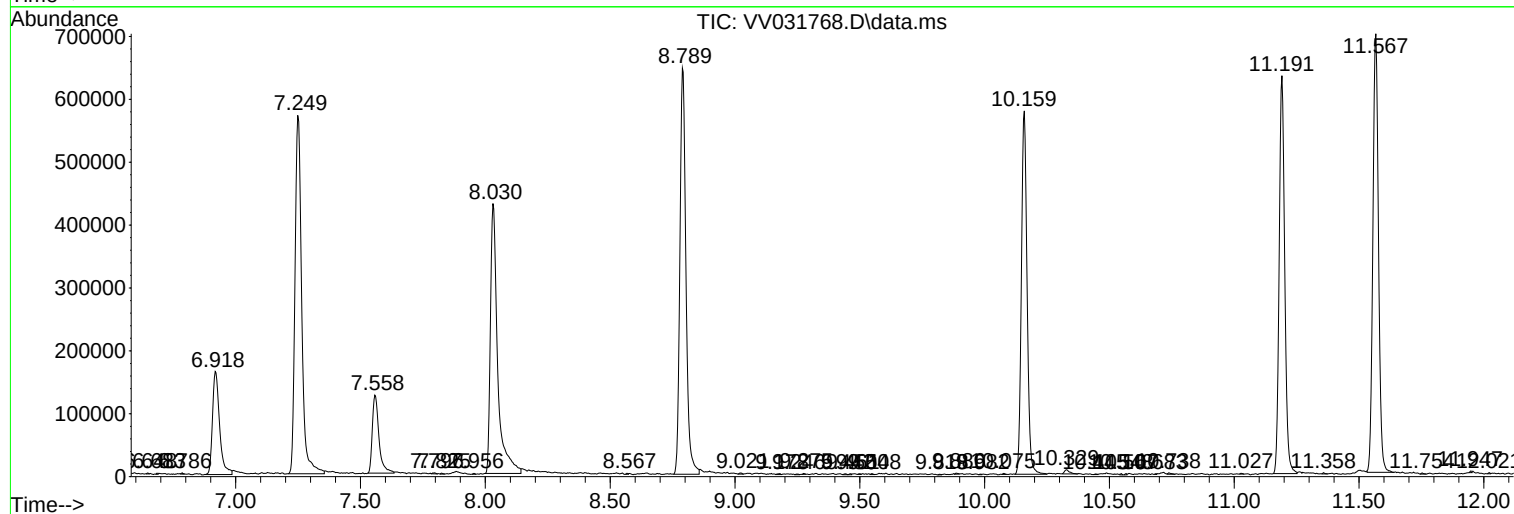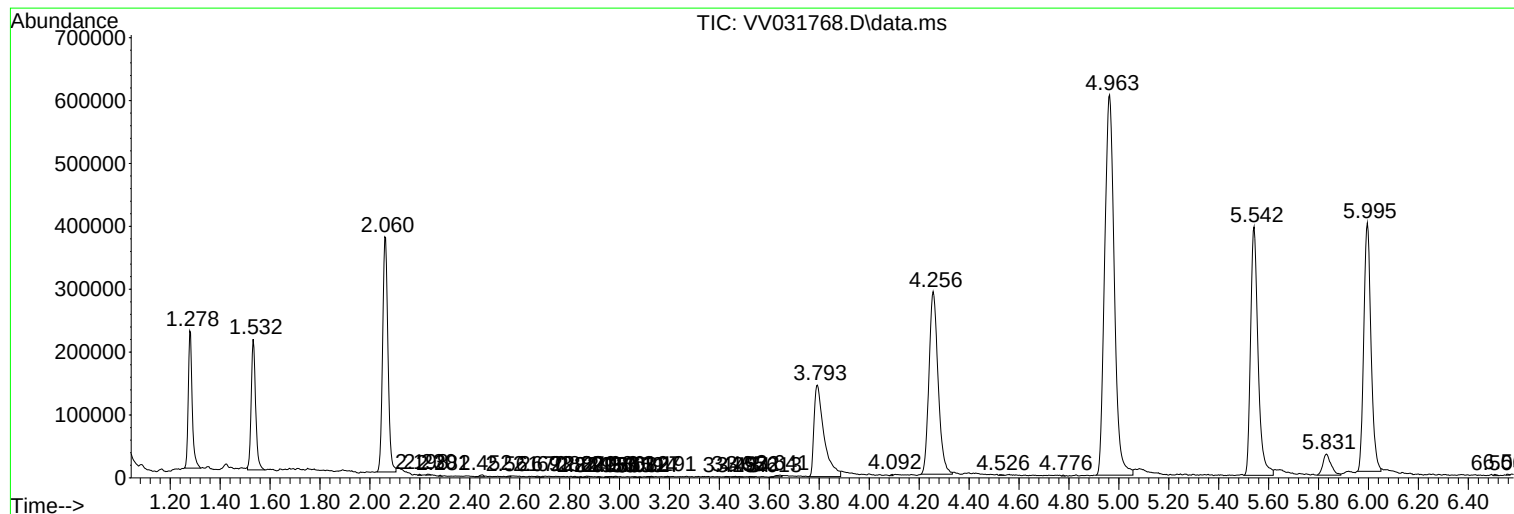

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031768.D
Acq On : 26 Jul 2023 14:49
Operator : SY/MD
Sample : 03754-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031768.D
Acq On : 26 Jul 2023 14:49
Operator : SY/MD
Sample : 03754-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------