

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031771.D
 Acq On : 26 Jul 2023 16:00
 Operator : SY/MD
 Sample : 03712-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	214117	236825	7.84%	1.426%
2	1.532	147	153	170	rVB	207516	253257	8.38%	1.525%
3	2.059	309	317	332	rVB	377945	547655	18.12%	3.298%
4	2.703	505	517	523	rBV7	10737	20240	0.67%	0.122%
5	2.889	572	575	578	rBV4	1385	958	0.03%	0.006%
6	3.018	612	615	616	rBV3	1508	867	0.03%	0.005%
7	3.166	657	661	664	rBV6	1154	942	0.03%	0.006%
8	3.201	669	672	673	rBV3	1355	899	0.03%	0.005%
9	3.259	688	690	691	rBV2	1320	498	0.02%	0.003%
10	3.330	711	712	716	rBV3	961	576	0.02%	0.003%
11	3.494	761	763	765	rBV3	1109	450	0.01%	0.003%
12	3.632	803	806	808	rBV4	1052	598	0.02%	0.004%
13	3.658	810	814	818	rVB5	1603	1475	0.05%	0.009%
14	3.735	836	838	839	rVB2	999	281	0.01%	0.002%
15	3.818	847	864	904	rBV2	551587	1617533	53.51%	9.742%
16	4.256	987	1000	1032	rVB	292302	750218	24.82%	4.518%
17	4.747	1151	1153	1161	rVB7	2200	1695	0.06%	0.010%
18	4.963	1202	1220	1250	rBV2	611054	1659892	54.92%	9.997%
19	5.542	1387	1400	1422	rBV	385080	816025	27.00%	4.915%
20	5.837	1481	1492	1512	rBV6	131927	286870	9.49%	1.728%
21	5.995	1528	1541	1561	rBV	396096	821601	27.18%	4.948%
22	6.866	1809	1812	1816	rVB5	1977	1561	0.05%	0.009%
23	6.918	1816	1828	1845	rBV	173881	330944	10.95%	1.993%
24	7.207	1915	1918	1919	rBV2	1486	827	0.03%	0.005%
25	7.249	1920	1931	1955	rVV	558965	1024005	33.88%	6.167%
26	7.558	2018	2027	2042	rBV	134316	228888	7.57%	1.379%
27	7.911	2124	2137	2164	rBV	1772982	3022596	100.00%	18.205%
28	8.030	2165	2174	2208	rVB	455000	871308	28.83%	5.248%
29	8.464	2303	2309	2316	rBV	2077	3153	0.10%	0.019%
30	8.789	2400	2410	2435	rBV	641919	1072941	35.50%	6.462%
31	9.175	2528	2530	2532	rBV3	1222	710	0.02%	0.004%
32	9.435	2607	2611	2614	rBV5	1893	1690	0.06%	0.010%
33	9.554	2645	2648	2653	rBV6	2057	2005	0.07%	0.012%
34	9.754	2708	2710	2712	rBV2	1024	604	0.02%	0.004%
35	10.159	2824	2836	2858	rBV	579459	931505	30.82%	5.610%
36	10.895	3061	3065	3068	rBV5	1886	1650	0.05%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072623\
 Data File : VW031771.D
 Acq On : 26 Jul 2023 16:00
 Operator : SY/MD
 Sample : 03712-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	11.191	3146	3157	3176	rBV	612405	965388	31.94%	5.814%
38	11.567	3263	3274	3292	rVB	699943	1096209	36.27%	6.602%
39	11.738	3325	3327	3330	rBV4	1230	785	0.03%	0.005%
40	11.805	3345	3348	3350	rBV4	995	684	0.02%	0.004%
41	11.837	3354	3358	3359	rBV3	571	362	0.01%	0.002%
42	11.860	3361	3365	3371	rVB4	1423	1354	0.04%	0.008%
43	11.885	3371	3373	3374	rBV	771	319	0.01%	0.002%
44	11.934	3385	3388	3389	rBV2	1460	672	0.02%	0.004%
45	11.950	3391	3393	3400	rVB6	1918	1861	0.06%	0.011%
46	12.014	3412	3413	3415	rBV2	559	230	0.01%	0.001%
47	12.027	3415	3417	3419	rVV2	715	345	0.01%	0.002%
48	12.088	3433	3436	3437	rBV3	478	274	0.01%	0.002%
49	12.098	3437	3439	3443	rVV4	649	389	0.01%	0.002%
50	12.152	3452	3456	3458	rBV3	1073	711	0.02%	0.004%
51	12.197	3463	3470	3471	rBV6	2044	2042	0.07%	0.012%
52	12.239	3481	3483	3485	rBV	430	172	0.01%	0.001%
53	12.255	3485	3488	3494	rBV6	1367	1236	0.04%	0.007%
54	12.297	3499	3501	3504	rBV4	1105	743	0.02%	0.004%
55	12.374	3523	3525	3527	rVB2	1121	460	0.02%	0.003%
56	12.387	3527	3529	3532	rBV4	900	573	0.02%	0.003%
57	12.413	3534	3537	3540	rBV6	1278	828	0.03%	0.005%
58	12.458	3548	3551	3554	rVV3	788	461	0.02%	0.003%
59	12.474	3554	3556	3558	rVB3	423	161	0.01%	0.001%
60	12.512	3566	3568	3573	rVB5	1558	1131	0.04%	0.007%
61	12.535	3573	3575	3576	rBV2	923	362	0.01%	0.002%
62	12.593	3589	3593	3597	rVB6	1275	1078	0.04%	0.006%
63	12.619	3597	3601	3604	rBV3	1001	726	0.02%	0.004%
64	12.635	3604	3606	3608	rVB2	618	222	0.01%	0.001%
65	12.667	3612	3616	3618	rBV4	1420	876	0.03%	0.005%
66	12.744	3638	3640	3642	rVB2	1564	662	0.02%	0.004%
67	12.760	3642	3645	3646	rBV2	1081	618	0.02%	0.004%
68	12.792	3653	3655	3659	rBV4	1233	816	0.03%	0.005%
69	12.943	3700	3702	3704	rBV3	1376	664	0.02%	0.004%
70	12.969	3708	3710	3713	rVB2	1616	775	0.03%	0.005%
71	13.001	3715	3720	3721	rBV4	1372	1117	0.04%	0.007%
72	13.223	3786	3789	3791	rBV3	2051	1558	0.05%	0.009%
73	13.638	3916	3918	3921	rBV3	1689	1188	0.04%	0.007%
74	14.181	4084	4087	4090	rBV5	1819	1599	0.05%	0.010%

Sum of corrected areas: 16603393




Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031771.D
Acq On : 26 Jul 2023 16:00
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

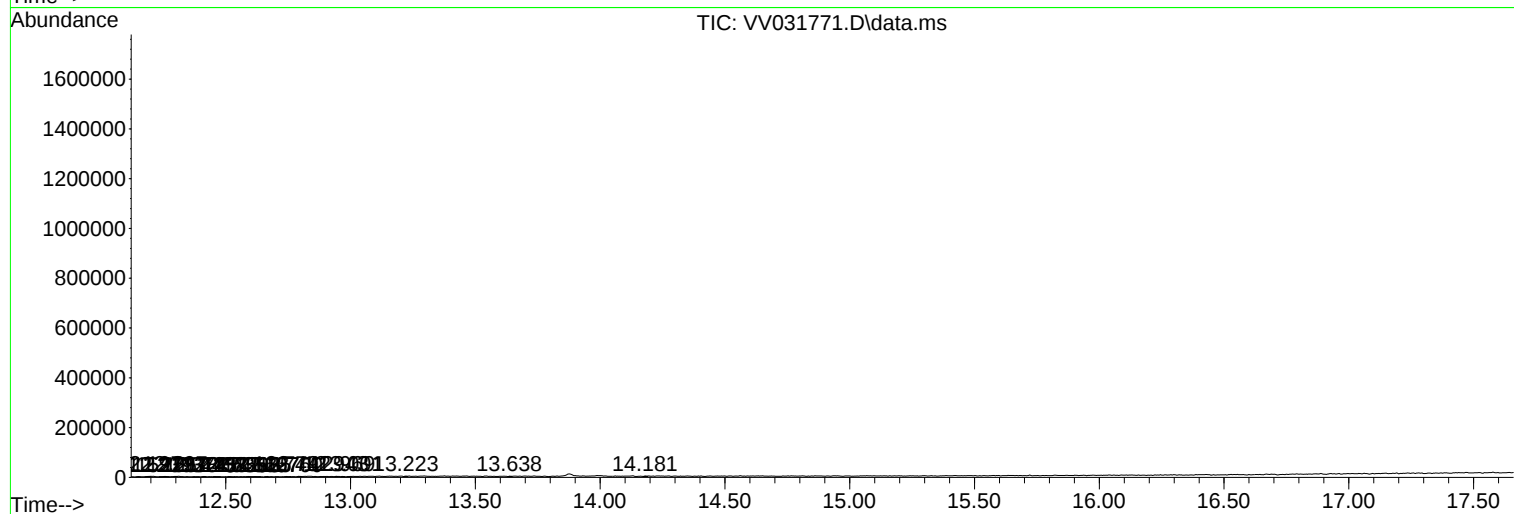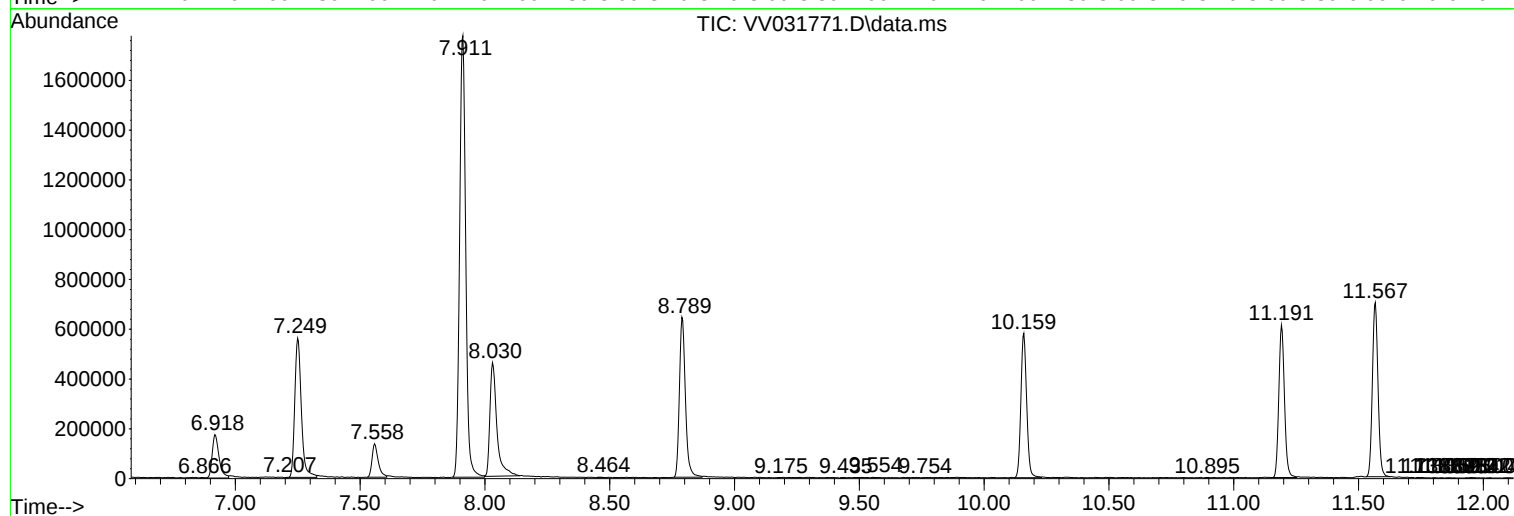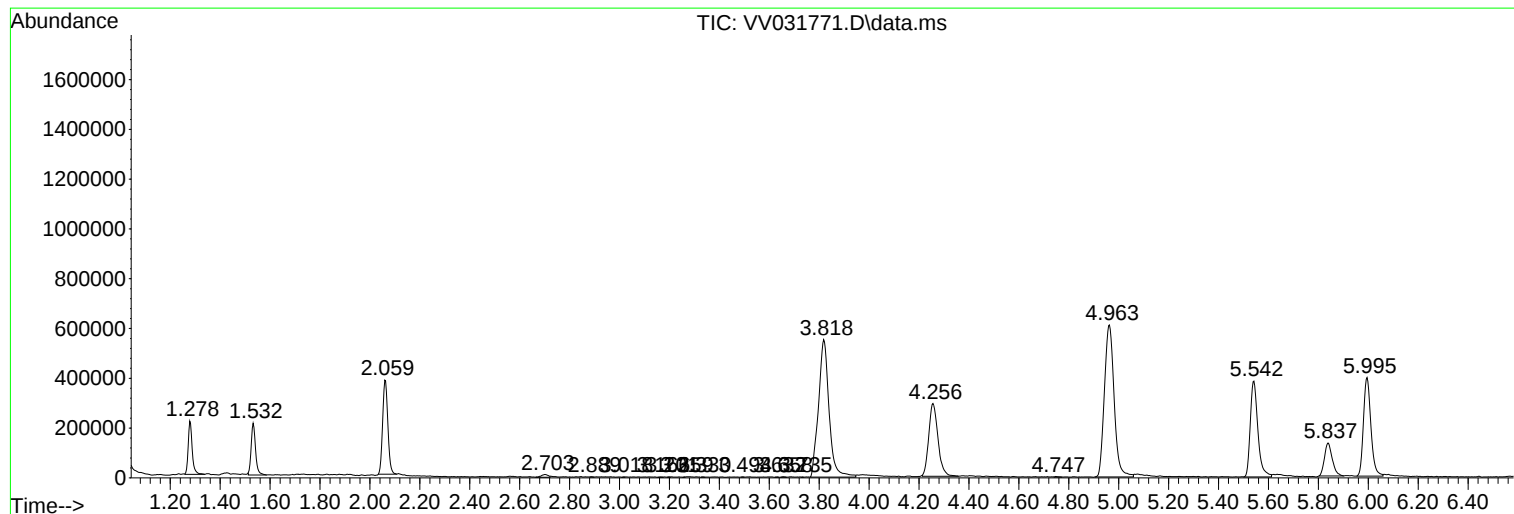

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031771.D
Acq On : 26 Jul 2023 16:00
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031771.D
Acq On : 26 Jul 2023 16:00
Operator : SY/MD
Sample : 03712-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------