

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031772.D
 Acq On : 26 Jul 2023 16:23
 Operator : SY/MD
 Sample : 03712-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	227009	248033	15.30%	2.045%
2	1.532	145	153	164	rBV	204598	244229	15.07%	2.014%
3	2.060	307	317	332	rBV	391790	574952	35.47%	4.740%
4	2.275	381	384	387	rVB4	1860	1100	0.07%	0.009%
5	2.362	408	411	413	rBV3	1295	901	0.06%	0.007%
6	2.449	434	438	439	rBV4	2353	1537	0.09%	0.013%
7	2.558	466	472	473	rBV5	1437	1314	0.08%	0.011%
8	2.706	516	518	522	rVB3	1728	1199	0.07%	0.010%
9	2.728	522	525	528	rBV4	2169	1677	0.10%	0.014%
10	2.748	528	531	536	rVB6	1477	1109	0.07%	0.009%
11	2.860	563	566	570	rBV4	1839	1253	0.08%	0.010%
12	2.979	600	603	605	rBV4	1410	869	0.05%	0.007%
13	3.085	632	636	639	rBV5	1311	1063	0.07%	0.009%
14	3.204	669	673	678	rVB7	1823	1738	0.11%	0.014%
15	3.230	678	681	683	rBV3	1770	1082	0.07%	0.009%
16	3.301	699	703	707	rVB6	1840	1494	0.09%	0.012%
17	3.471	752	756	759	rBV5	1717	1140	0.07%	0.009%
18	3.539	773	777	779	rBV4	1721	1197	0.07%	0.010%
19	3.744	837	841	845	rVB4	1323	1176	0.07%	0.010%
20	3.793	845	856	891	rBV	136503	401323	24.76%	3.309%
21	4.124	955	959	961	rBV5	1226	912	0.06%	0.008%
22	4.256	984	1000	1025	rBV	285538	742672	45.82%	6.123%
23	4.796	1166	1168	1175	rVB5	1035	977	0.06%	0.008%
24	4.960	1202	1219	1245	rBV2	602527	1620986	100.00%	13.365%
25	5.310	1325	1328	1331	rBV4	1356	1000	0.06%	0.008%
26	5.404	1354	1357	1359	rBV4	1995	1036	0.06%	0.009%
27	5.487	1380	1383	1385	rBV4	1766	1189	0.07%	0.010%
28	5.539	1387	1399	1425	rBV	365728	784961	48.42%	6.472%
29	5.767	1466	1470	1473	rBV6	1074	867	0.05%	0.007%
30	5.831	1479	1490	1507	rBV6	28361	64736	3.99%	0.534%
31	5.995	1528	1541	1561	rBV	392666	812251	50.11%	6.697%
32	6.249	1618	1620	1624	rBV5	1312	990	0.06%	0.008%
33	6.468	1682	1688	1692	rBV8	1849	2347	0.14%	0.019%
34	6.526	1702	1706	1707	rBV4	1735	1306	0.08%	0.011%
35	6.551	1711	1714	1718	rBV5	1603	1504	0.09%	0.012%
36	6.648	1741	1744	1747	rBV5	1501	1072	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031772.D
 Acq On : 26 Jul 2023 16:23
 Operator : SY/MD
 Sample : 03712-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.773	1780	1783	1785	rBV4	1386	932	0.06%	0.008%
38	6.918	1818	1828	1845	rBV2	165468	311040	19.19%	2.564%
39	7.249	1918	1931	1969	rBV	560323	1037279	63.99%	8.552%
40	7.558	2015	2027	2042	rBV	122607	228137	14.07%	1.881%
41	7.764	2087	2091	2094	rVB7	1635	1142	0.07%	0.009%
42	7.786	2095	2098	2103	rVV5	2143	1756	0.11%	0.014%
43	7.866	2120	2123	2127	rVB5	2579	1598	0.10%	0.013%
44	7.915	2127	2138	2140	rBV10	5998	9437	0.58%	0.078%
45	8.030	2163	2174	2214	rBV	434276	882607	54.45%	7.277%
46	8.352	2272	2274	2278	rBV5	1847	1233	0.08%	0.010%
47	8.371	2278	2280	2286	rBV6	1686	1686	0.10%	0.014%
48	8.420	2292	2295	2298	rBV6	2553	2176	0.13%	0.018%
49	8.555	2334	2337	2346	rBV10	1916	2093	0.13%	0.017%
50	8.648	2364	2366	2370	rVB4	1669	1005	0.06%	0.008%
51	8.789	2397	2410	2435	rBV	614646	1049491	64.74%	8.653%
52	8.960	2460	2463	2464	rBV3	2405	1197	0.07%	0.010%
53	9.092	2499	2504	2506	rBV5	1681	1314	0.08%	0.011%
54	9.329	2573	2578	2584	rBV8	1840	1944	0.12%	0.016%
55	9.391	2595	2597	2601	rBV4	1432	948	0.06%	0.008%
56	9.497	2627	2630	2635	rVB5	1918	1706	0.11%	0.014%
57	9.522	2635	2638	2644	rBV6	1947	1770	0.11%	0.015%
58	9.789	2718	2721	2724	rBV5	1485	1107	0.07%	0.009%
59	9.963	2769	2775	2778	rBV7	1886	1768	0.11%	0.015%
60	10.159	2823	2836	2857	rBV	568373	910144	56.15%	7.504%
61	10.362	2896	2899	2902	rVB4	1469	871	0.05%	0.007%
62	10.403	2907	2912	2913	rBV5	1344	1163	0.07%	0.010%
63	10.490	2936	2939	2942	rVV4	1417	1269	0.08%	0.010%
64	10.529	2949	2951	2953	rVV2	1772	946	0.06%	0.008%
65	10.542	2953	2955	2961	rVV6	1280	1475	0.09%	0.012%
66	10.580	2965	2967	2971	rVB3	1596	838	0.05%	0.007%
67	10.625	2976	2981	2985	rBV4	1125	1081	0.07%	0.009%
68	10.731	3008	3014	3019	rVB5	965	1008	0.06%	0.008%
69	11.008	3097	3100	3105	rVB4	992	902	0.06%	0.007%
70	11.191	3145	3157	3178	rBV	616792	976956	60.27%	8.055%
71	11.333	3199	3201	3205	rBV4	1433	1057	0.07%	0.009%
72	11.567	3261	3274	3296	rVV	707954	1123448	69.31%	9.263%
73	11.677	3306	3308	3314	rVB7	1341	893	0.06%	0.007%
74	11.847	3358	3361	3364	rBV5	1754	1415	0.09%	0.012%
75	11.960	3395	3396	3400	rVV3	1727	1310	0.08%	0.011%
76	12.014	3408	3413	3415	rBV4	879	834	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
 Data File : VV031772.D
 Acq On : 26 Jul 2023 16:23
 Operator : SY/MD
 Sample : 03712-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.043	3419	3422	3426	rVV6	1369	1076	0.07%	0.009%
78	12.079	3429	3433	3437	rVB5	1367	1254	0.08%	0.010%
79	12.188	3462	3467	3468	rBV4	1592	1444	0.09%	0.012%
80	12.271	3490	3493	3495	rBV3	1179	829	0.05%	0.007%
81	12.561	3580	3583	3585	rBV4	1368	940	0.06%	0.008%
82	12.596	3592	3594	3601	rVB7	2301	1566	0.10%	0.013%
83	12.667	3610	3616	3618	rBV7	1290	1515	0.09%	0.012%
84	12.767	3642	3647	3648	rBV3	1450	1260	0.08%	0.010%
85	12.834	3665	3668	3671	rVB4	1734	1015	0.06%	0.008%
86	12.908	3688	3691	3693	rBV4	1935	1374	0.08%	0.011%
87	12.998	3716	3719	3722	rBV4	2114	1237	0.08%	0.010%
88	13.378	3834	3837	3839	rBV4	1745	828	0.05%	0.007%
89	13.622	3911	3913	3917	rBV4	1731	1245	0.08%	0.010%
90	13.689	3932	3934	3937	rVB4	1921	1189	0.07%	0.010%
91	13.747	3950	3952	3955	rVV4	1554	1017	0.06%	0.008%
92	14.024	4034	4038	4042	rBV6	1824	2067	0.13%	0.017%
93	14.062	4047	4050	4052	rBV4	1295	858	0.05%	0.007%
94	14.162	4079	4081	4083	rBV3	1593	897	0.06%	0.007%
95	14.226	4099	4101	4106	rVB6	3063	2256	0.14%	0.019%
96	14.329	4127	4133	4134	rBV6	2078	2212	0.14%	0.018%
97	14.400	4152	4155	4158	rBV5	1695	1261	0.08%	0.010%
98	14.535	4193	4197	4199	rBV5	2403	2165	0.13%	0.018%
99	14.789	4273	4276	4279	rVB4	2735	1486	0.09%	0.012%
100	14.963	4327	4330	4334	rBV5	1986	1823	0.11%	0.015%




Sum of corrected areas: 12128982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031772.D
Acq On : 26 Jul 2023 16:23
Operator : SY/MD
Sample : 03712-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

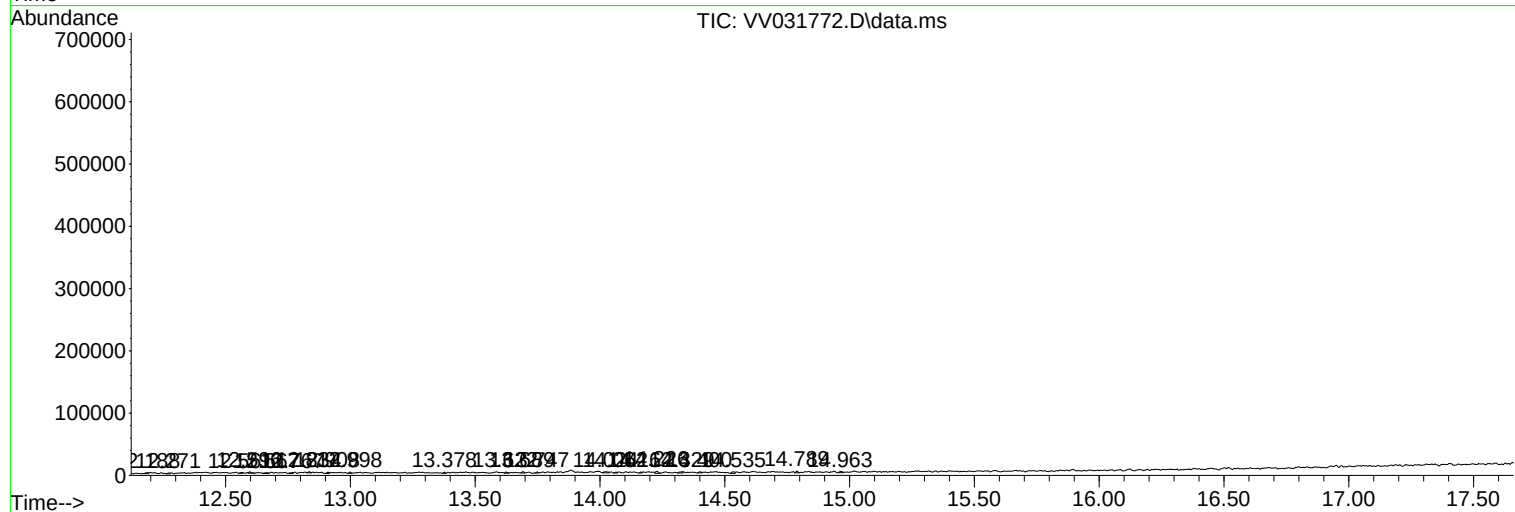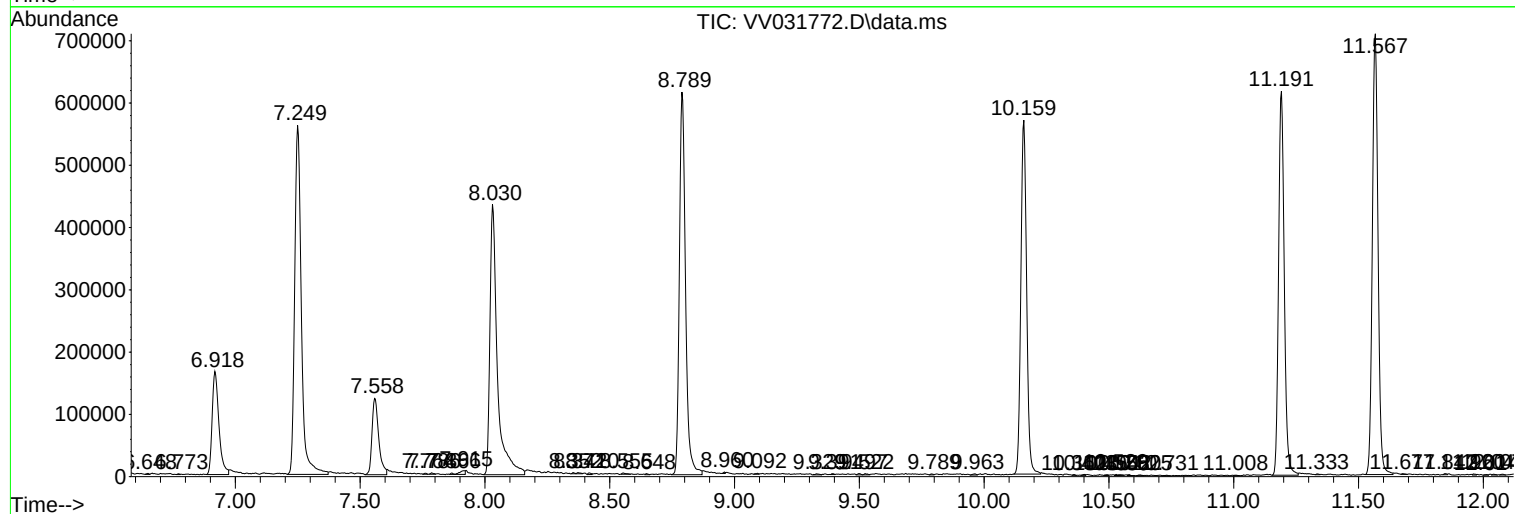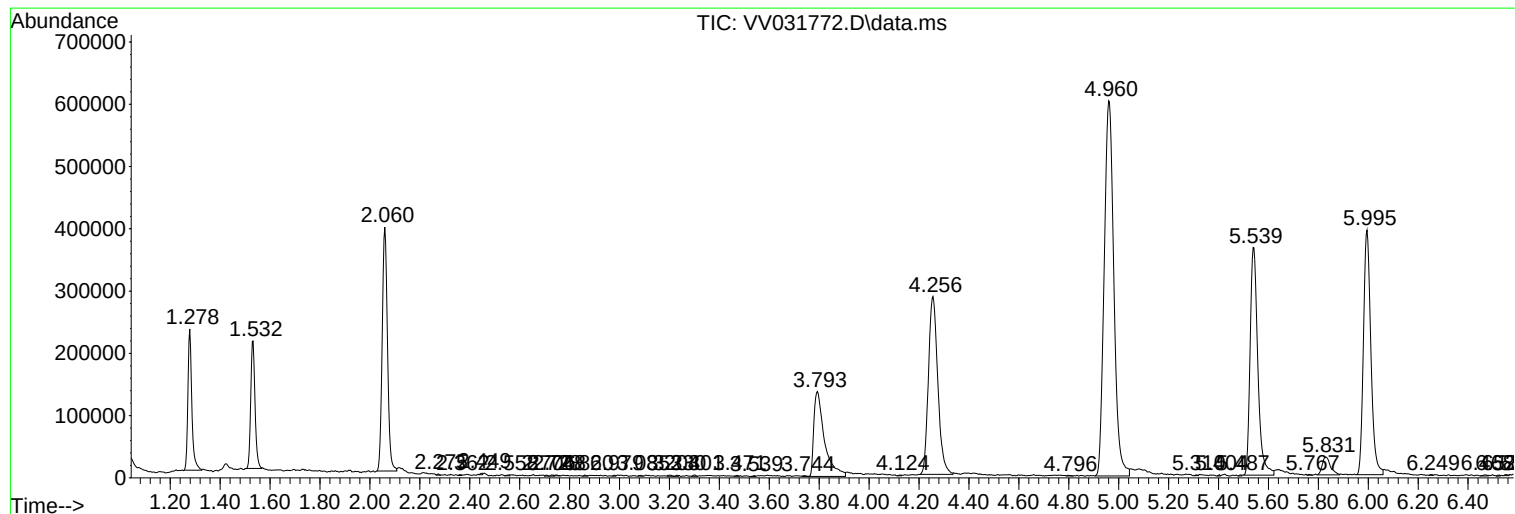

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031772.D
Acq On : 26 Jul 2023 16:23
Operator : SY/MD
Sample : 03712-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031772.D
Acq On : 26 Jul 2023 16:23
Operator : SY/MD
Sample : 03712-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------