
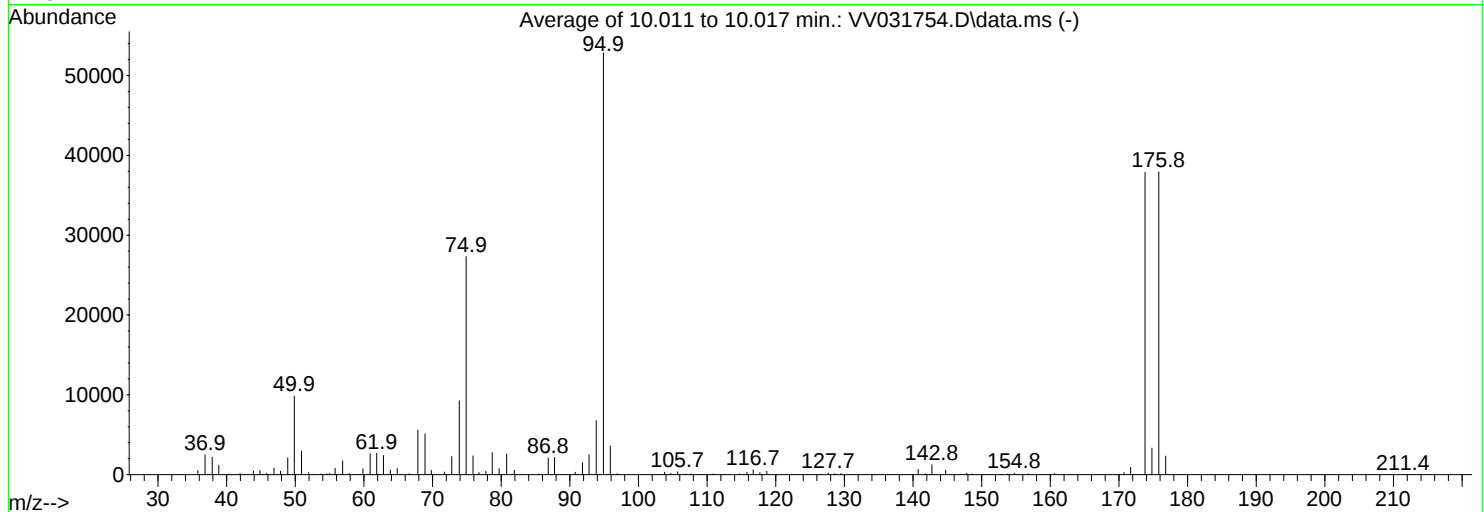


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072623\
Data File : VV031754.D
Acq On : 26 Jul 2023 08:31
Operator : SY/MD
Sample : BFB399
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB399

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis
Last Update : Thu Jul 27 05:18:30 2023

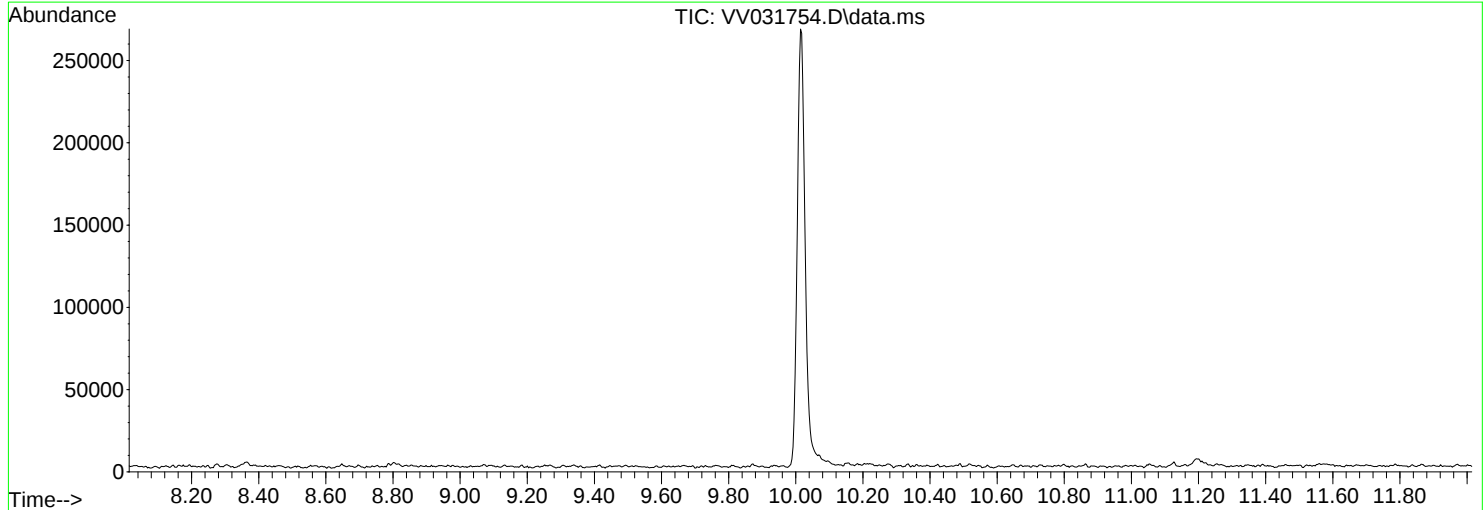

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9845	PASS
75	95	30	80	51.7	27333	PASS
95	95	100	100	100.0	52848	PASS
96	95	5	9	6.8	3594	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.6	37864	PASS
175	174	5	9	8.8	3339	PASS
176	174	95	105	100.2	37931	PASS
177	176	5	10	6.1	2324	PASS

m/z	Abundance
35.80	611.0
36.80	2198.0
37.90	2074.0
38.90	1100.0
39.70	450.0
41.90	124.0
42.60	114.0
43.90	1191.0
44.80	569.0
45.80	162.0
46.90	833.0
47.90	451.0
48.90	1985.0
49.90	9123.0
50.90	2845.0
52.00	324.0
53.60	189.0
54.60	135.0
55.00	119.0
55.70	692.0
56.90	1737.0
57.80	117.0
59.90	645.0
60.90	2761.0
61.90	2522.0
62.90	2334.0
63.80	573.0
64.80	732.0
66.60	217.0
67.90	5305.0
68.90	5158.0
69.80	514.0
71.80	479.0
72.80	2376.0
73.90	8658.0
74.90	26144.0
75.90	2161.0
76.80	458.0
77.80	447.0
78.70	2657.0
79.70	637.0
80.80	2532.0
81.90	492.0
82.70	138.0
86.80	1773.0
87.80	2191.0
90.80	328.0
91.80	1626.0
92.80	2415.0
93.90	6422.0
94.90	50072.0
95.90	3543.0
96.90	111.0
103.80	288.0
104.70	121.0
105.70	339.0
106.80	144.0
110.90	111.0
115.80	246.0
116.70	523.0
117.70	211.0
118.70	410.0
127.60	214.0
128.50	101.0
129.50	159.0
140.70	620.0
141.80	117.0
142.70	1273.0
144.70	557.0
147.80	119.0
152.90	100.0
154.70	195.0
156.80	182.0
160.60	111.0
170.90	191.0
171.70	709.0
173.80	35096.0
174.80	3274.0
175.80	34912.0
176.80	2172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
35.80	724.0
36.90	2589.0
37.90	2246.0
38.80	1272.0
39.70	510.0
40.70	107.0
42.00	155.0
43.90	1188.0
44.80	522.0
45.80	191.0
46.90	875.0
47.90	469.0
48.90	2221.0
49.80	10340.0
50.90	3000.0
52.00	282.0
53.60	183.0
54.60	154.0
55.00	154.0
55.80	780.0
56.90	1779.0
57.90	179.0
59.80	743.0
60.90	2669.0
61.80	2807.0
62.90	2366.0
63.80	611.0
64.80	768.0
66.60	156.0
67.80	5688.0
68.90	5189.0
69.80	579.0
71.70	435.0
72.80	2309.0
73.90	9640.0
74.90	28384.0
75.90	2395.0
76.70	424.0
77.70	455.0
78.70	2855.0
79.70	809.0
80.80	2721.0
81.90	591.0
82.70	130.0
85.50	126.0
86.80	2079.0
87.80	2290.0
90.80	290.0
91.80	1513.0
92.80	2626.0
93.80	6981.0
94.90	54560.0
95.90	3729.0
96.90	124.0
103.80	302.0
104.70	152.0
105.70	327.0
106.80	107.0
107.70	111.0
110.90	117.0
114.70	137.0
115.80	345.0
116.70	620.0
117.70	245.0
118.70	412.0
127.70	214.0
128.60	128.0
129.50	151.0
140.70	697.0
141.90	135.0
142.70	1298.0
144.70	568.0
147.80	156.0
148.60	124.0
153.80	115.0
154.70	194.0
156.80	113.0
160.60	174.0
170.70	241.0
171.70	952.0
173.80	38888.0
174.80	3552.0
175.80	39272.0
176.80	2353.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
35.80	751.0
36.90	2647.0
37.90	2208.0
38.80	1202.0
39.70	596.0
40.30	204.0
41.90	174.0
43.90	1057.0
44.90	451.0
45.40	202.0
45.90	194.0
46.90	787.0
47.80	423.0
48.90	2115.0
49.90	10073.0
50.90	2979.0
51.90	240.0
52.60	100.0
53.70	204.0
55.00	205.0
55.90	943.0
56.90	1650.0
57.90	185.0
59.80	758.0
60.90	2448.0
61.80	2666.0
62.80	2517.0
63.90	573.0
64.90	779.0
67.80	5702.0
68.90	4980.0
69.80	518.0
71.70	384.0
72.80	2101.0
73.90	9433.0
74.90	27472.0
75.90	2496.0
76.80	433.0
77.70	343.0
78.70	2778.0
79.70	842.0
80.80	2537.0
81.90	559.0
82.90	118.0
85.50	115.0
86.90	2403.0
87.70	2044.0
90.80	274.0
91.90	1329.0
92.80	2480.0
93.90	6913.0
94.90	53912.0
95.90	3511.0
96.90	107.0
103.80	297.0
104.70	199.0
105.70	348.0
107.80	124.0
114.70	140.0
115.80	325.0
116.70	680.0
117.70	267.0
118.70	436.0
124.70	139.0
127.70	196.0
128.70	129.0
129.50	139.0
134.60	114.0
140.80	690.0
141.90	109.0
142.80	1160.0
144.80	570.0
147.80	196.0
148.60	135.0
153.80	113.0
154.80	216.0
160.60	216.0
169.70	101.0
170.70	335.0
171.70	1044.0
173.80	39608.0
174.80	3192.0
175.80	39608.0
176.80	2447.0
211.40	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
35.90	165.0
38.30	146.0
39.90	586.0
41.20	168.0
43.90	683.0
53.80	120.0
58.70	109.0
66.00	110.0
70.70	104.0
71.80	106.0
76.80	183.0
82.60	114.0
103.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399