


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017679.D
Acq On : 27 Jul 2020 15:30
Operator : SY/MD
Sample : L3459-03MSD
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY43MSD

Manual Integrations
APPROVED

MMDadoda
7/29/2020 11:40:46 AM

Quant Time: Jul 28 06:19:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

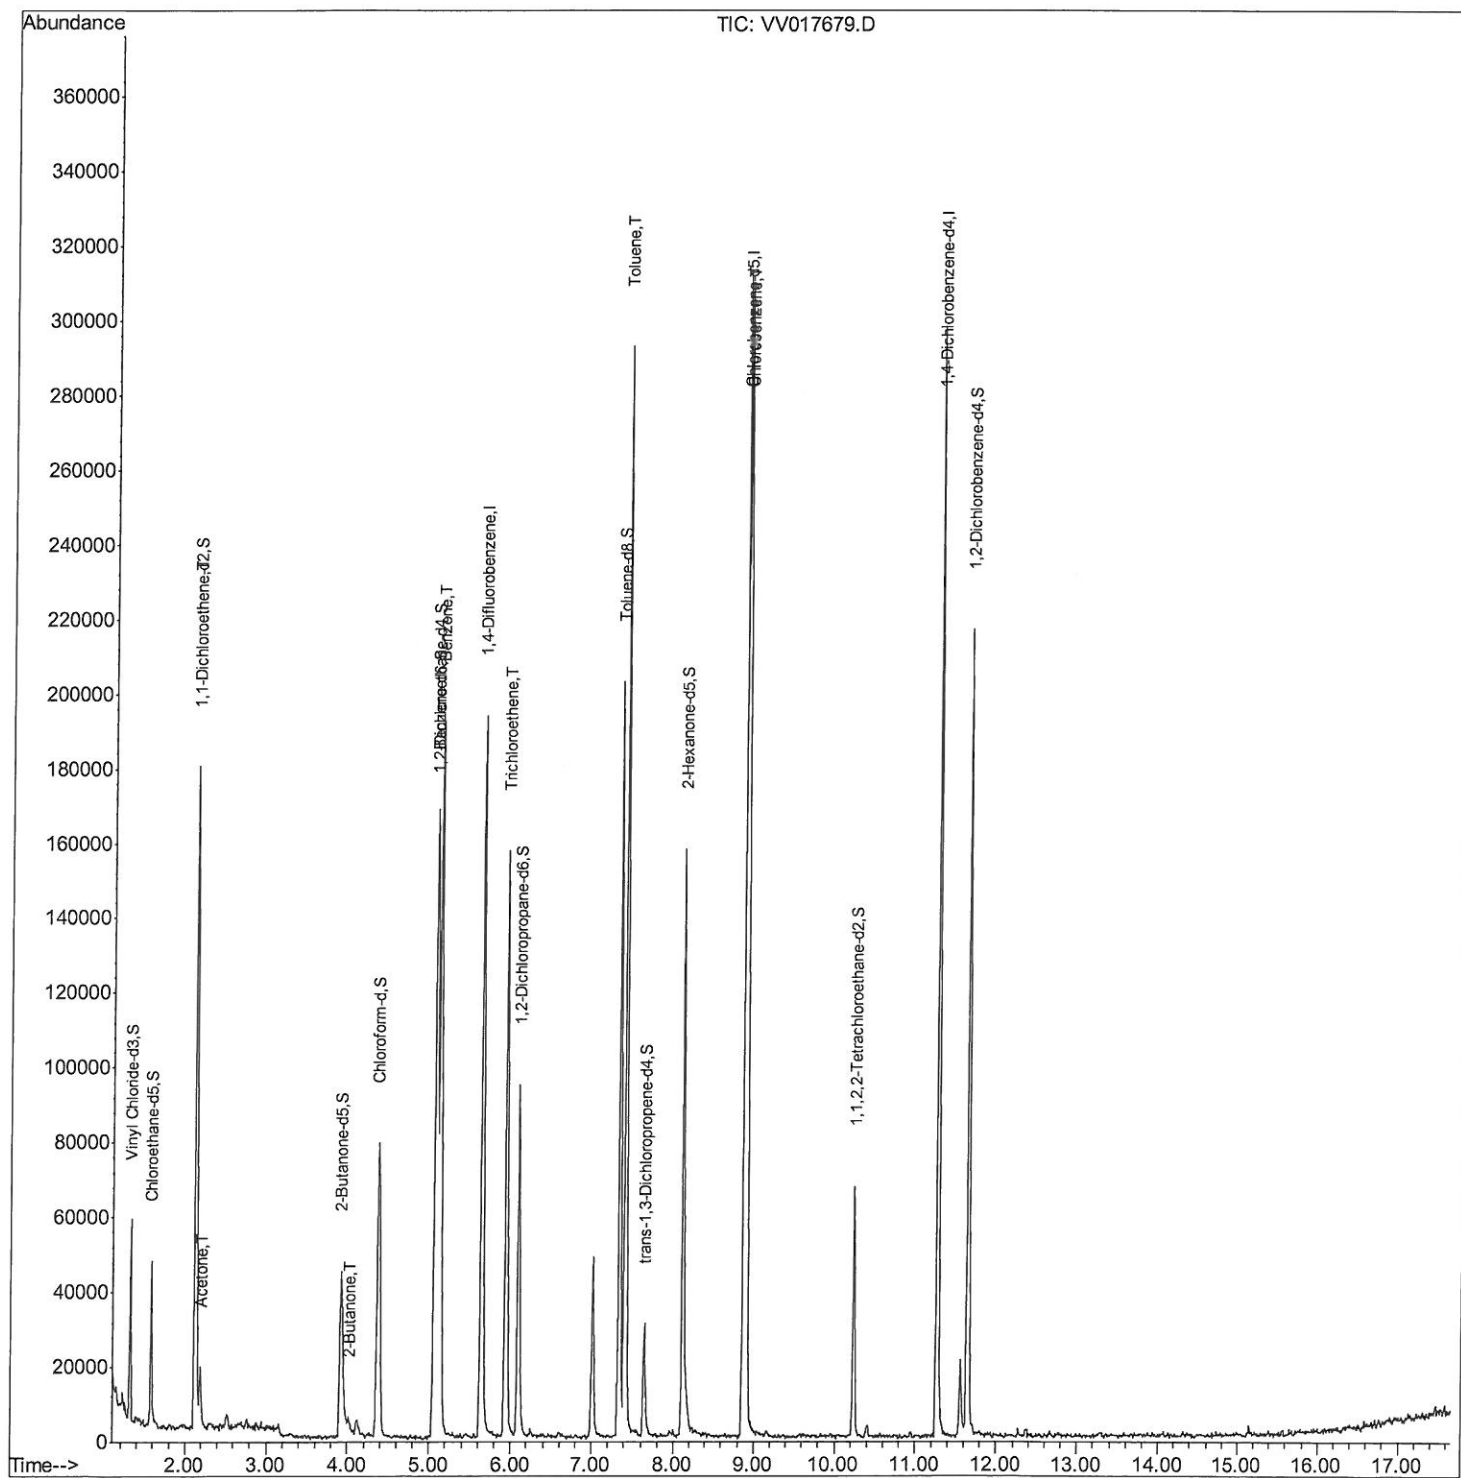

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017679.D
 Acq On : 27 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3459-03MSD
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 GAY43MSD

Manual Integrations
APPROVED

MMDadoda
 7/29/2020 11:40:46 AM

Quant Time: Jul 28 04:56:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

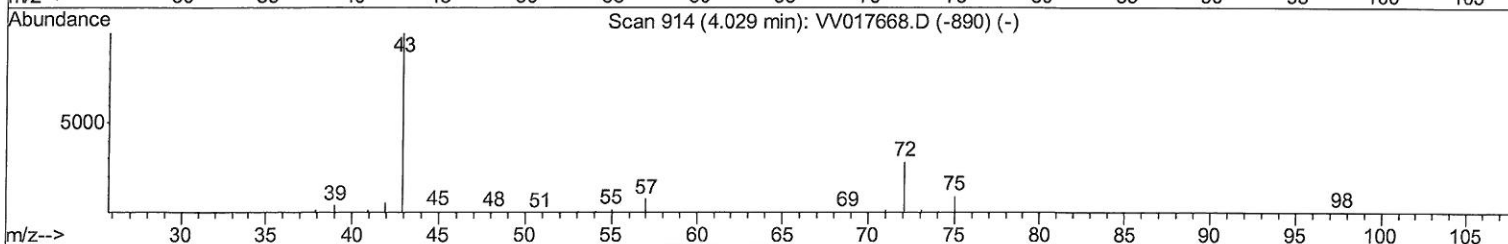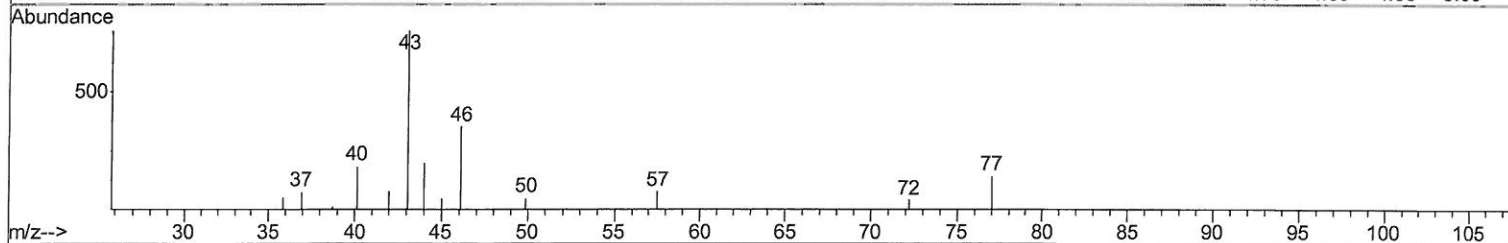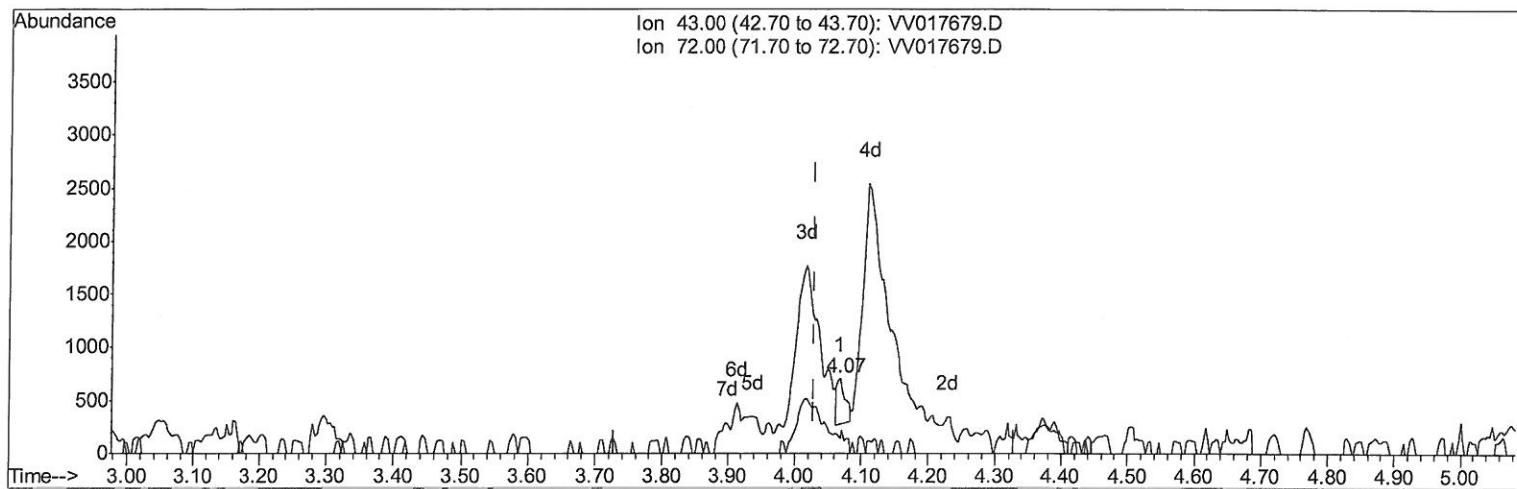

TIC: VV017679.D

(21) 2-Butanone (T)

4.068min (+0.038) 0.15ug/L

response 364

Ion	Exp%	Act%
43.00	100	100
72.00	25.90	23.08
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017679.D
 Acq On : 27 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3459-03MSD
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 GAY43MSD

Manual Integrations
APPROVED

MMDadoda
 7/29/2020 11:40:46 AM

Quant Time: Jul 28 04:56:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

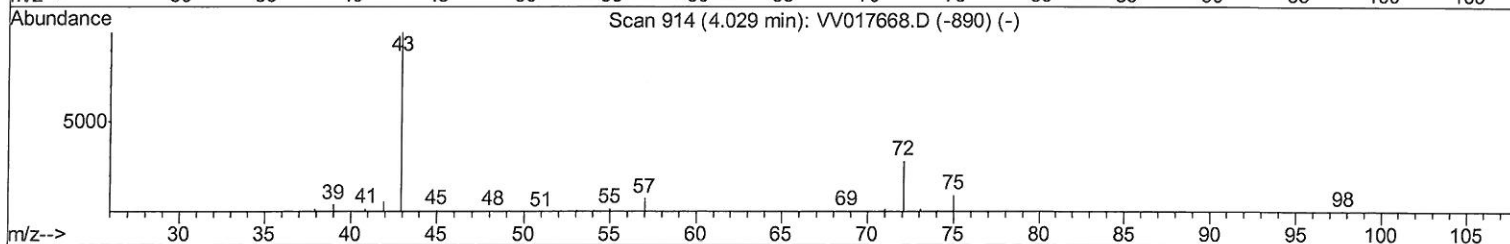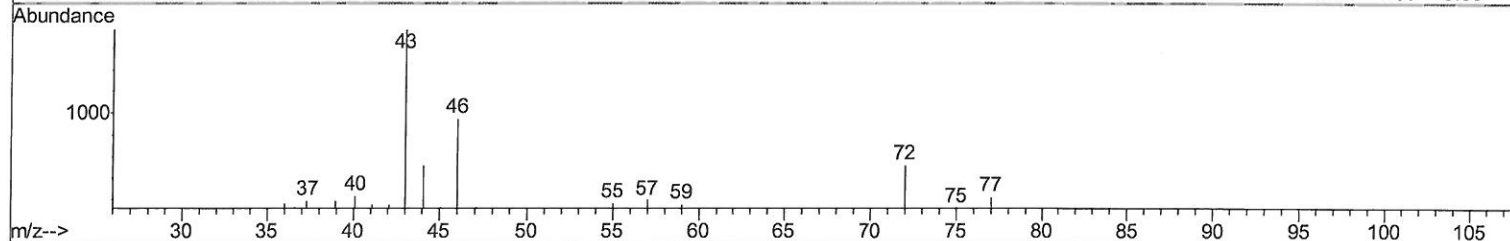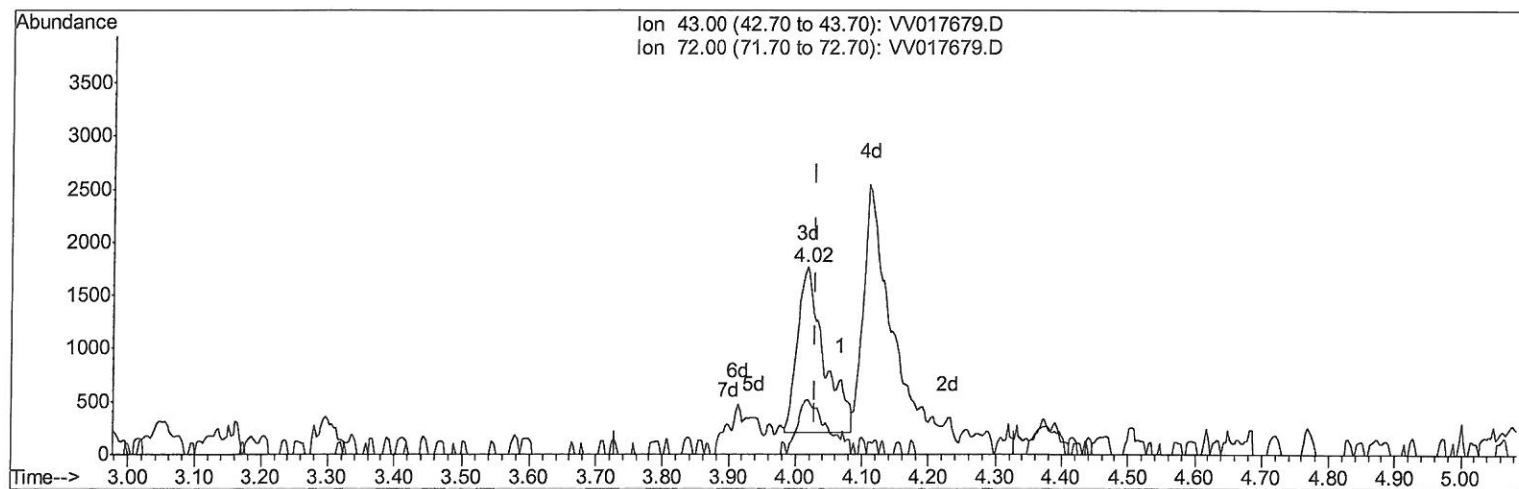

TIC: VV017679.D

(21) 2-Butanone (T)

4.016min (-0.013) 1.80ug/L m

response 4299

Ion	Exp%	Act%
43.00	100	100
72.00	25.90	1.95#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 7 MD
 7/31/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017679.D
 Acq On : 27 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3459-03MSD
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY43MSD

Manual Integrations
 APPROVED

MMDadoda
 7/29/2020 11:40:46 AM

Quant Time: Jul 28 06:19:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	158082	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	155219	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	76478	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	29634	3.93	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	78.60%	
7) Chloroethane-d5	1.58	69	24790	4.29	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.80%	
11) 1,1-Dichloroethene-d2	2.13	63	68354	4.04	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	80.80%	
20) 2-Butanone-d5	3.92	46	71899	39.82	ug/L	-0.04
Spiked Amount 50.000	Range 40	- 130	Recovery	=	79.64%	
24) Chloroform-d	4.37	84	80991	4.43	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	88.60%	
26) 1,2-Dichloroethane-d4	5.06	65	43491	4.62	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	92.40%	
32) Benzene-d6	5.07	84	141892	4.15	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	83.00%	
36) 1,2-Dichloropropane-d6	6.09	67	38188	4.01	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	80.20%	
41) Toluene-d8	7.34	98	129261	3.94	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	78.80%	
45) trans-1,3-Dichloropropene-	7.65	79	17406	4.04	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	80.80%	
48) 2-Hexanone-d5	8.11	63	48828	36.55	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	73.10%	
59) 1,1,2,2-Tetrachloroethane-	10.24	84	27349	4.13	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	82.60%	
65) 1,2-Dichlorobenzene-d4	11.65	152	55102	4.76	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	95.20%	
Target Compounds						
12) 1,1-Dichloroethene	2.13	96	33869	3.979	ug/L	89
13) Acetone	2.19	43	21116	14.937	ug/L #	53
21) 2-Butanone	4.02	43	4299m	1.801	ug/L	
33) Benzene	5.13	78	183128	4.168	ug/L	100
34) Trichloroethene	5.94	95	52723	4.296	ug/L	94
42) Toluene	7.41	91	210440	4.391	ug/L	98
53) Chlorobenzene	8.90	112	150533	4.711	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed