


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017686.D
Acq On : 27 Jul 2020 18:42
Operator : SY/MD
Sample : L3459-08
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY48

Manual Integrations
APPROVED

MMDadoda
7/29/2020 11:41:00 AM

Quant Time: Jul 28 07:07:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

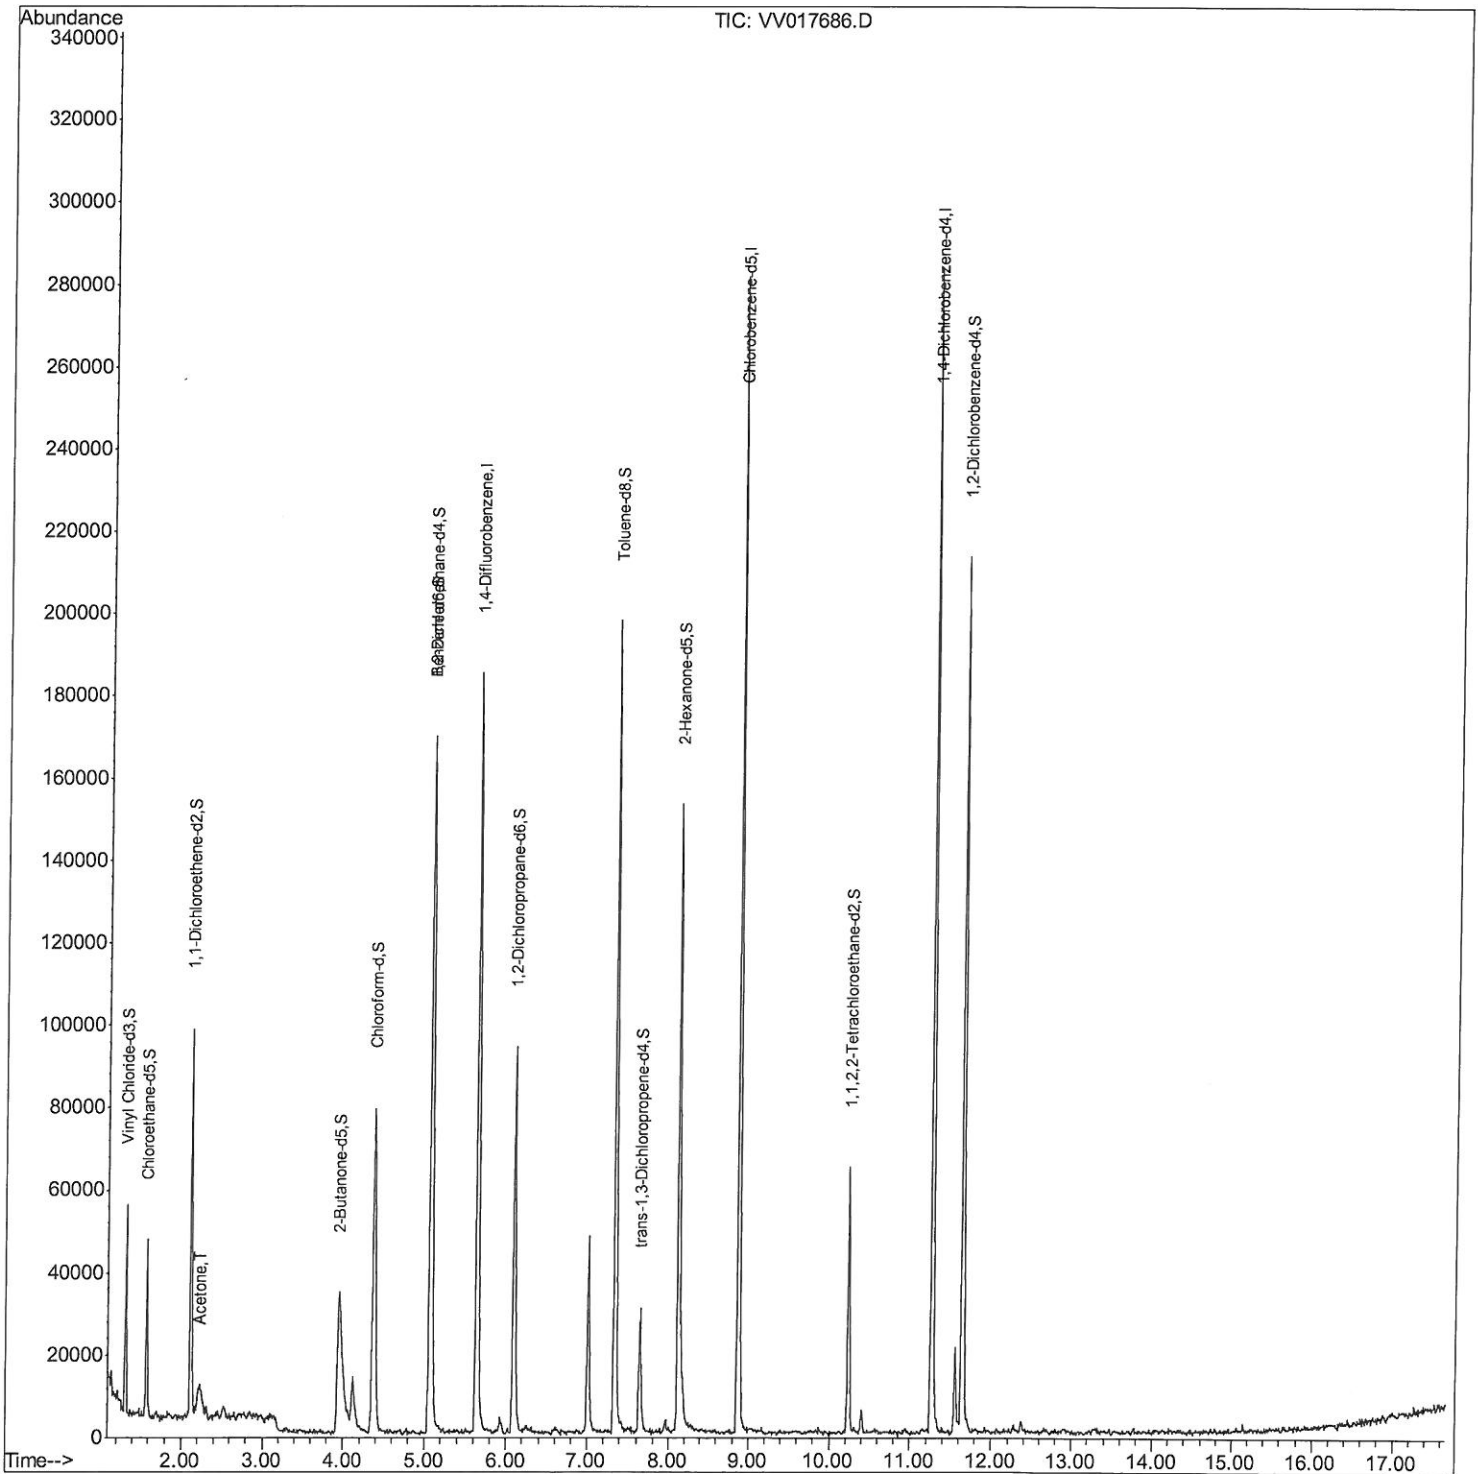

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017686.D
 Acq On : 27 Jul 2020 18:42
 Operator : SY/MD
 Sample : L3459-08
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 GAY48

Manual Integrations
APPROVED

MMDadoda
 7/29/2020 11:41:00 AM

Quant Time: Jul 28 04:58:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

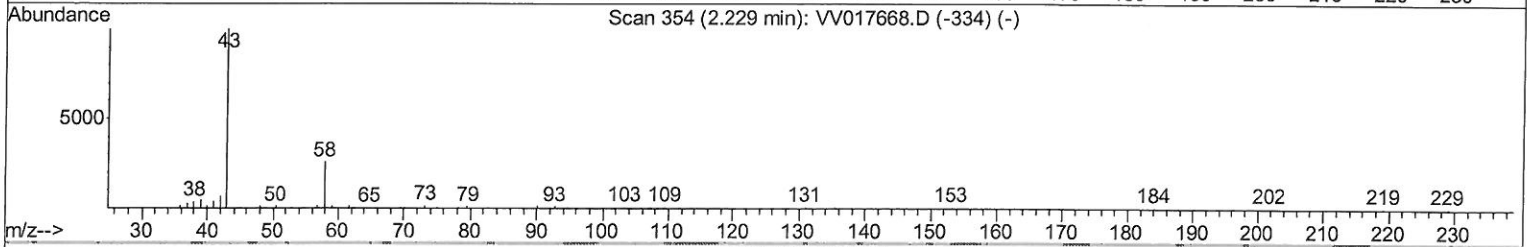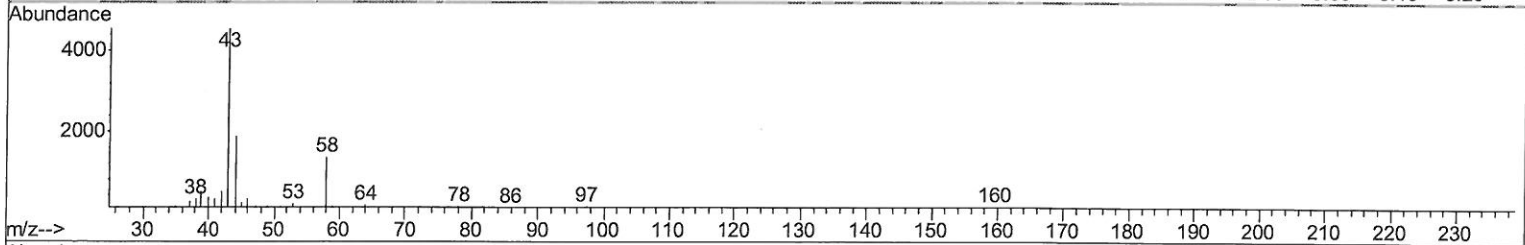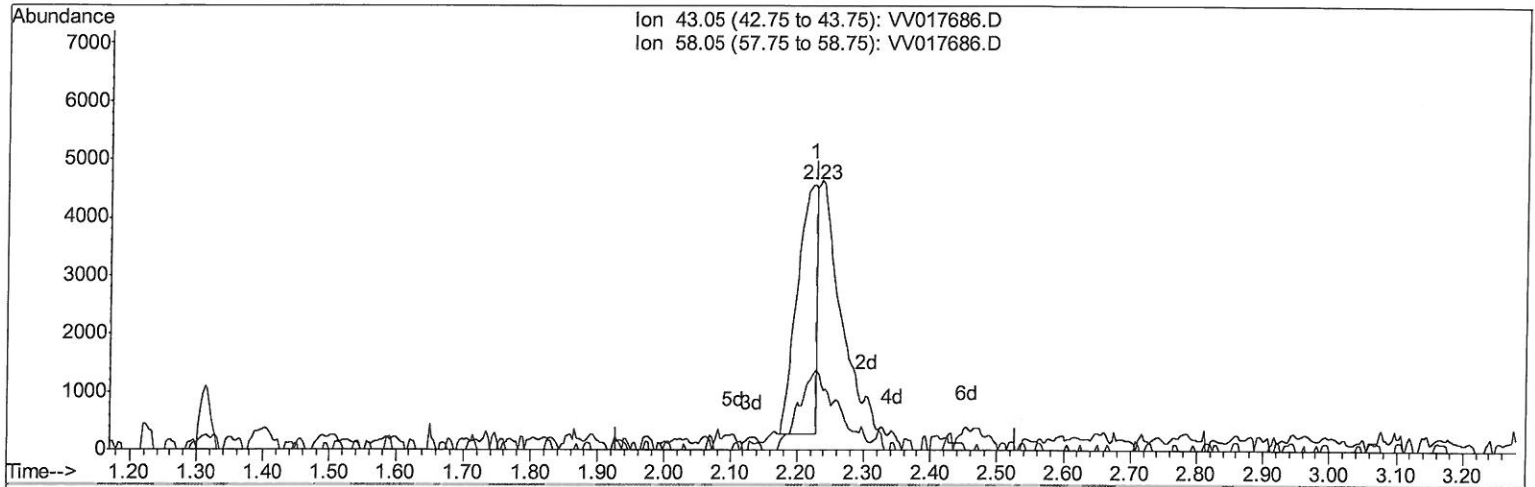

TIC: VV017686.D

(13) Acetone (T)

2.225min (-0.003) 6.59ug/L

response 8986

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	43.69#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017686.D
Acq On : 27 Jul 2020 18:42
Operator : SY/MD
Sample : L3459-08
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY48

Manual Integrations
APPROVED

MMDadoda
7/29/2020 11:41:00 AM

Quant Time: Jul 28 04:58:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

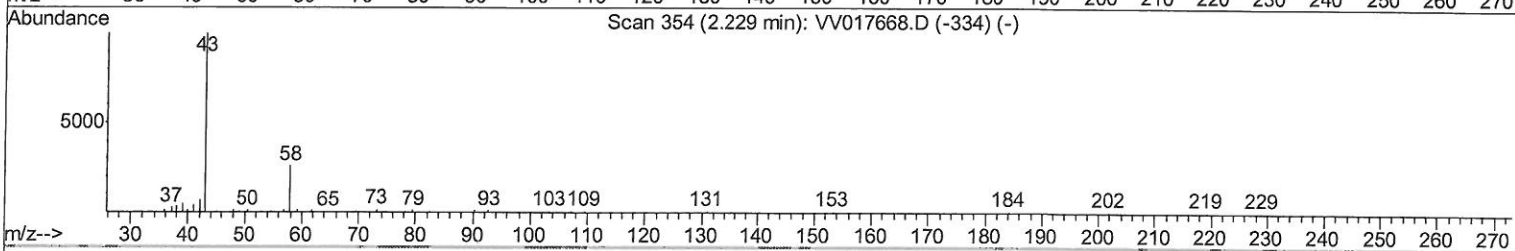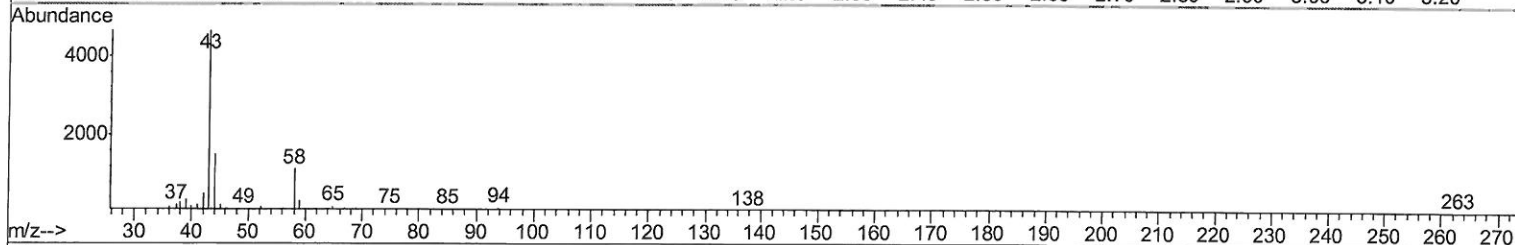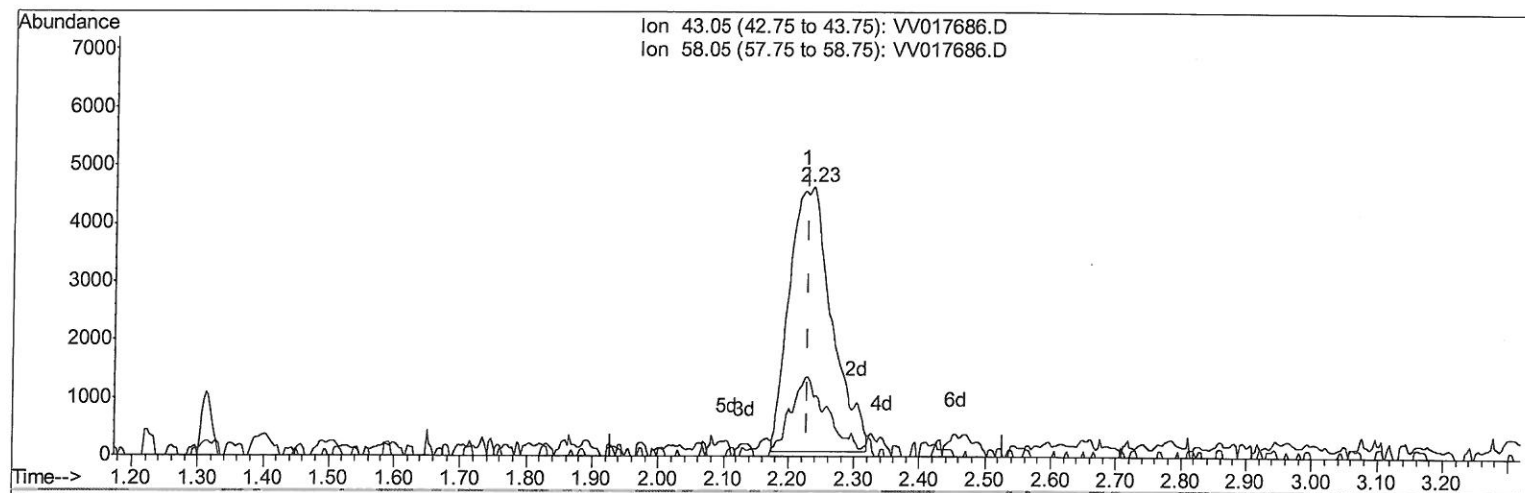

TIC: VV017686.D

(13) Acetone (T)

2.235min (+0.006) 15.03ug/L m

response 20481

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	19.17#
0.00	0.00	0.00
0.00	0.00	0.00

MD
7/31/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017686.D
 Acq On : 27 Jul 2020 18:42
 Operator : SY/MD
 Sample : L3459-08
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 GAY48

Manual Integrations
 APPROVED

MMDadoda
 7/29/2020 11:41:00 AM

Quant Time: Jul 28 07:07:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	152433	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	151031	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	74647	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	28592	3.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.60%
7) Chloroethane-d5	1.58	69	24897	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.12	63	48341	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.95	46	77497	44.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.02%
24) Chloroform-d	4.37	84	79244	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	5.06	65	43970	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.07	84	138135	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.00%
36) 1,2-Dichloropropane-d6	6.09	67	38496	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.20%
41) Toluene-d8	7.34	98	126898	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.40%
45) trans-1,3-Dichloropropene-	7.65	79	17599	4.20	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.00%
48) 2-Hexanone-d5	8.11	63	47741	36.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.46%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	26617	4.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	53800	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.23	43	20481m	15.025	ug/L	2.00

(#) = qualifier out of range (m) = manual integration (+) = signals summed