

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017673.D
 Acq On : 27 Jul 2020 12:50
 Operator : SY/MD
 Sample : L3443-08
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Quant Time: Jul 28 05:36:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	144959	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	143310	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	68800	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35779	5.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.40%
7) Chloroethane-d5	1.58	69	29523	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.40%
11) 1,1-Dichloroethene-d2	2.12	63	60598	3.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.20%
20) 2-Butanone-d5	3.93	46	72371	43.71	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.42%
24) Chloroform-d	4.38	84	91535	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.20%
26) 1,2-Dichloroethane-d4	5.06	65	49031	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.40%
32) Benzene-d6	5.07	84	165539	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
36) 1,2-Dichloropropane-d6	6.09	67	45366	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.34	98	146986	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
45) trans-1,3-Dichloropropene-	7.65	79	18125	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
48) 2-Hexanone-d5	8.11	63	50609	41.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.08%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	28947	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	60397	5.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	6241	4.815 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017673.D
Acq On : 27 Jul 2020 12:50
Operator : SY/MD
Sample : L3443-08
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1

Quant Time: Jul 28 05:36:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

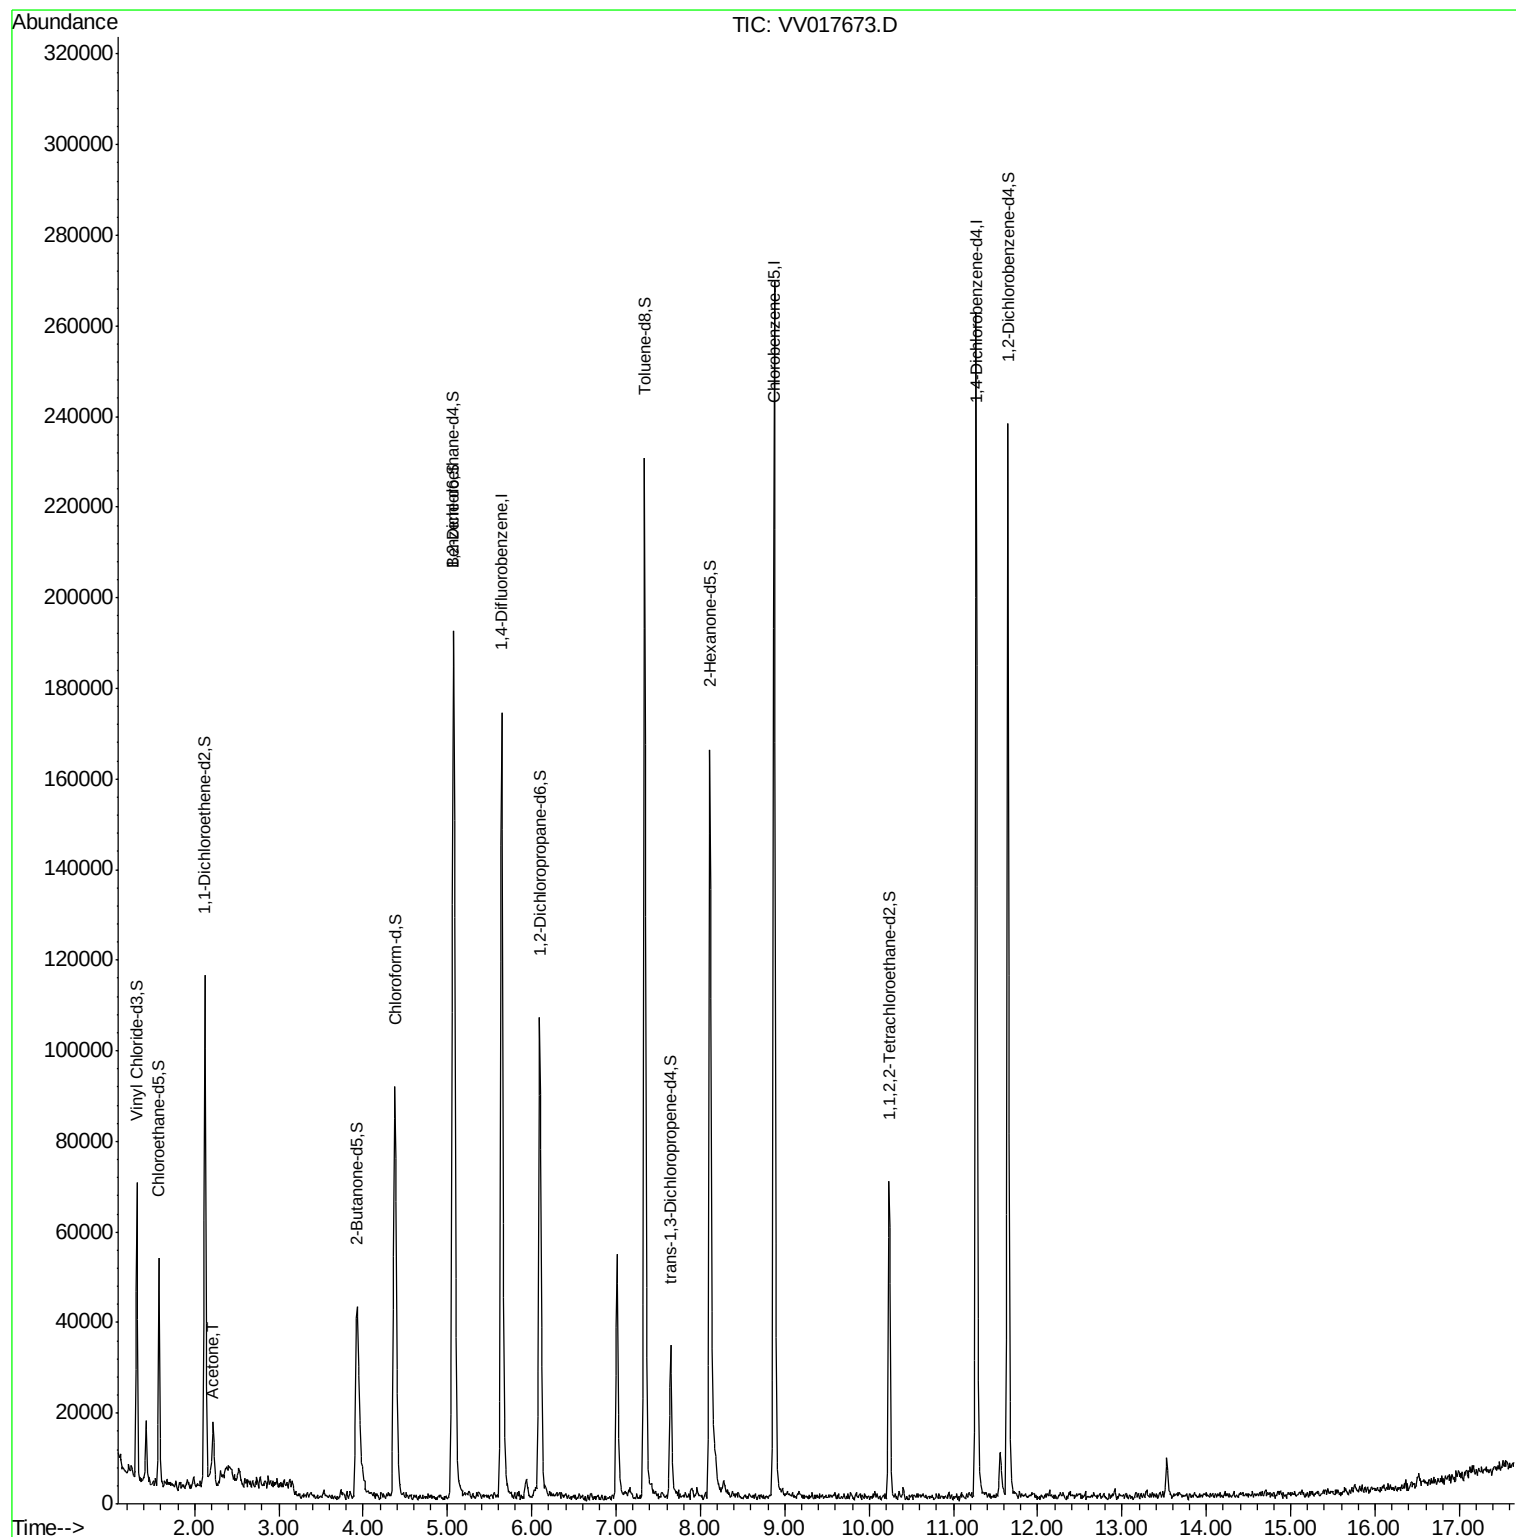

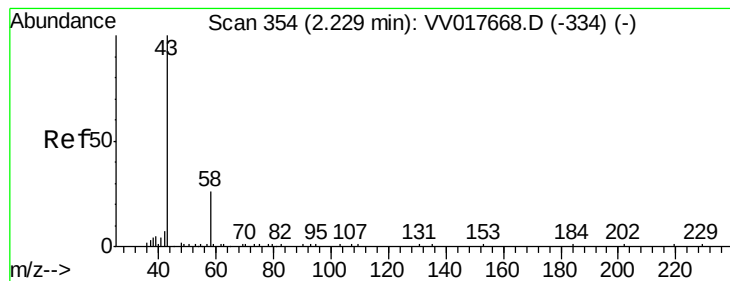

#13
 Acetone
 Concen: 4.815 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.04 min
 Lab File: VV017673.D
 Acq: 27 Jul 2020 12:50

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Tot Ion: 43 Resp: 6241
 Ion Ratio Lower Upper
 43 100
 58 17.2 0.0 18.6

