

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017685.D
 Acq On : 27 Jul 2020 18:18
 Operator : SY/MD
 Sample : L3459-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY47

Quant Time: Jul 28 06:48:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	146734	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	146015	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	71344	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	28924	4.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.60%
7) Chloroethane-d5	1.58	69	25623	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.60%
11) 1,1-Dichloroethene-d2	2.12	63	52335	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.94	46	72841	43.46	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.92%
24) Chloroform-d	4.38	84	80743	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.06	65	45241	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.07	84	141152	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.10	67	39475	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.20%
41) Toluene-d8	7.34	98	128652	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.40%
45) trans-1,3-Dichloropropene-	7.64	79	17061	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
48) 2-Hexanone-d5	8.11	63	47317	37.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.32%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	26786	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	54296	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%


Target Compounds					Ovalue
13) Acetone	2.22	43	18462	14.070 ug/L	# 52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017685.D
Acq On : 27 Jul 2020 18:18
Operator : SY/MD
Sample : L3459-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY47

Quant Time: Jul 28 06:48:16 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

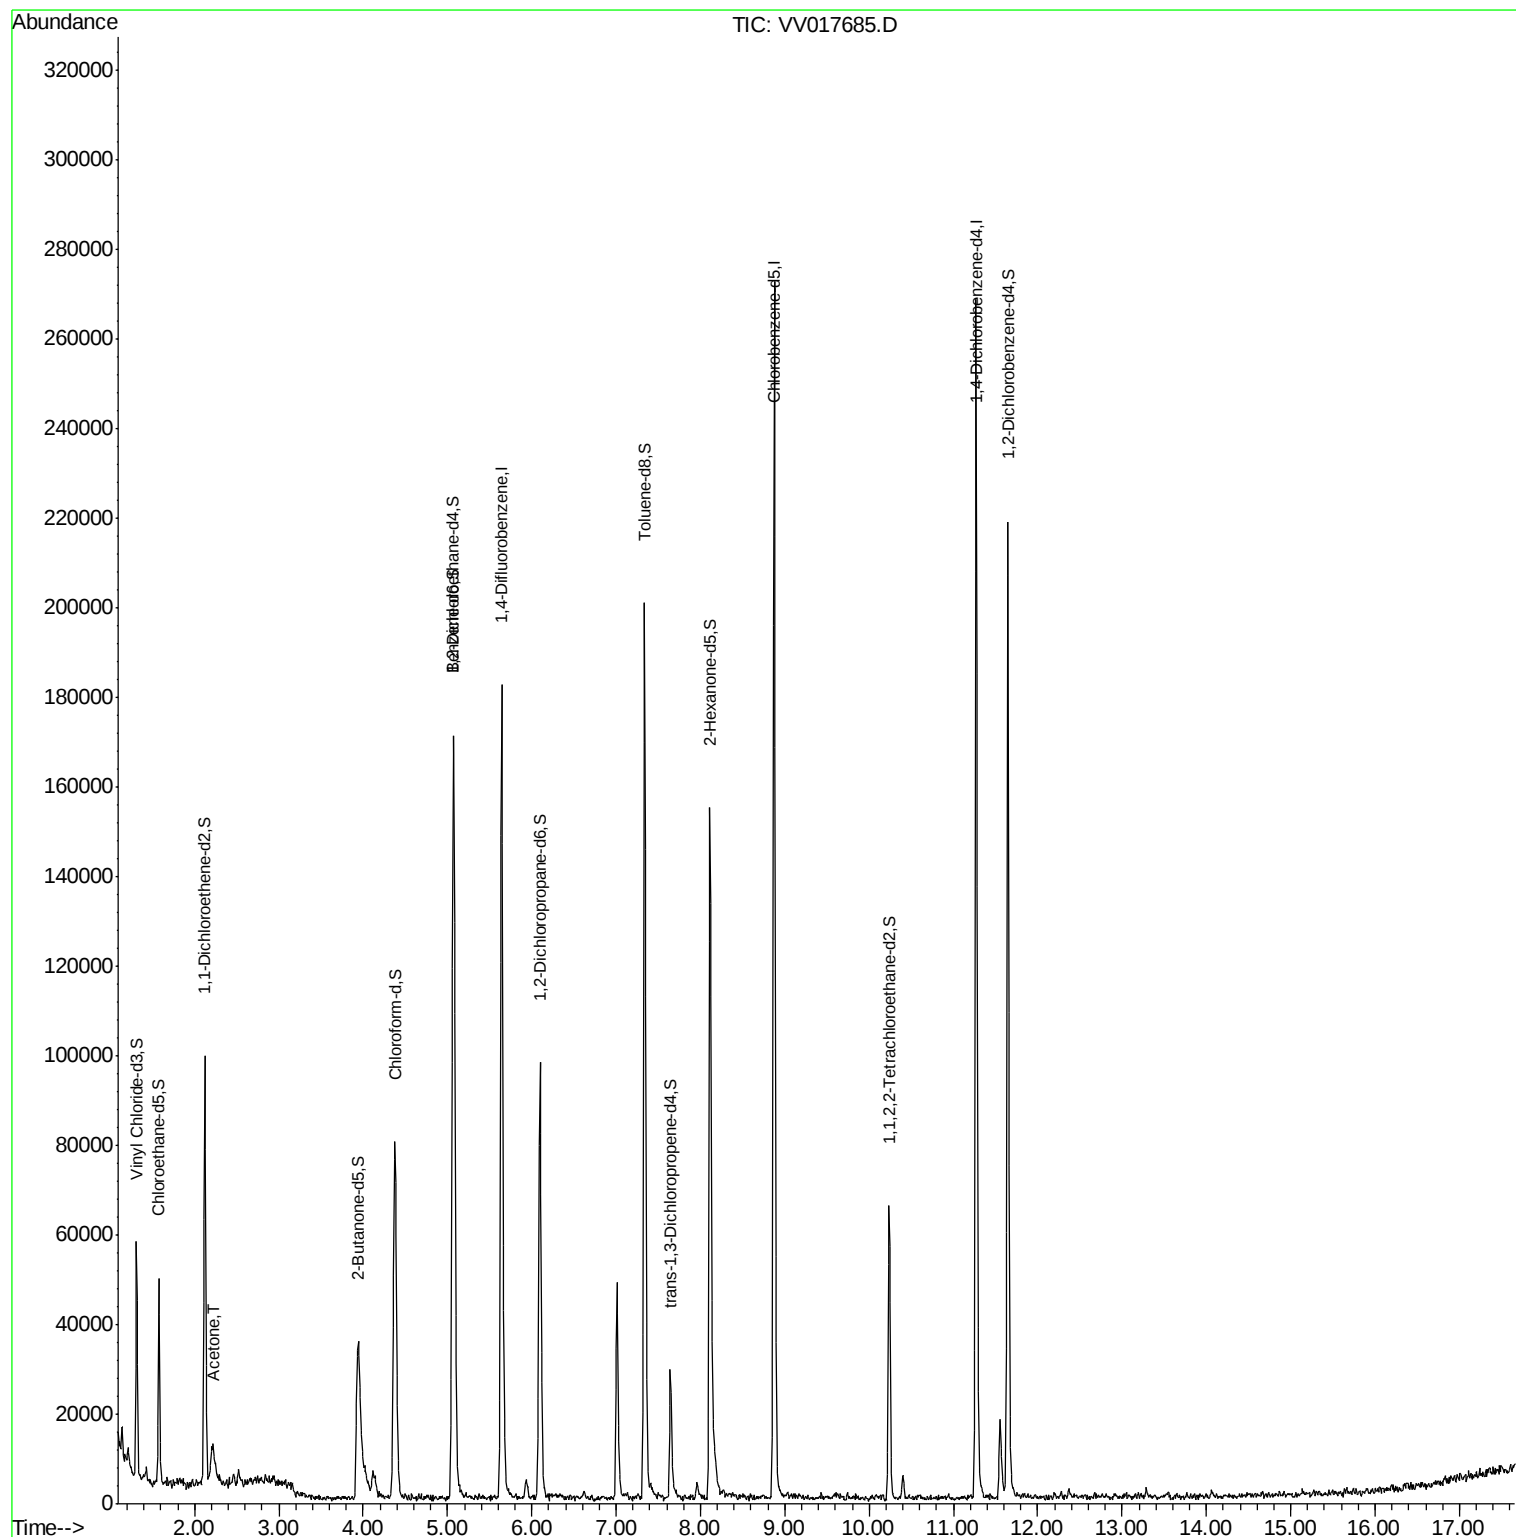

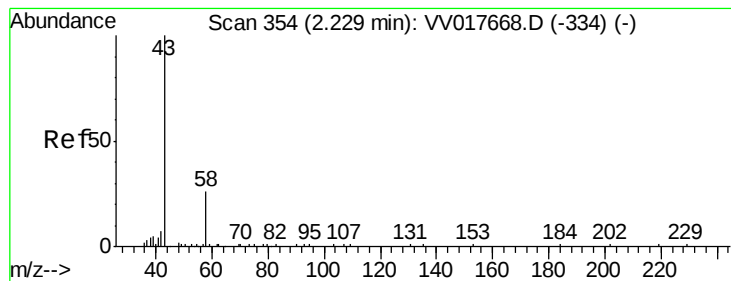

#13
 Acetone
 Concen: 14.070 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. -0.01 min
 Lab File: VV017685.D
 Acq: 27 Jul 2020 18:18

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY47

Tot Ion: 43 Resp: 18462
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 18.6#

