

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017688.D
 Acq On : 27 Jul 2020 19:30
 Operator : SY/MD
 Sample : L3459-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAY50

Quant Time: Jul 28 07:18:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 28 04:52:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	147932	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	144240	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	71581	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	27791	3.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.60%
7) Chloroethane-d5	1.58	69	24966	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.12	63	51277	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	3.95	46	75140	44.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.94%
24) Chloroform-d	4.37	84	82350	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.06	65	44355	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.07	84	139412	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.10	67	39944	4.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.40%
41) Toluene-d8	7.34	98	126233	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
45) trans-1,3-Dichloropropene-	7.65	79	16574	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
48) 2-Hexanone-d5	8.12	63	45408	36.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.16%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	26664	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	54988	5.08	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.60%


Target Compounds					Ovalue
13) Acetone	2.24	43	18289	13.825 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017688.D
Acq On : 27 Jul 2020 19:30
Operator : SY/MD
Sample : L3459-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAY50

Quant Time: Jul 28 07:18:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 28 04:52:47 2020
Response via : Initial Calibration

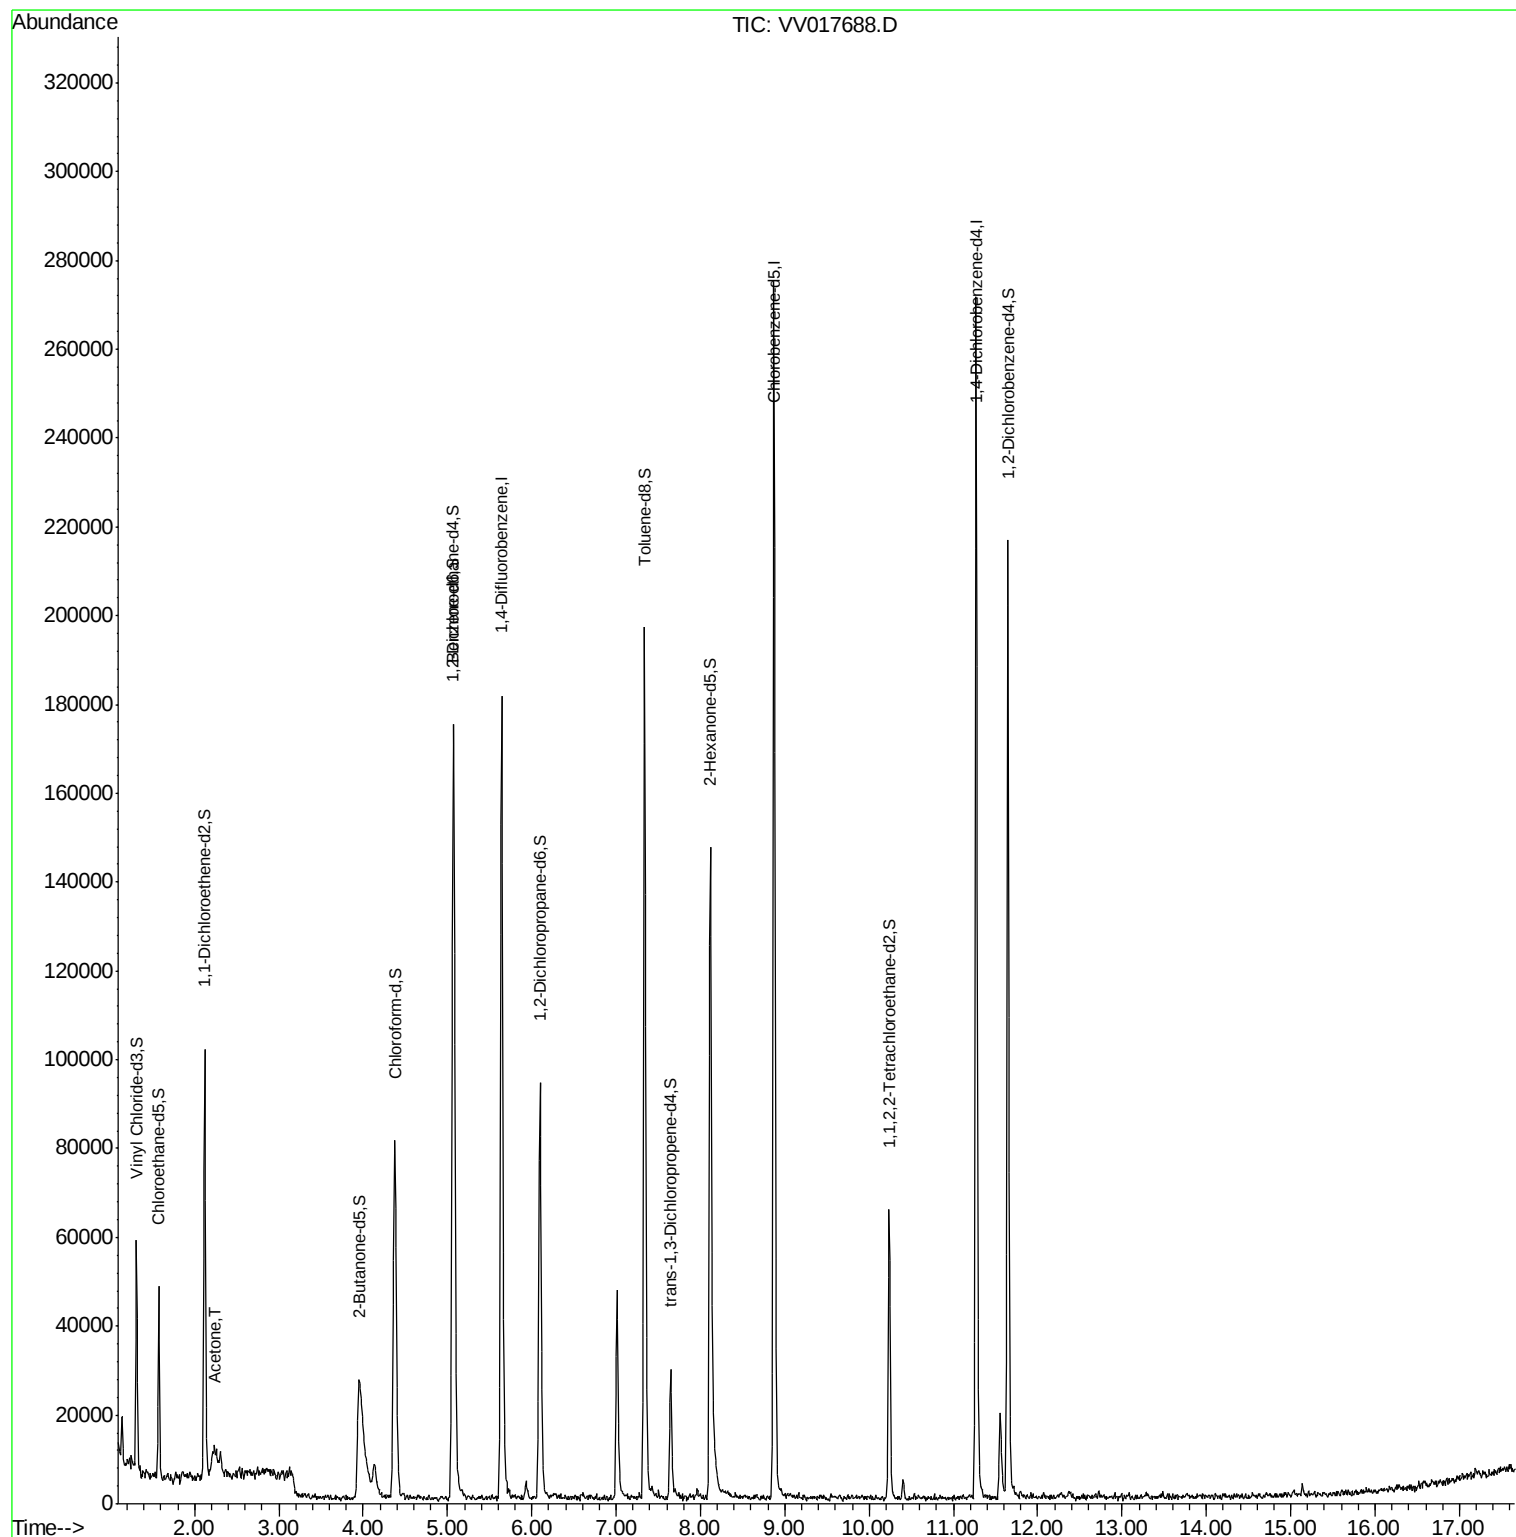

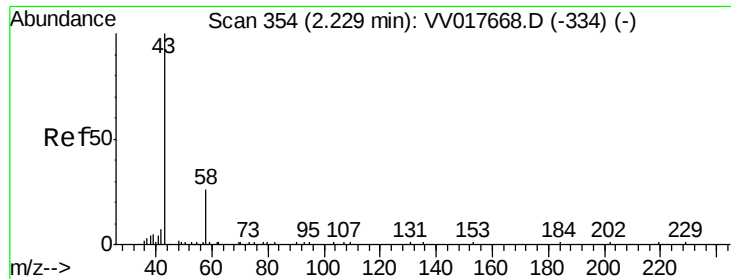

#13

Acetone

Concen: 13.825 ug/L

RT: 2.24 min Scan# 357

Delta R.T. 0.01 min

Lab File: VV017688.D

Acq: 27 Jul 2020 19:30

Instrument :
MSVOA_V
ClientSampleId :
GAY50

Tot Ion: 43 Resp: 18289

Ion Ratio Lower Upper

43 100

58 7.3 0.0 18.6

