

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072720\
 Data File : VV017670.D
 Acq On : 27 Jul 2020 11:33
 Operator : SY/MD
 Sample : L3443-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	60	69	77	rBV	54562	56322	12.94%	1.535%
2	1.425	99	104	110	rVB	8819	8780	2.02%	0.239%
3	1.576	143	151	162	rBV	47535	53188	12.22%	1.450%
4	2.122	310	321	332	rBV	96129	141565	32.52%	3.858%
5	2.222	345	352	360	rBV6	7929	11212	2.58%	0.306%
6	3.949	877	889	926	rBV2	26554	137612	31.61%	3.751%
7	4.373	1005	1021	1040	rBV3	78663	194702	44.72%	5.306%
8	5.068	1222	1237	1259	rBV4	172944	421446	96.80%	11.486%
9	5.640	1402	1415	1433	rBV	173875	350915	80.60%	9.564%
10	5.929	1498	1505	1518	rVB	3809	7476	1.72%	0.204%
11	6.093	1543	1556	1573	rVB2	93115	189713	43.58%	5.170%
12	7.010	1829	1841	1857	rBV	46092	87432	20.08%	2.383%
13	7.338	1930	1943	1959	rBV	195426	338316	77.71%	9.221%
14	7.646	2027	2039	2053	rBV2	28026	54181	12.45%	1.477%
15	7.891	2110	2115	2124	rBV10	3253	5127	1.18%	0.140%
16	8.116	2169	2185	2213	rBV	156529	331468	76.14%	9.034%
17	8.871	2407	2420	2442	rBV	261743	435362	100.00%	11.865%
18	10.238	2835	2845	2856	rBV	67362	104857	24.09%	2.858%
19	10.399	2886	2895	2904	rBV3	6567	10811	2.48%	0.295%
20	11.270	3155	3166	3184	rBV	261397	405377	93.11%	11.048%
21	11.556	3248	3255	3257	rBV8	5722	6537	1.50%	0.178%
22	11.646	3271	3283	3300	rBV	195129	316749	72.76%	8.633%


Sum of corrected areas: 3669148

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072720\
Data File : VV017670.D
Acq On : 27 Jul 2020 11:33
Operator : SY/MD
Sample : L3443-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

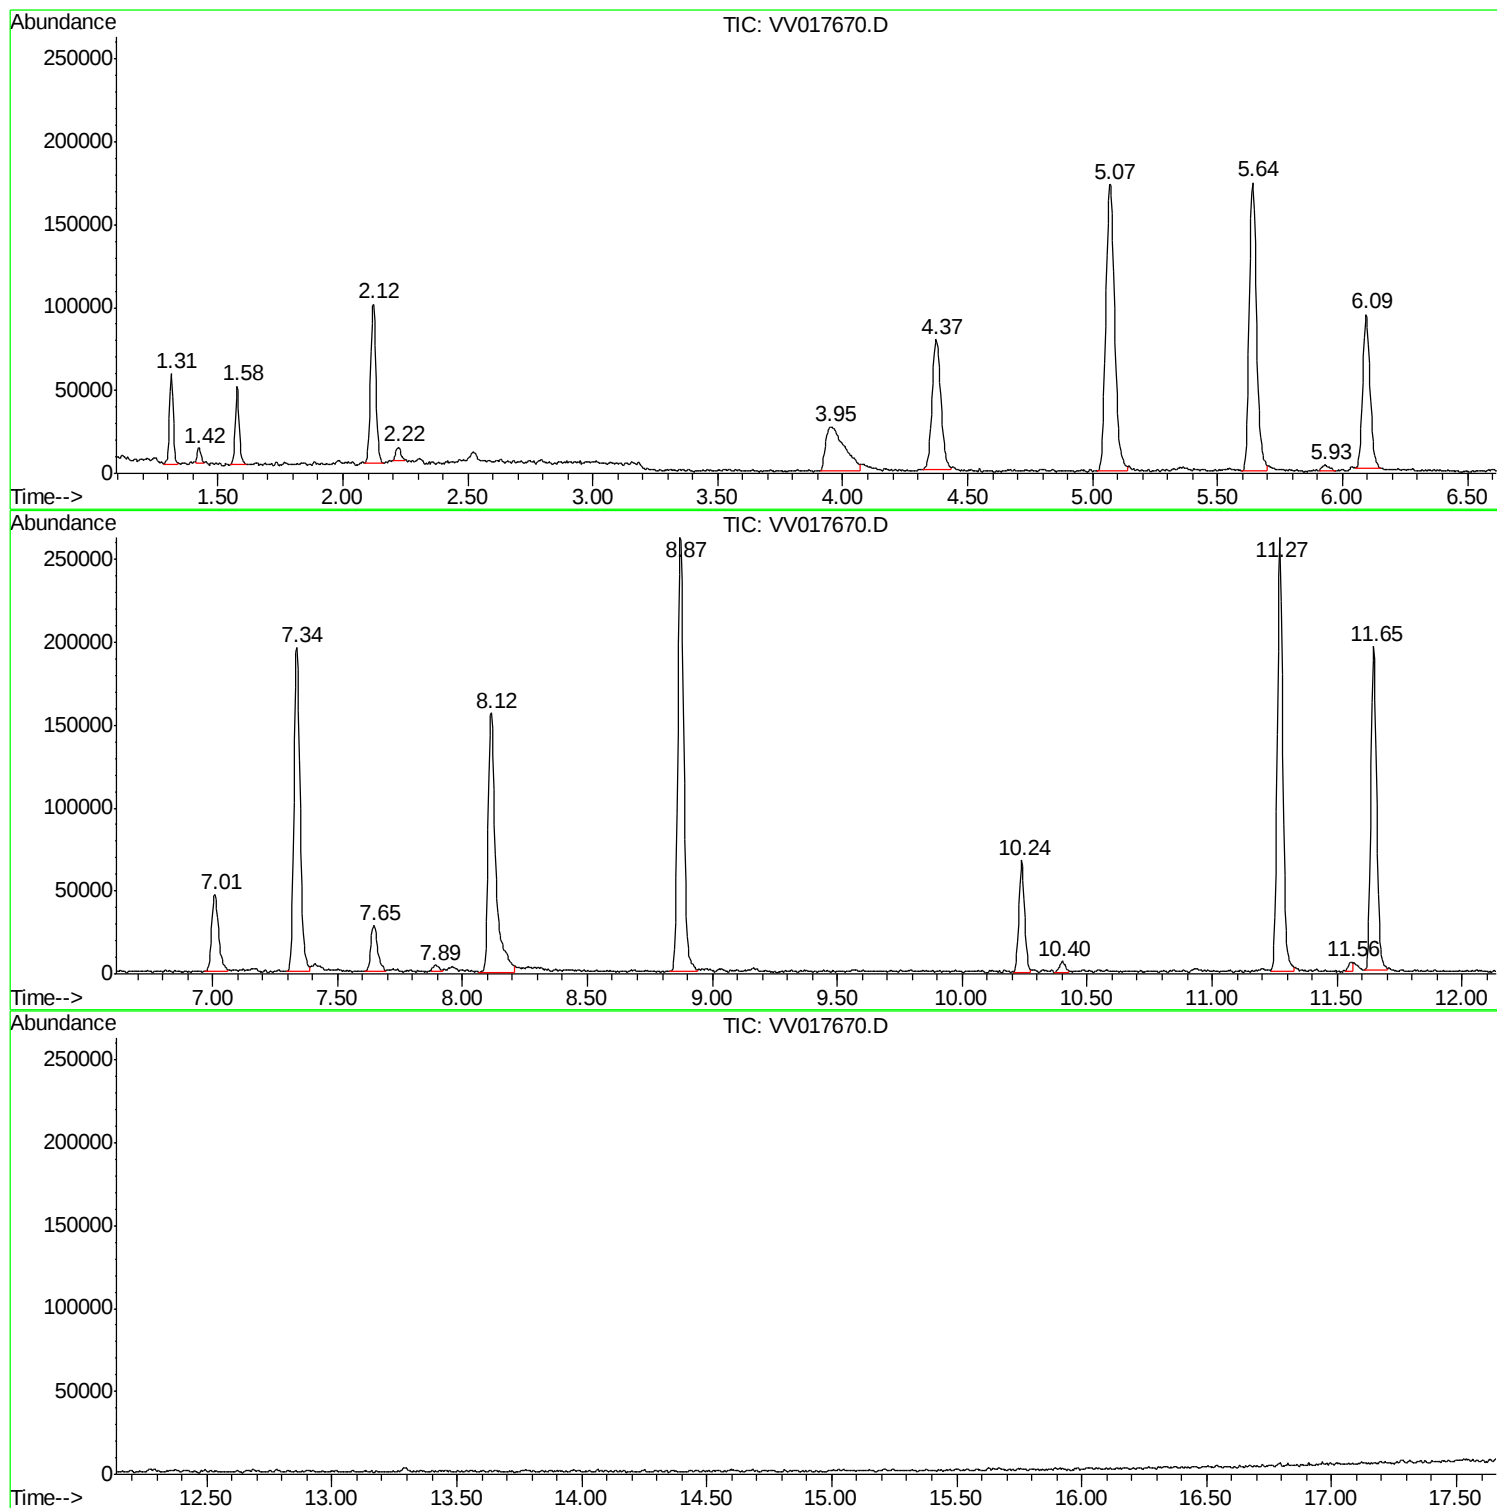

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072720\
Data File : VV017670.D
Acq On : 27 Jul 2020 11:33
Operator : SY/MD
Sample : L3443-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072720\
Data File : VV017670.D
Acq On : 27 Jul 2020 11:33
Operator : SY/MD
Sample : L3443-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc