


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072720\
 Data File : VV017667.D
 Acq On : 27 Jul 2020 09:29
 Operator : SY/MD
 Sample : BFB53
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB53

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 29 18:07:18 2020

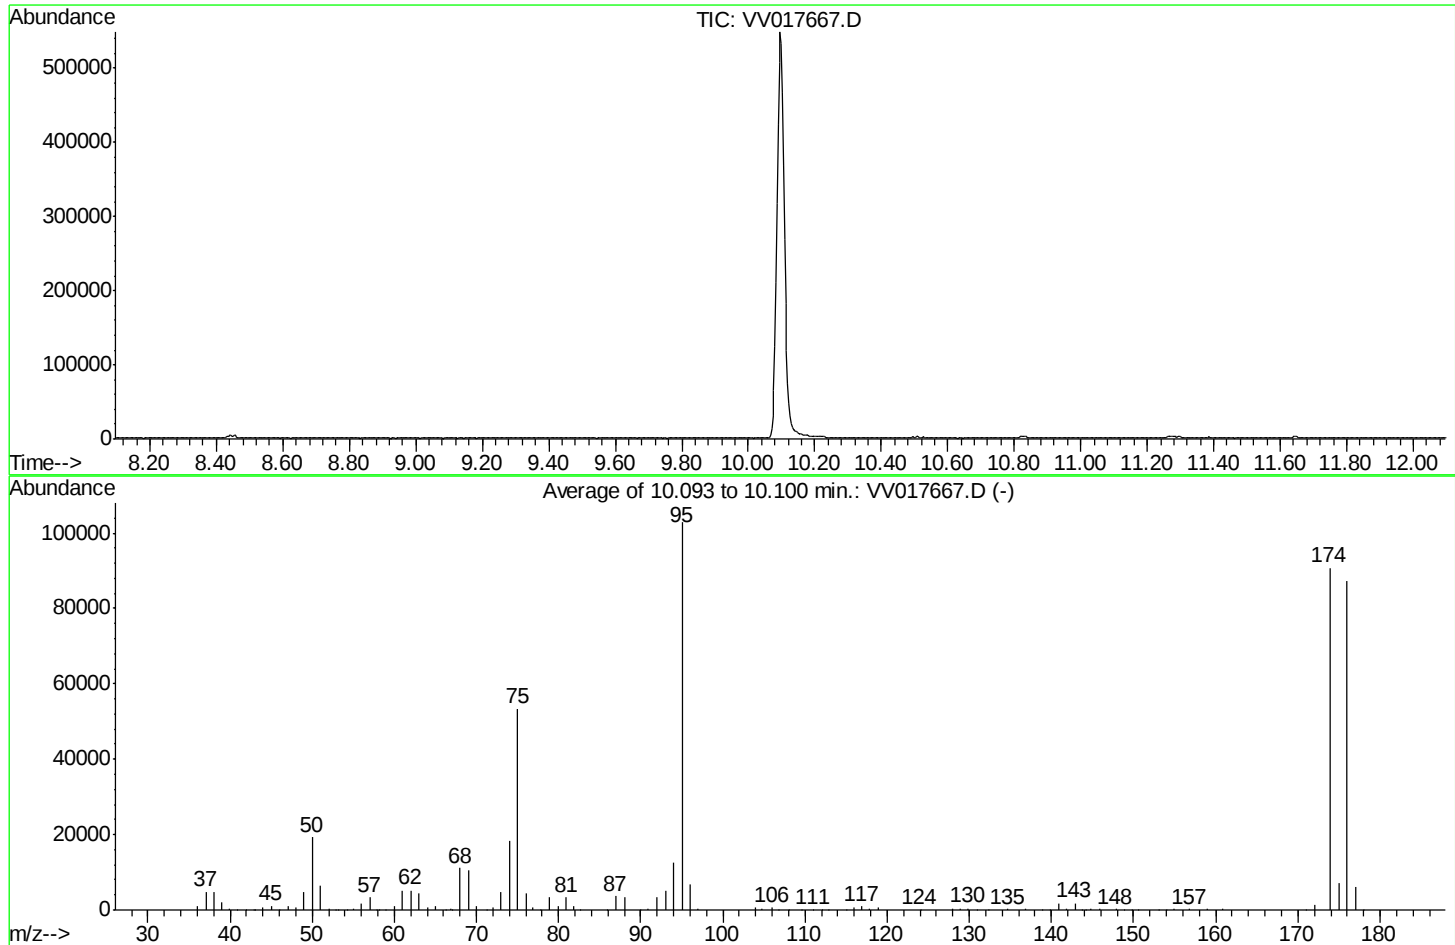

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	19349	PASS
75	95	30	80	51.9	53338	PASS
95	95	100	100	100.0	102845	PASS
96	95	5	9	6.6	6792	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.2	90725	PASS
175	174	5	9	8.0	7279	PASS
176	174	95	101	96.1	87202	PASS
177	176	5	9	6.9	6043	PASS

Scan 2788 (10.055 min): VV017667.D
BFB53

m/z	Abundance
35.30	133.0
37.10	102.0
39.10	129.0
40.00	175.0
41.60	111.0
43.90	211.0
55.80	119.0
60.00	131.0
69.50	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
36.00	1217.0
37.00	4802.0
38.00	4915.0
39.00	2118.0
39.90	418.0
41.50	173.0
43.10	114.0
44.00	688.0
45.00	1045.0
46.10	130.0
47.10	982.0
48.00	706.0
49.00	4627.0
50.00	19248.0
51.00	6248.0
52.00	304.0
52.90	168.0
53.20	183.0
54.20	126.0
55.00	336.0
56.00	1685.0
57.00	3234.0
57.90	127.0
60.00	1141.0
61.00	5097.0
62.00	5274.0
63.00	4327.0
64.10	683.0
65.10	1070.0
66.30	110.0
67.10	281.0
68.00	10885.0
69.00	10626.0
70.00	871.0
71.20	147.0
72.00	587.0
73.00	4782.0
74.00	17912.0
75.00	53944.0
76.00	4230.0
76.90	712.0
78.90	3361.0
80.00	1145.0
80.90	3483.0
81.90	891.0
82.60	113.0
85.80	152.0
86.90	3783.0
88.00	3493.0
90.90	487.0
92.00	3558.0
93.00	5315.0
94.00	12904.0
95.00	102080.0
96.00	6648.0
96.90	209.0
103.90	567.0
104.70	220.0
106.00	519.0
106.80	160.0
109.60	102.0
111.00	148.0
112.00	138.0
112.90	154.0
116.00	492.0
116.90	991.0
117.80	392.0
118.90	765.0
128.00	427.0
128.80	164.0
129.80	530.0
131.00	219.0
132.30	110.0
134.70	388.0
136.80	224.0
138.90	105.0
139.70	108.0
140.80	1595.0
141.80	185.0
142.90	1910.0
144.20	108.0
144.90	505.0
145.90	295.0
147.90	331.0
149.80	145.0
154.80	374.0
156.80	237.0
159.00	275.0
160.90	245.0
170.90	288.0
172.00	1403.0
173.90	92360.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

175.00	7354.0
175.90	88480.0
177.00	6073.0
178.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
36.00	1218.0
37.00	5078.0
38.00	4987.0
39.00	2257.0
39.90	422.0
41.50	116.0
42.80	136.0
44.00	760.0
45.00	1139.0
45.90	168.0
47.10	1008.0
47.80	639.0
48.00	642.0
49.00	4926.0
50.00	19992.0
51.00	6720.0
52.00	313.0
53.20	157.0
54.20	137.0
55.00	341.0
56.00	1827.0
57.00	3463.0
60.00	1321.0
61.00	5238.0
62.00	5351.0
63.00	4477.0
64.00	752.0
65.00	1120.0
66.90	322.0
68.00	11507.0
69.00	10626.0
70.00	935.0
71.30	144.0
72.00	530.0
73.00	4922.0
74.00	18896.0
75.00	55136.0
76.00	4365.0
76.90	614.0
77.70	194.0
78.90	3440.0
79.90	1048.0
80.90	3496.0
81.90	941.0
82.60	146.0
85.90	138.0
86.90	3794.0
88.00	3760.0
90.00	108.0
90.80	446.0
92.00	3730.0
93.00	5266.0
94.00	12770.0
95.00	106352.0
96.00	7035.0
97.00	205.0
103.90	585.0
104.70	245.0
106.00	596.0
106.80	126.0
111.00	155.0
112.00	124.0
112.90	138.0
115.00	111.0
115.90	582.0
116.90	958.0
117.80	397.0
118.90	798.0
128.00	438.0
128.90	253.0
129.90	517.0
130.90	191.0
134.70	334.0
136.80	234.0
138.80	111.0
140.80	1706.0
141.90	218.0
142.90	1933.0
143.70	102.0
144.80	523.0
145.90	273.0
147.90	307.0
149.80	142.0
153.00	119.0
154.90	318.0
156.80	357.0
159.00	295.0
160.80	215.0
172.00	1462.0
173.90	93960.0
175.00	7515.0
175.90	90568.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

177.00
178.00

6335.0
186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.20	107.0
36.10	1017.0
37.10	4827.0
38.00	4441.0
39.00	2161.0
40.00	474.0
40.80	164.0
41.90	107.0
42.90	161.0
43.90	835.0
45.00	1145.0
46.00	182.0
47.00	942.0
47.90	525.0
49.00	4644.0
50.00	18808.0
51.00	6430.0
52.00	312.0
53.20	170.0
54.30	113.0
55.10	330.0
55.90	1655.0
57.00	3122.0
58.20	112.0
59.00	120.0
60.00	1301.0
61.00	4982.0
62.00	4871.0
63.00	4191.0
64.00	784.0
65.00	1099.0
66.90	339.0
68.00	10827.0
69.00	9895.0
70.00	892.0
72.00	471.0
73.00	4586.0
74.00	18232.0
75.00	50936.0
76.00	4182.0
76.90	529.0
77.80	244.0
78.90	3295.0
79.90	933.0
80.90	3069.0
81.90	820.0
82.70	126.0
87.00	3414.0
88.00	3459.0
90.90	420.0
92.00	3379.0
93.00	4609.0
94.00	11709.0
95.00	100104.0
96.00	6693.0
97.00	200.0
103.90	501.0
104.80	219.0
106.00	574.0
108.00	104.0
111.00	157.0
115.00	119.0
115.80	583.0
116.90	820.0
117.80	383.0
119.00	804.0
124.00	118.0
127.90	378.0
128.90	305.0
129.80	458.0
130.90	140.0
134.70	259.0
136.80	210.0
139.80	115.0
140.90	1465.0
141.90	249.0
142.90	1682.0
144.90	459.0
145.90	252.0
147.80	267.0
148.80	112.0
149.70	115.0
150.60	111.0
153.00	135.0
153.90	103.0
155.00	238.0
156.80	424.0
159.00	257.0
160.80	152.0
172.00	1386.0
173.90	85856.0
175.00	6970.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

175.90

177.00

177.90

82560.0

5723.0

150.0

Instrument :

MSVOA_V

ClientSampleId :

BFB53