
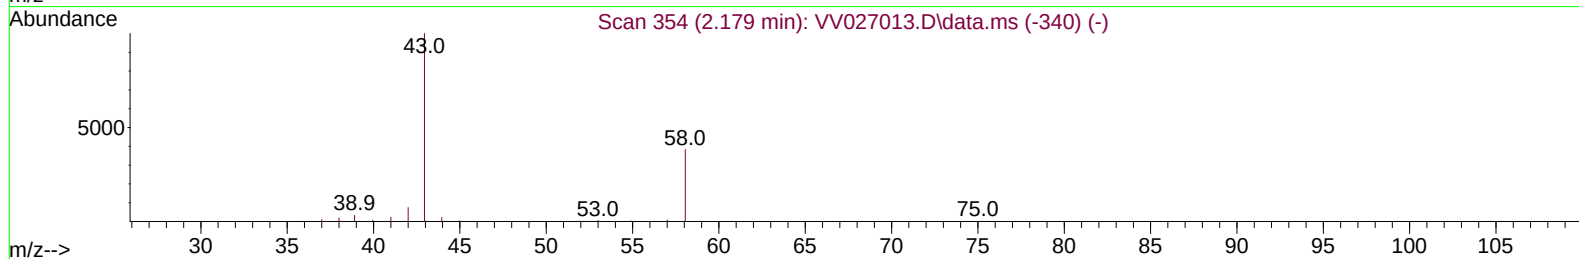
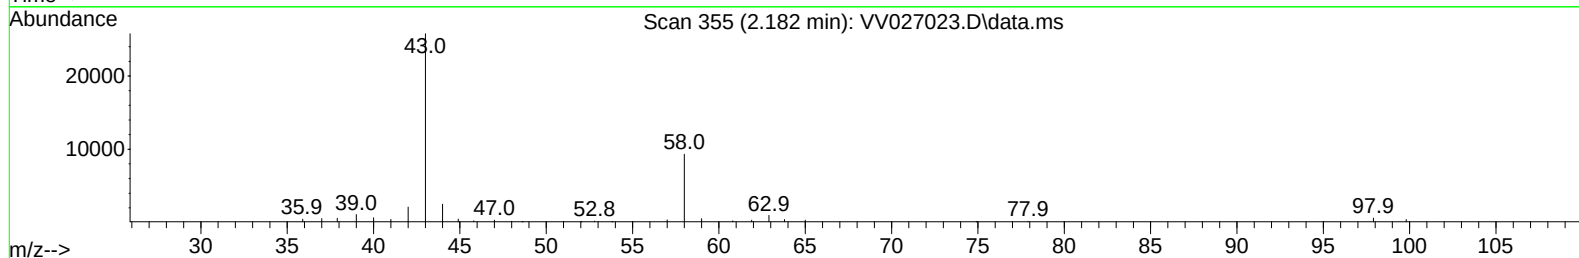


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jul 28 06:18:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 02:51:09 2022
Response via : Initial Calibration

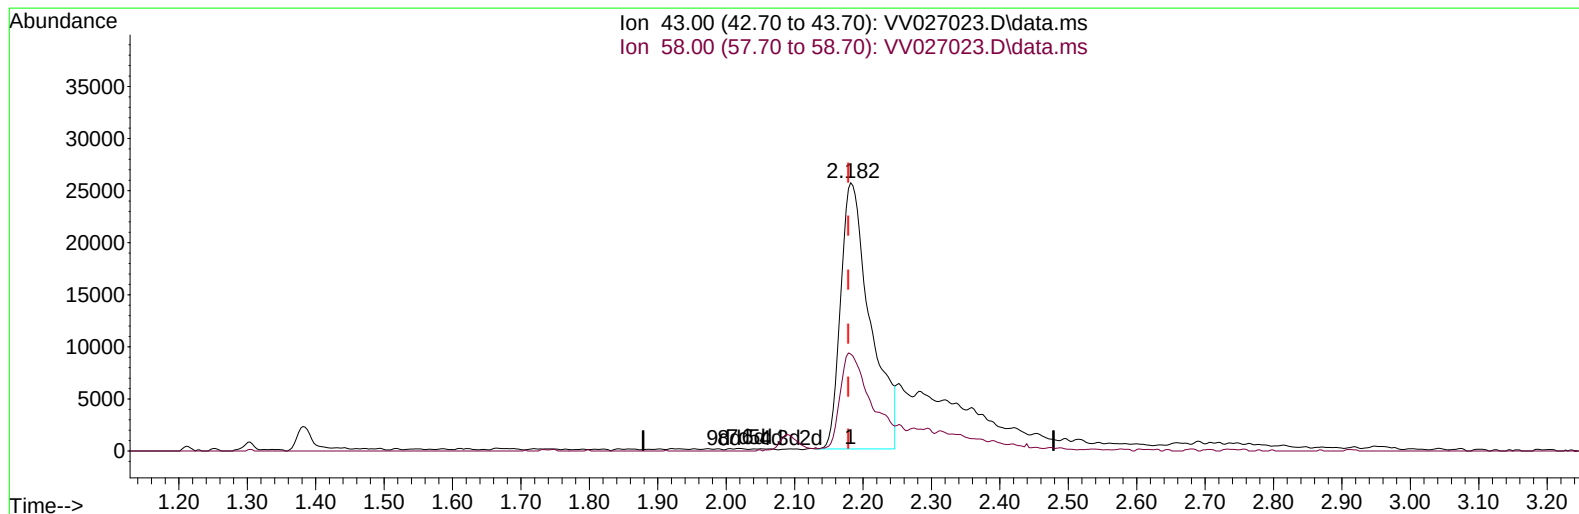

TIC: VV027023.D\data.ms

(13) Acetone (T)

2.182min (+ 0.003) 41.85 ug/L

response 77021

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	31.43
0.00	0.00	0.00
0.00	0.00	0.00