

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026995.D
 Acq On : 27 Jul 2022 13:07
 Operator : SY/MD
 Sample : VV0727WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Quant Time: Jul 28 01:42:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 01:41:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	582403	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	587620	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	260298	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	230428	47.174	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.340%
7) Chloroethane-d5	1.564	69	184444	46.675	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.340%
11) 1,1-Dichloroethene-d2	2.101	63	301690	34.330	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.660%
21) 2-Butanone-d5	3.883	46	238026	72.294	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.290%
24) Chloroform-d	4.339	84	385141	40.063	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.120%
26) 1,2-Dichloroethane-d4	5.024	65	225676	41.040	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.080%
32) Benzene-d6	5.043	84	787650	44.343	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.680%
36) 1,2-Dichloropropane-d6	6.063	67	243874	42.604	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.200%
41) Toluene-d8	7.313	98	656744	42.258	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.520%
43) trans-1,3-Dichloroprop...	7.619	79	97031	40.455	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.900%
47) 2-Hexanone-d5	8.088	63	158811	63.718	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	63.720%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	328587	37.787	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	75.580%
66) 1,2-Dichlorobenzene-d4	11.622	152	236764	48.484	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.960%
Target Compounds						
39) cis-1,3-Dichloropropene	6.982	75	6030	0.883	ug/L	Qvalue # 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026995.D
Acq On : 27 Jul 2022 13:07
Operator : SY/MD
Sample : VV0727WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Time: Jul 28 01:42:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 01:41:31 2022
Response via : Initial Calibration

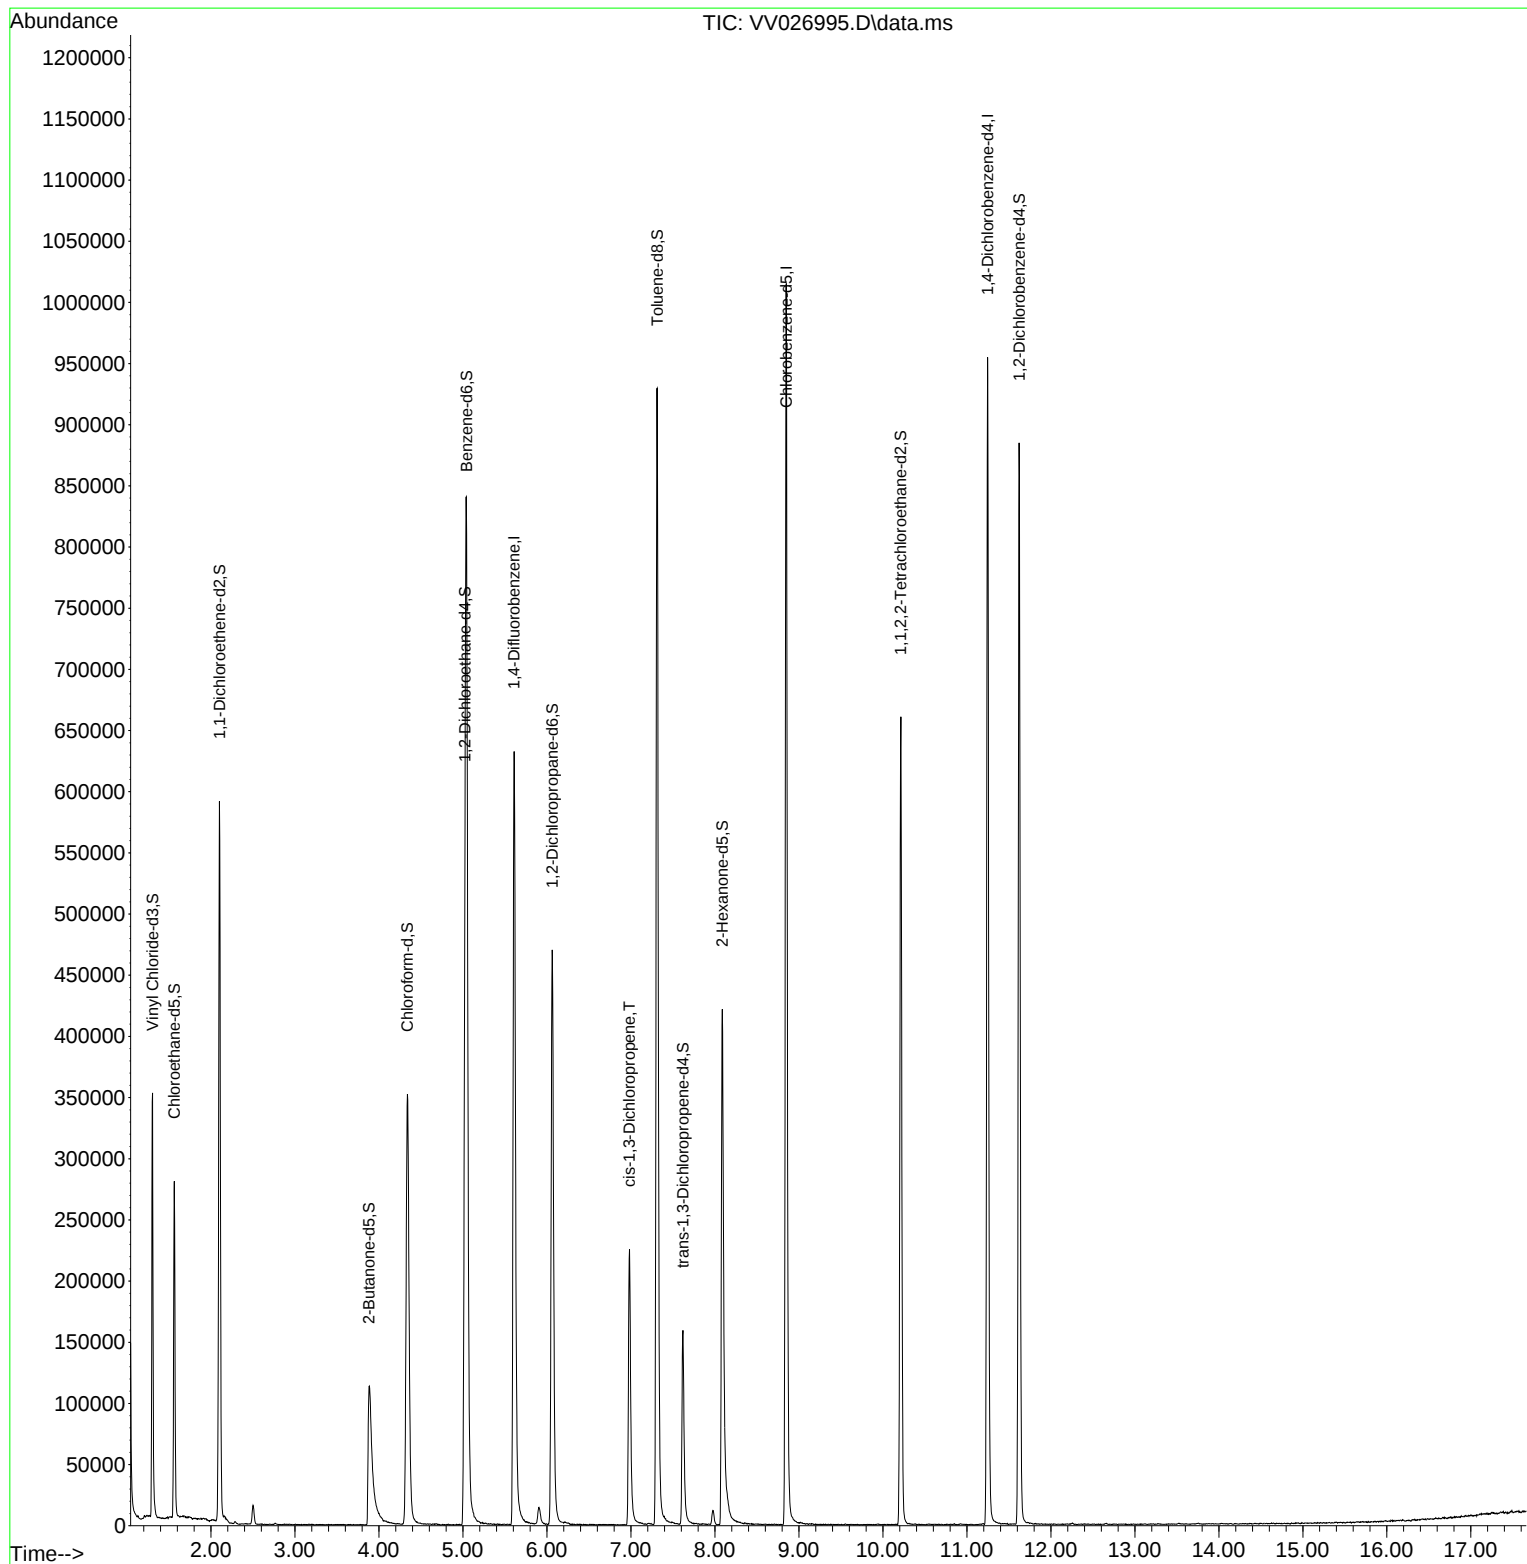

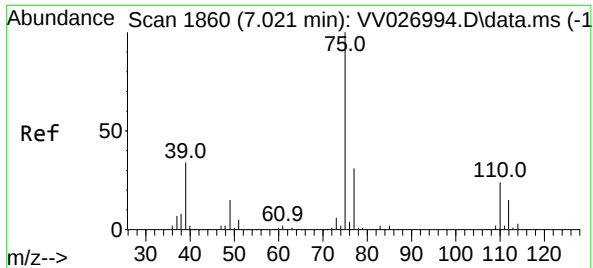

#39
 cis-1,3-Dichloropropene
 Concen: 0.883 ug/L
 RT: 6.982 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV026995.D
 Acq: 27 Jul 2022 13:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Tgt Ion: 75 Resp: 6030
 Ion Ratio Lower Upper
 75 100
 77 48.9 22.4 41.6#

