

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027002.D
 Acq On : 27 Jul 2022 16:33
 Operator : SY/MD
 Sample : N3897-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ1

Quant Time: Jul 28 01:43:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 01:41:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	571147	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	563388	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	254864	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	171545	35.811	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	71.620%	
7) Chloroethane-d5	1.564	69	168823	43.564	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	87.120%	
11) 1,1-Dichloroethene-d2	2.101	63	268735	31.183	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	62.360%	
21) 2-Butanone-d5	3.886	46	353503	109.483	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	109.480%	
24) Chloroform-d	4.342	84	435786	46.225	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.440%	
26) 1,2-Dichloroethane-d4	5.027	65	258026	47.847	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.700%	
32) Benzene-d6	5.046	84	872597	51.239	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.480%	
36) 1,2-Dichloropropane-d6	6.066	67	282236	51.427	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	102.860%	
41) Toluene-d8	7.313	98	706449	47.411	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.820%	
43) trans-1,3-Dichloroprop...	7.622	79	111407	48.446	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.900%	
47) 2-Hexanone-d5	8.088	63	256757	107.446	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	107.450%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	403214	48.363	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	96.720%	
66) 1,2-Dichlorobenzene-d4	11.622	152	284175	59.433	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	118.860%	
Target Compounds						
					Qvalue	
13) Acetone	2.178	43	80610	35.556	ug/L	98
39) cis-1,3-Dichloropropene	6.989	75	6114	0.934	ug/L #	66
42) Toluene	7.394	91	26016	1.407	ug/L	100
71) Naphthalene	13.499	128	278749	19.311	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027002.D
Acq On : 27 Jul 2022 16:33
Operator : SY/MD
Sample : N3897-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ1

Quant Time: Jul 28 01:43:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 01:41:31 2022
Response via : Initial Calibration




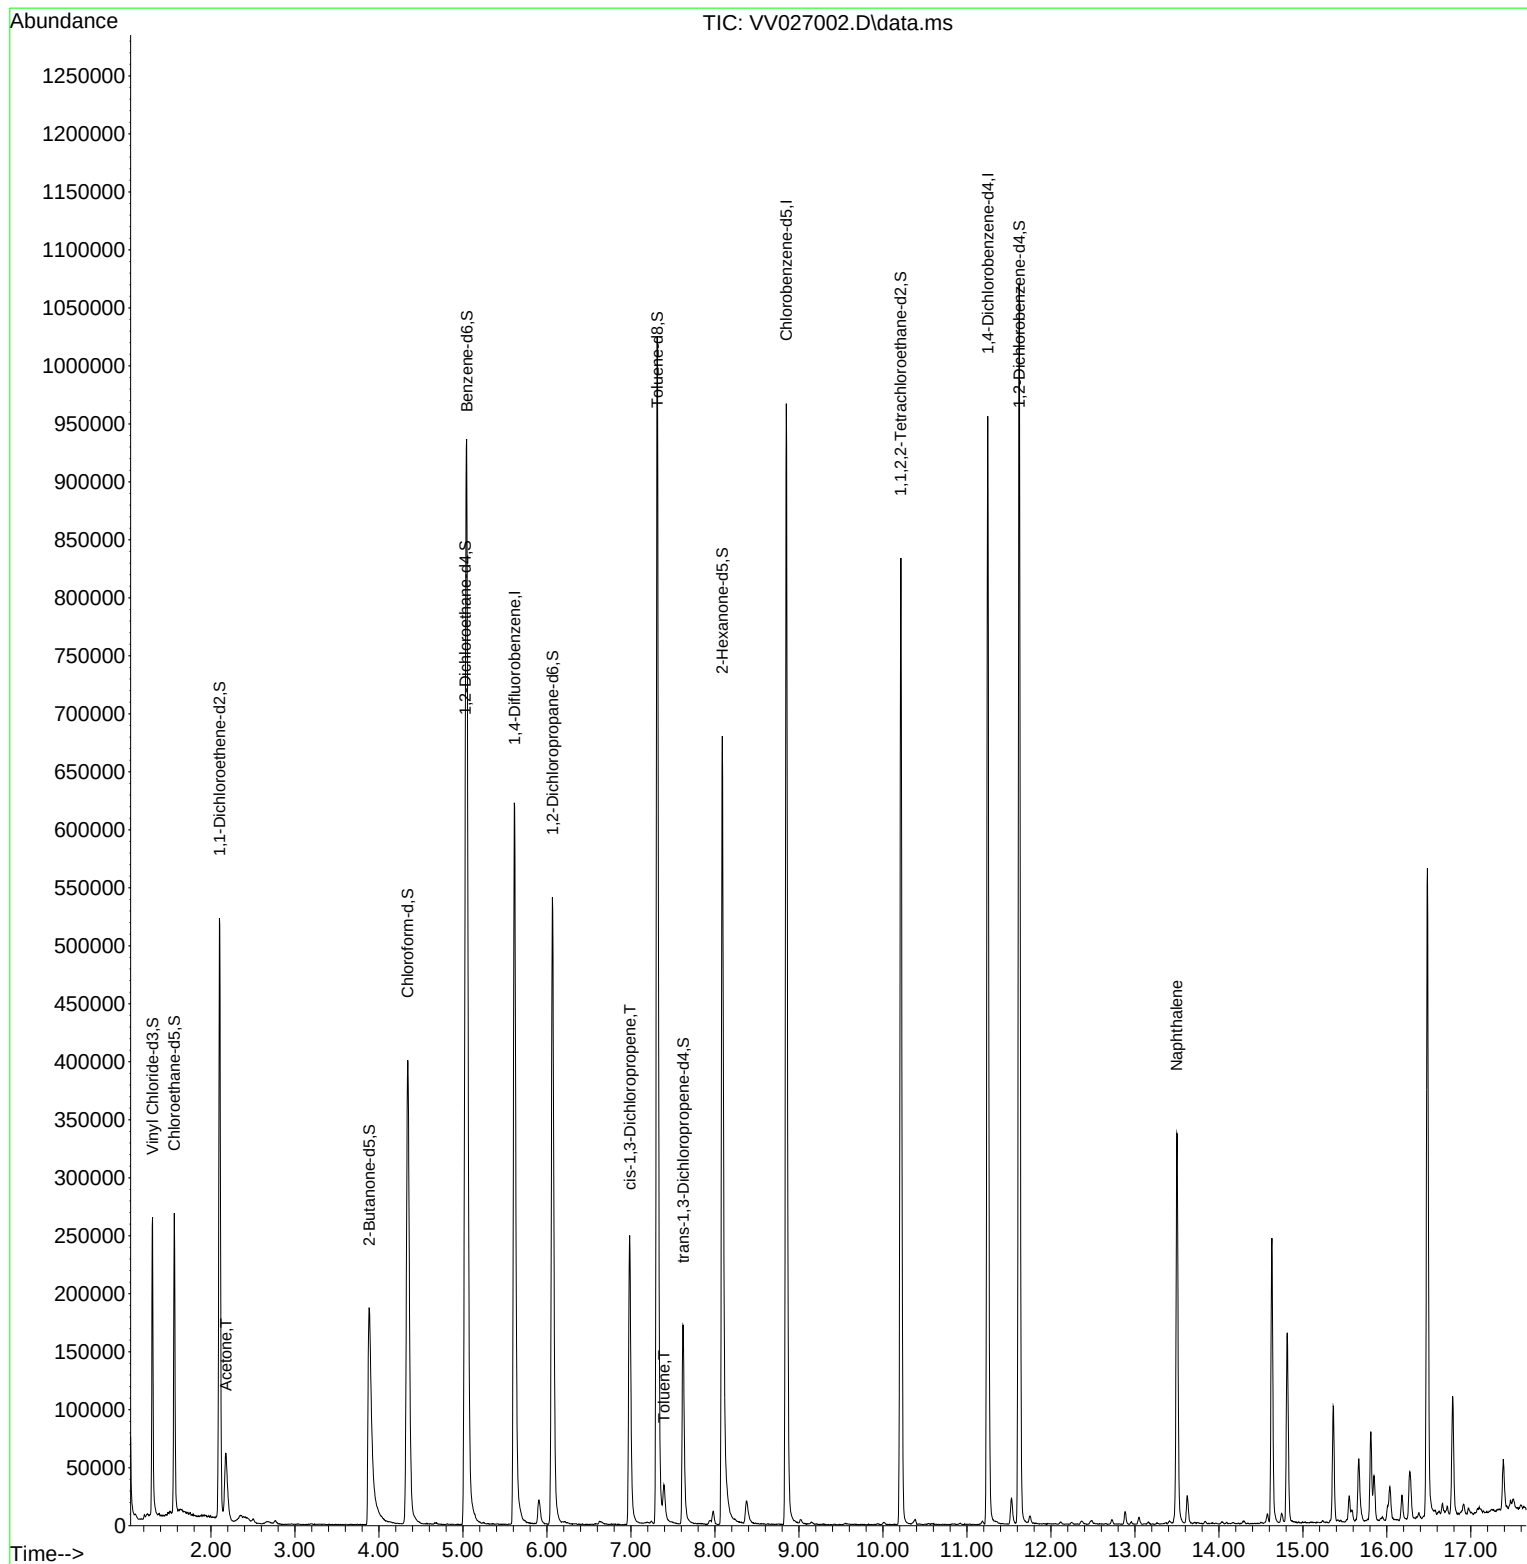


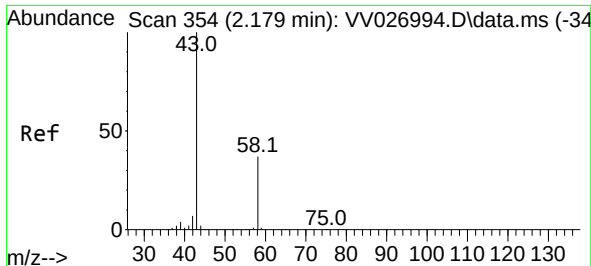

#13
Acetone
Concen: 35.556 ug/L
RT: 2.178 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV027002.D
Acq: 27 Jul 2022 16:33




Instrument :
MSVOA_V
ClientSampleId :
DBUQ1


Tgt Ion: 43 Resp: 80610
Ion Ratio Lower Upper
43 100
58 37.6 0.0 72.6

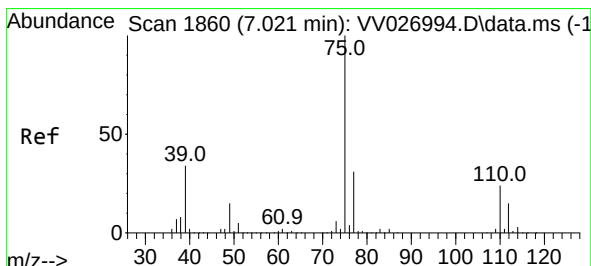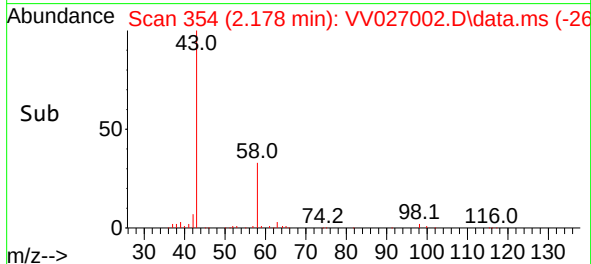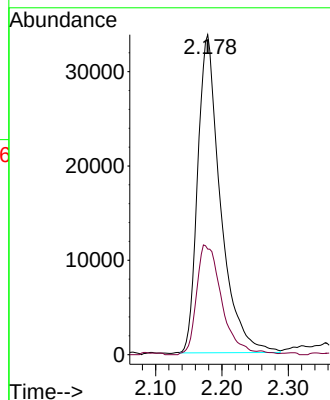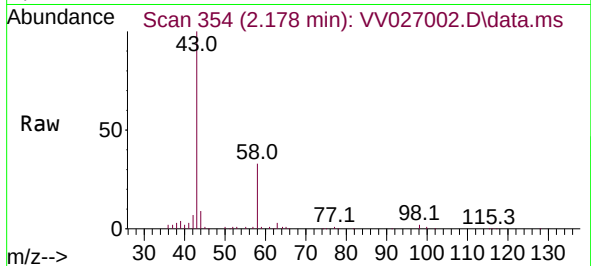

#39
cis-1,3-Dichloropropene
Concen: 0.934 ug/L
RT: 6.989 min Scan# 1850
Delta R.T. -0.032 min
Lab File: VV027002.D
Acq: 27 Jul 2022 16:33

Tgt Ion: 75 Resp: 6114
Ion Ratio Lower Upper
75 100
77 51.0 22.4 41.6#

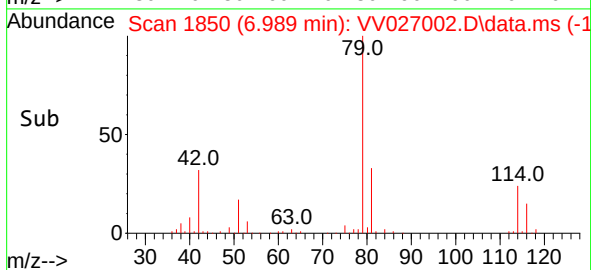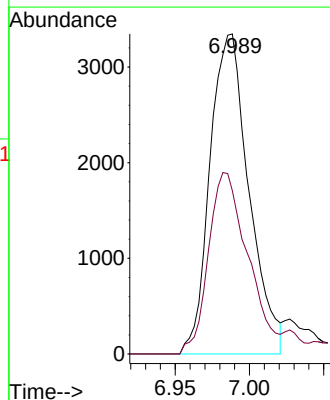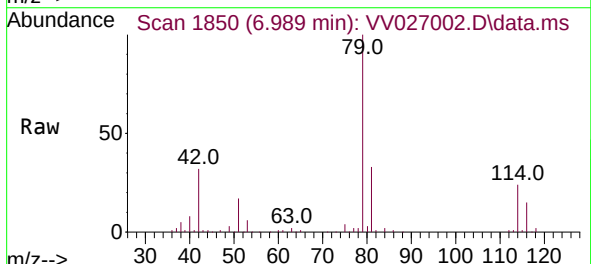

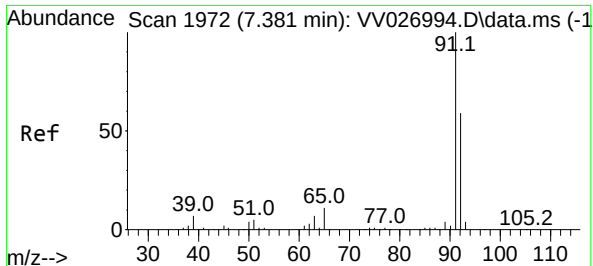

#42

Toluene

Concen: 1.407 ug/L

RT: 7.394 min Scan# 1972

Delta R.T. 0.013 min

Lab File: VV027002.D

Acq: 27 Jul 2022 16:33

Instrument :

MSVOA_V

ClientSampleId :





DBUQ1

Tgt Ion: 91 Resp: 26016

Ion Ratio Lower Upper

91 100

92 58.1 40.5 75.1

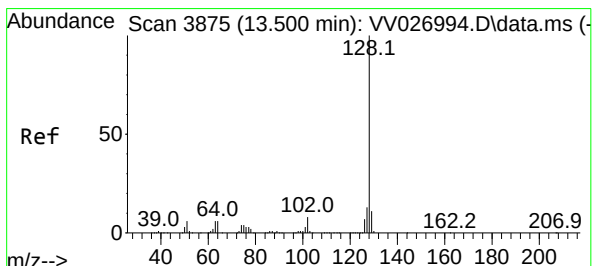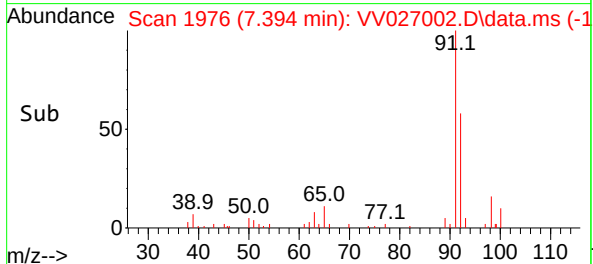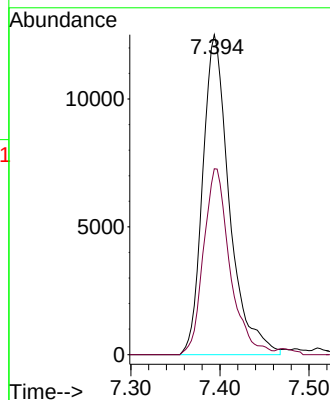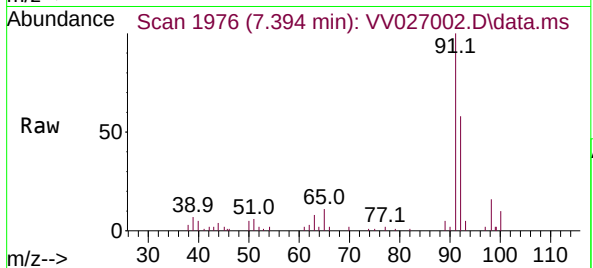

#71

Naphthalene

Concen: 19.311 ug/L

RT: 13.499 min Scan# 3875

Delta R.T. -0.000 min

Lab File: VV027002.D

Acq: 27 Jul 2022 16:33

Tgt Ion: 128 Resp: 278749

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 11.0 8.6 13.0

