




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP7

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 02:51:09 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
Supervised By :Mahesh Dadoda 07/28/2022

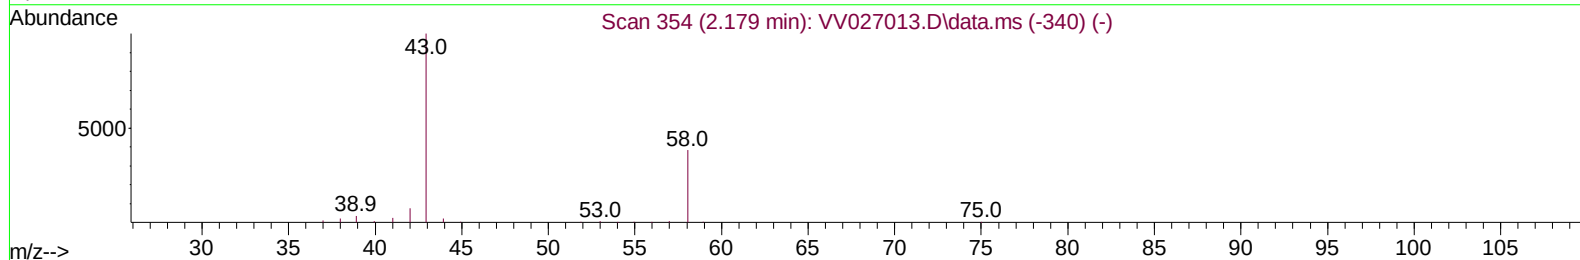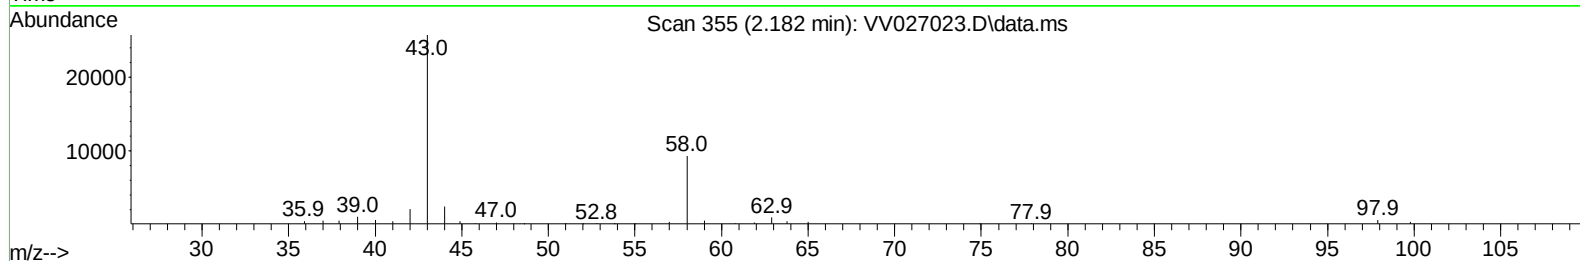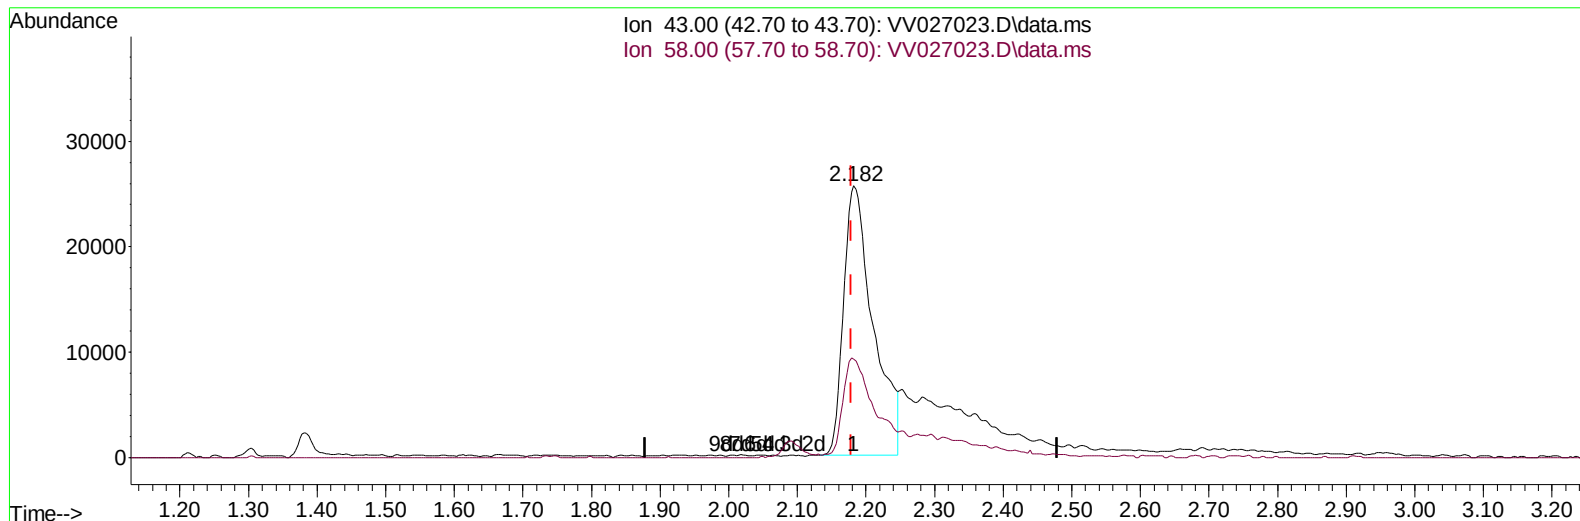

TIC: VV027023.D\data.ms

(13) Acetone (T)

2.182min (+ 0.003) 41.85 ug/L

response 77021

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	31.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027023.D
 Acq On : 28 Jul 2022 01:33
 Operator : SY/MD
 Sample : N3897-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP7

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
 Supervised By :Mahesh Dadoda 07/28/2022

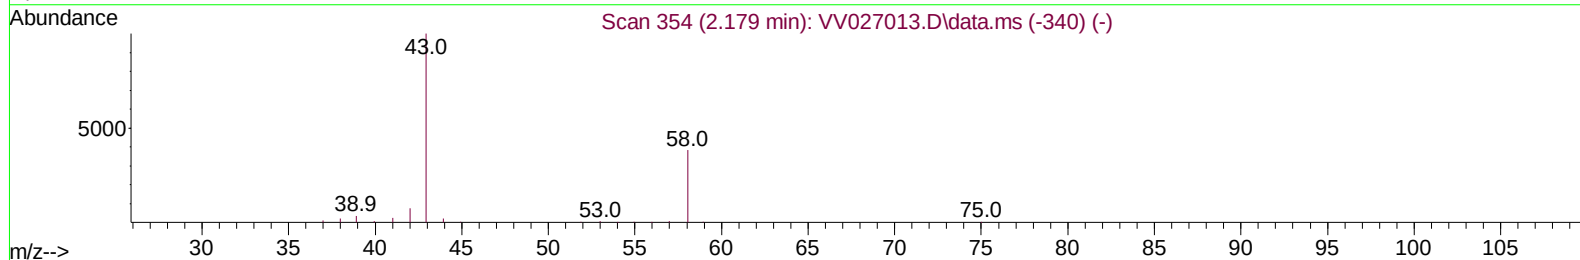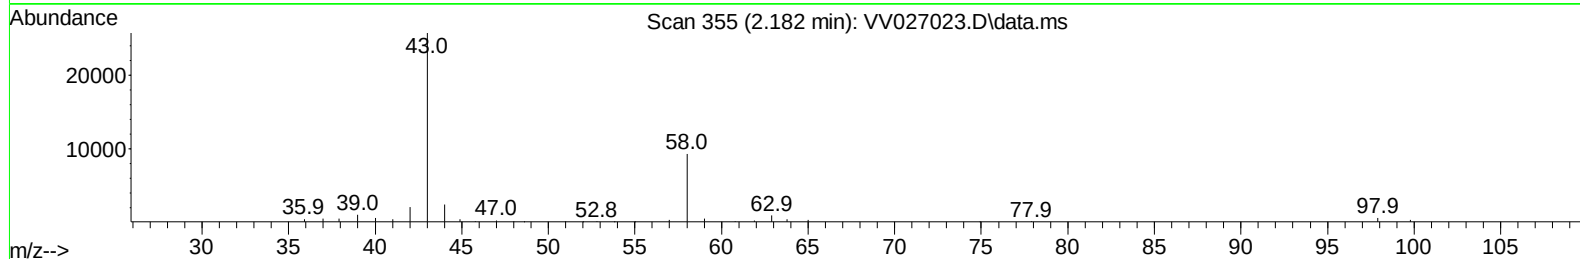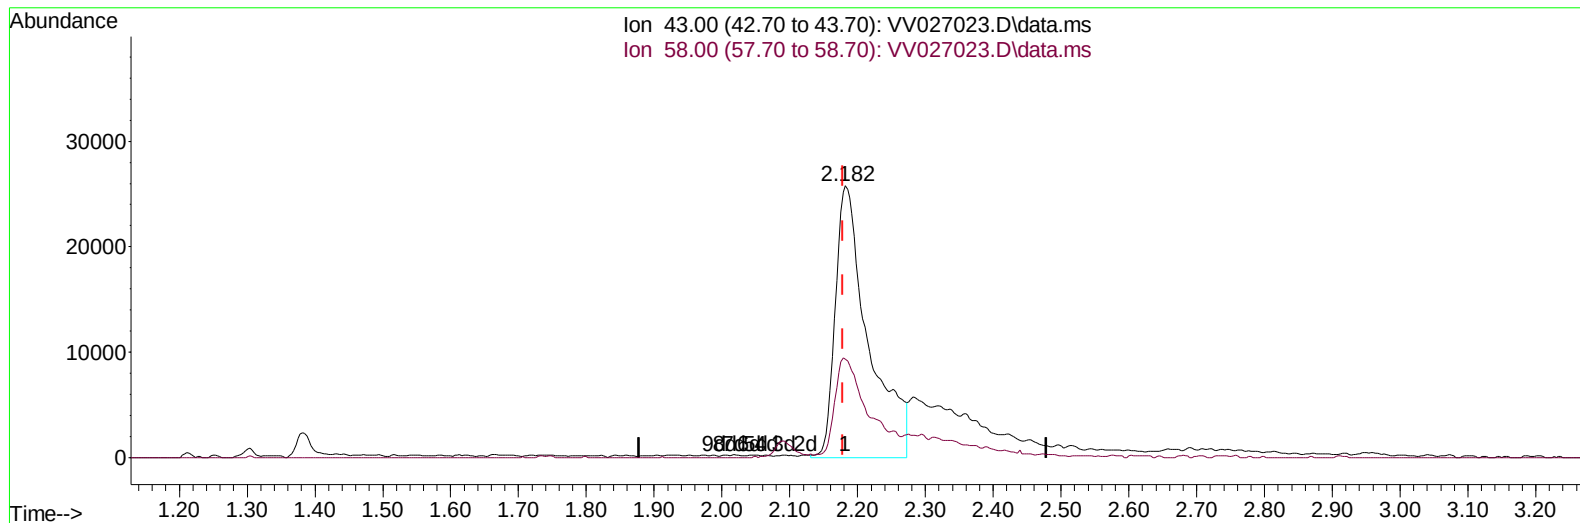

TIC: VV027023.D\data.ms

(13) Acetone (T)

2.182min (+ 0.003) 47.48 ug/L m

response 87385

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	27.70
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027023.D
 Acq On : 28 Jul 2022 01:33
 Operator : SY/MD
 Sample : N3897-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP7

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
 Supervised By :Mahesh Dadoda 07/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	463672	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	463738	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	197092	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	205882	52.942	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	105.880%	
7) Chloroethane-d5	1.561	69	172165	54.724	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	109.440%	
11) 1,1-Dichloroethene-d2	2.102	63	277786	39.704	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.400%	
21) 2-Butanone-d5	3.892	46	200354	76.434	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	76.430%	
24) Chloroform-d	4.343	84	373703	48.828	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.660%	
26) 1,2-Dichloroethane-d4	5.027	65	219717	50.187	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.380%	
32) Benzene-d6	5.044	84	758144	54.084	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.160%	
36) 1,2-Dichloropropane-d6	6.066	67	239060	52.920	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	105.840%	
41) Toluene-d8	7.314	98	615682	50.198	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.400%	
43) trans-1,3-Dichloroprop...	7.619	79	90115	47.608	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	95.220%	
47) 2-Hexanone-d5	8.088	63	172575	87.737	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	87.740%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	335728	48.922	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	97.840%	
66) 1,2-Dichlorobenzene-d4	11.622	152	222159	60.082	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	120.160%#	
Target Compounds						
13) Acetone	2.182	43	87385m	47.478	ug/L	
22) 2-Butanone	3.992	43	31942	12.725	ug/L	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP7

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 02:51:09 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
Supervised By :Mahesh Dadoda 07/28/2022

