




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027026.D
 Acq On : 28 Jul 2022 02:47
 Operator : SY/MD
 Sample : N3897-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
 Supervised By :Mahesh Dadoda 07/28/2022

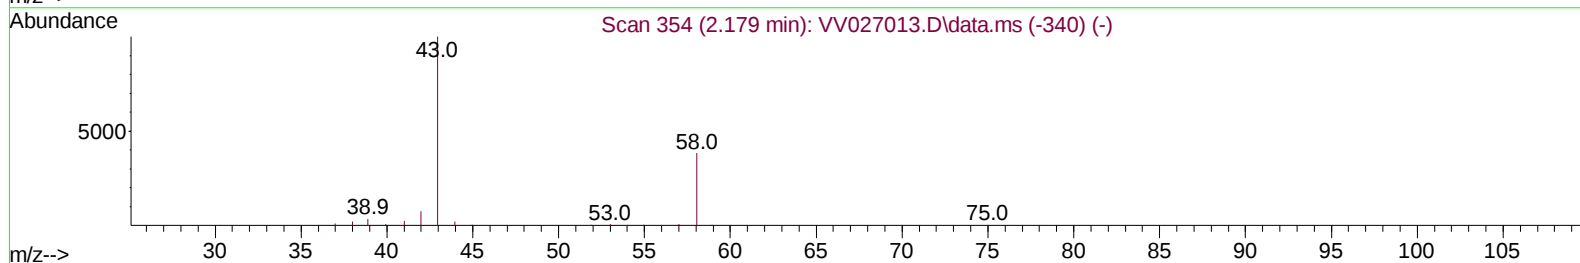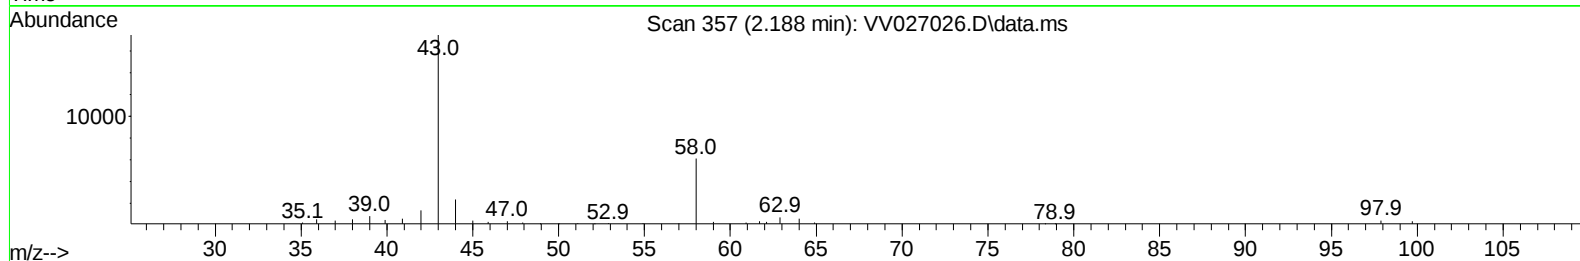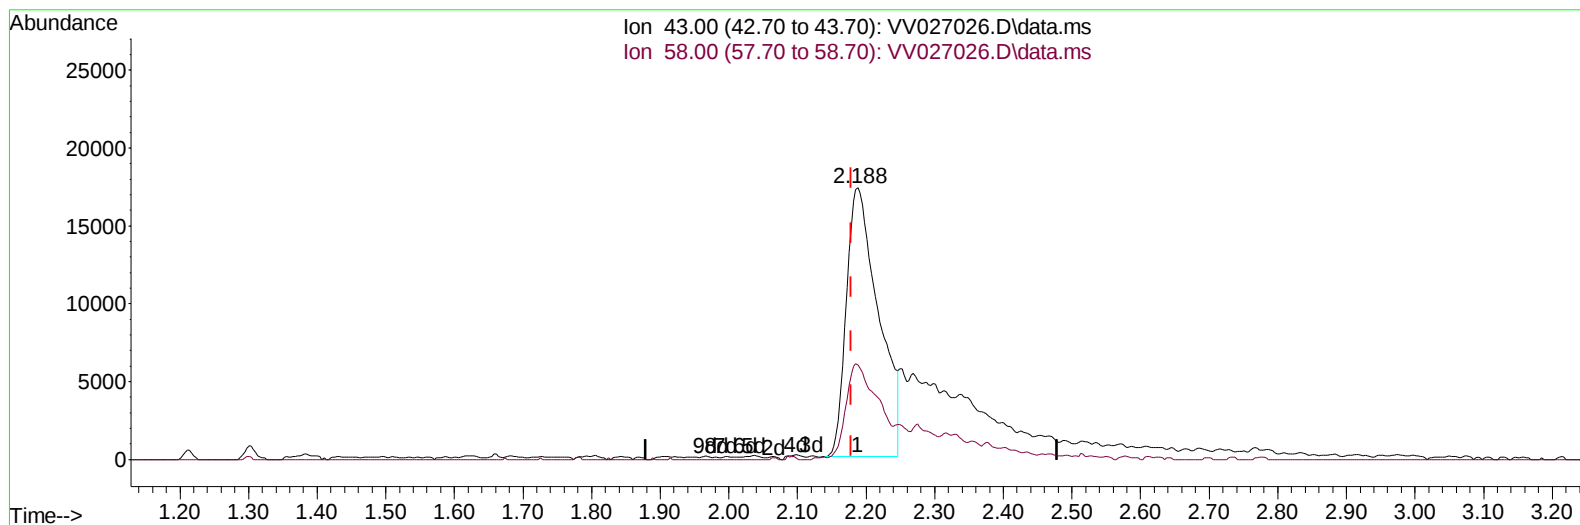

TIC: VV027026.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 32.58 ug/L

response 56279

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	34.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027026.D
 Acq On : 28 Jul 2022 02:47
 Operator : SY/MD
 Sample : N3897-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
 Supervised By :Mahesh Dadoda 07/28/2022

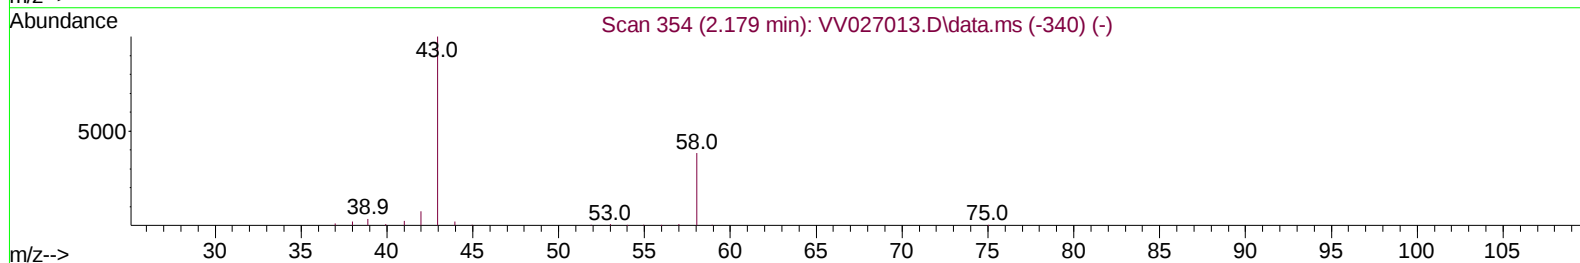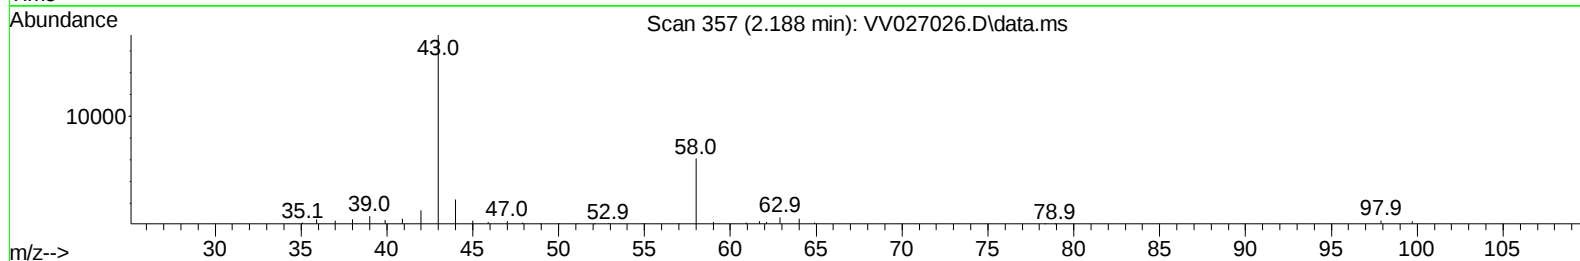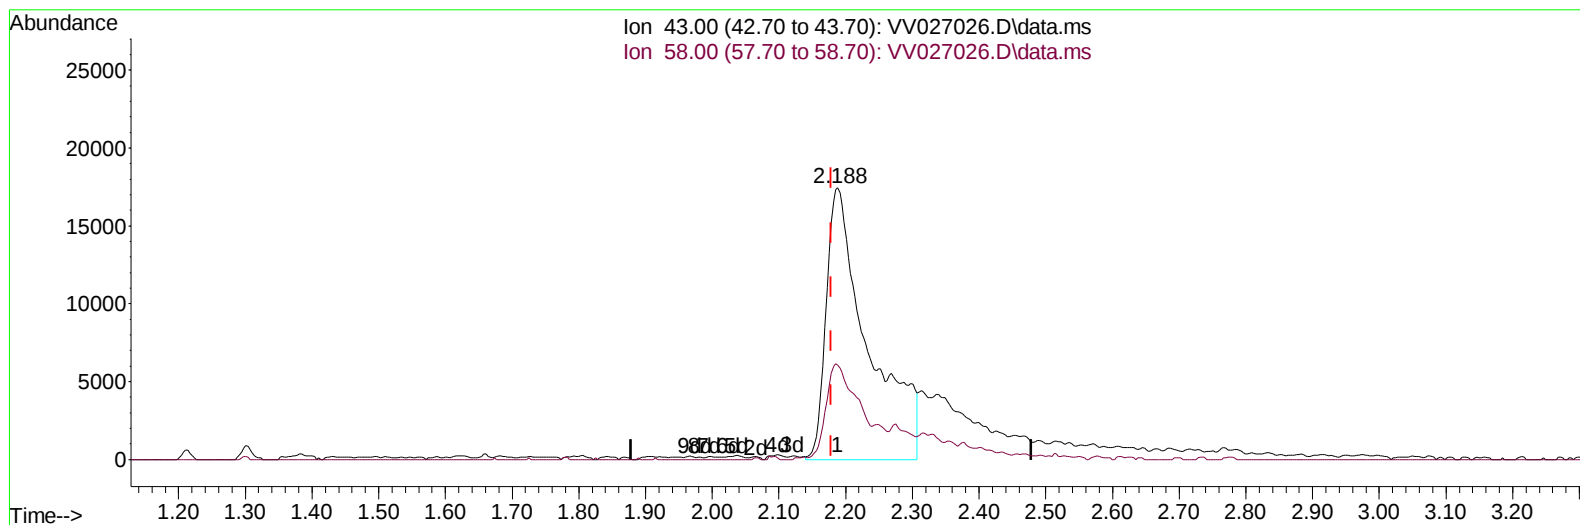

TIC: VV027026.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 43.96 ug/L m

response 75938

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	36.30	25.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027026.D
 Acq On : 28 Jul 2022 02:47
 Operator : SY/MD
 Sample : N3897-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
 Supervised By :Mahesh Dadoda 07/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	435161	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	446972	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	187187	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	207279	56.793	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	113.580%	
7) Chloroethane-d5	1.564	69	173858	58.883	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	117.760%	
11) 1,1-Dichloroethene-d2	2.101	63	280738	42.755	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.520%	
21) 2-Butanone-d5	3.895	46	188523	76.633	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	76.630%	
24) Chloroform-d	4.342	84	379226	52.796	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.600%	
26) 1,2-Dichloroethane-d4	5.027	65	223369	54.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.720%	
32) Benzene-d6	5.043	84	763699	56.524	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.040%	
36) 1,2-Dichloropropane-d6	6.066	67	243092	55.831	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	111.660%	
41) Toluene-d8	7.313	98	616335	52.136	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	104.280%	
43) trans-1,3-Dichloroprop...	7.619	79	87437	47.926	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	95.860%	
47) 2-Hexanone-d5	8.091	63	172943	91.222	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	91.220%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	340661	51.502	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	103.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	225436	64.195	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	128.380%#	
Target Compounds						
13) Acetone	2.188	43	75938m	43.962	ug/L	
19) 1,1-Dichloroethane	3.185	63	5068	0.774	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027026.D
Acq On : 28 Jul 2022 02:47
Operator : SY/MD
Sample : N3897-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 06:18:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 02:51:09 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/28/2022
Supervised By :Mahesh Dadoda 07/28/2022

