

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072722\
 Data File : VW027007.D
 Acq On : 27 Jul 2022 18:36
 Operator : SY/MD
 Sample : N3880-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF6DL

Quant Time: Jul 28 01:44:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 01:41:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	497003	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	484498	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	212617	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	150999	36.225	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.440%		
7) Chloroethane-d5	1.565	69	148587	44.062	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.120%		
11) 1,1-Dichloroethene-d2	2.101	63	232635	31.021	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.040%		
21) 2-Butanone-d5	3.883	46	321072	114.273	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	114.270%		
24) Chloroform-d	4.343	84	388462	47.352	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.700%		
26) 1,2-Dichloroethane-d4	5.027	65	233263	49.708	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.420%		
32) Benzene-d6	5.043	84	767730	52.421	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.840%		
36) 1,2-Dichloropropane-d6	6.066	67	254582	53.941	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	107.880%		
41) Toluene-d8	7.313	98	613285	47.860	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.720%		
43) trans-1,3-Dichloroprop...	7.619	79	98150	49.631	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.260%		
47) 2-Hexanone-d5	8.088	63	237380	115.512	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	115.510%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	373059	52.032	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.060%		
66) 1,2-Dichlorobenzene-d4	11.622	152	242700	60.845	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	121.680%#		
Target Compounds					Qvalue	
46) Tetrachloroethene	7.973	164	96101	30.769	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027007.D
Acq On : 27 Jul 2022 18:36
Operator : SY/MD
Sample : N3880-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF6DL


Quant Time: Jul 28 01:44:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 01:41:31 2022
Response via : Initial Calibration

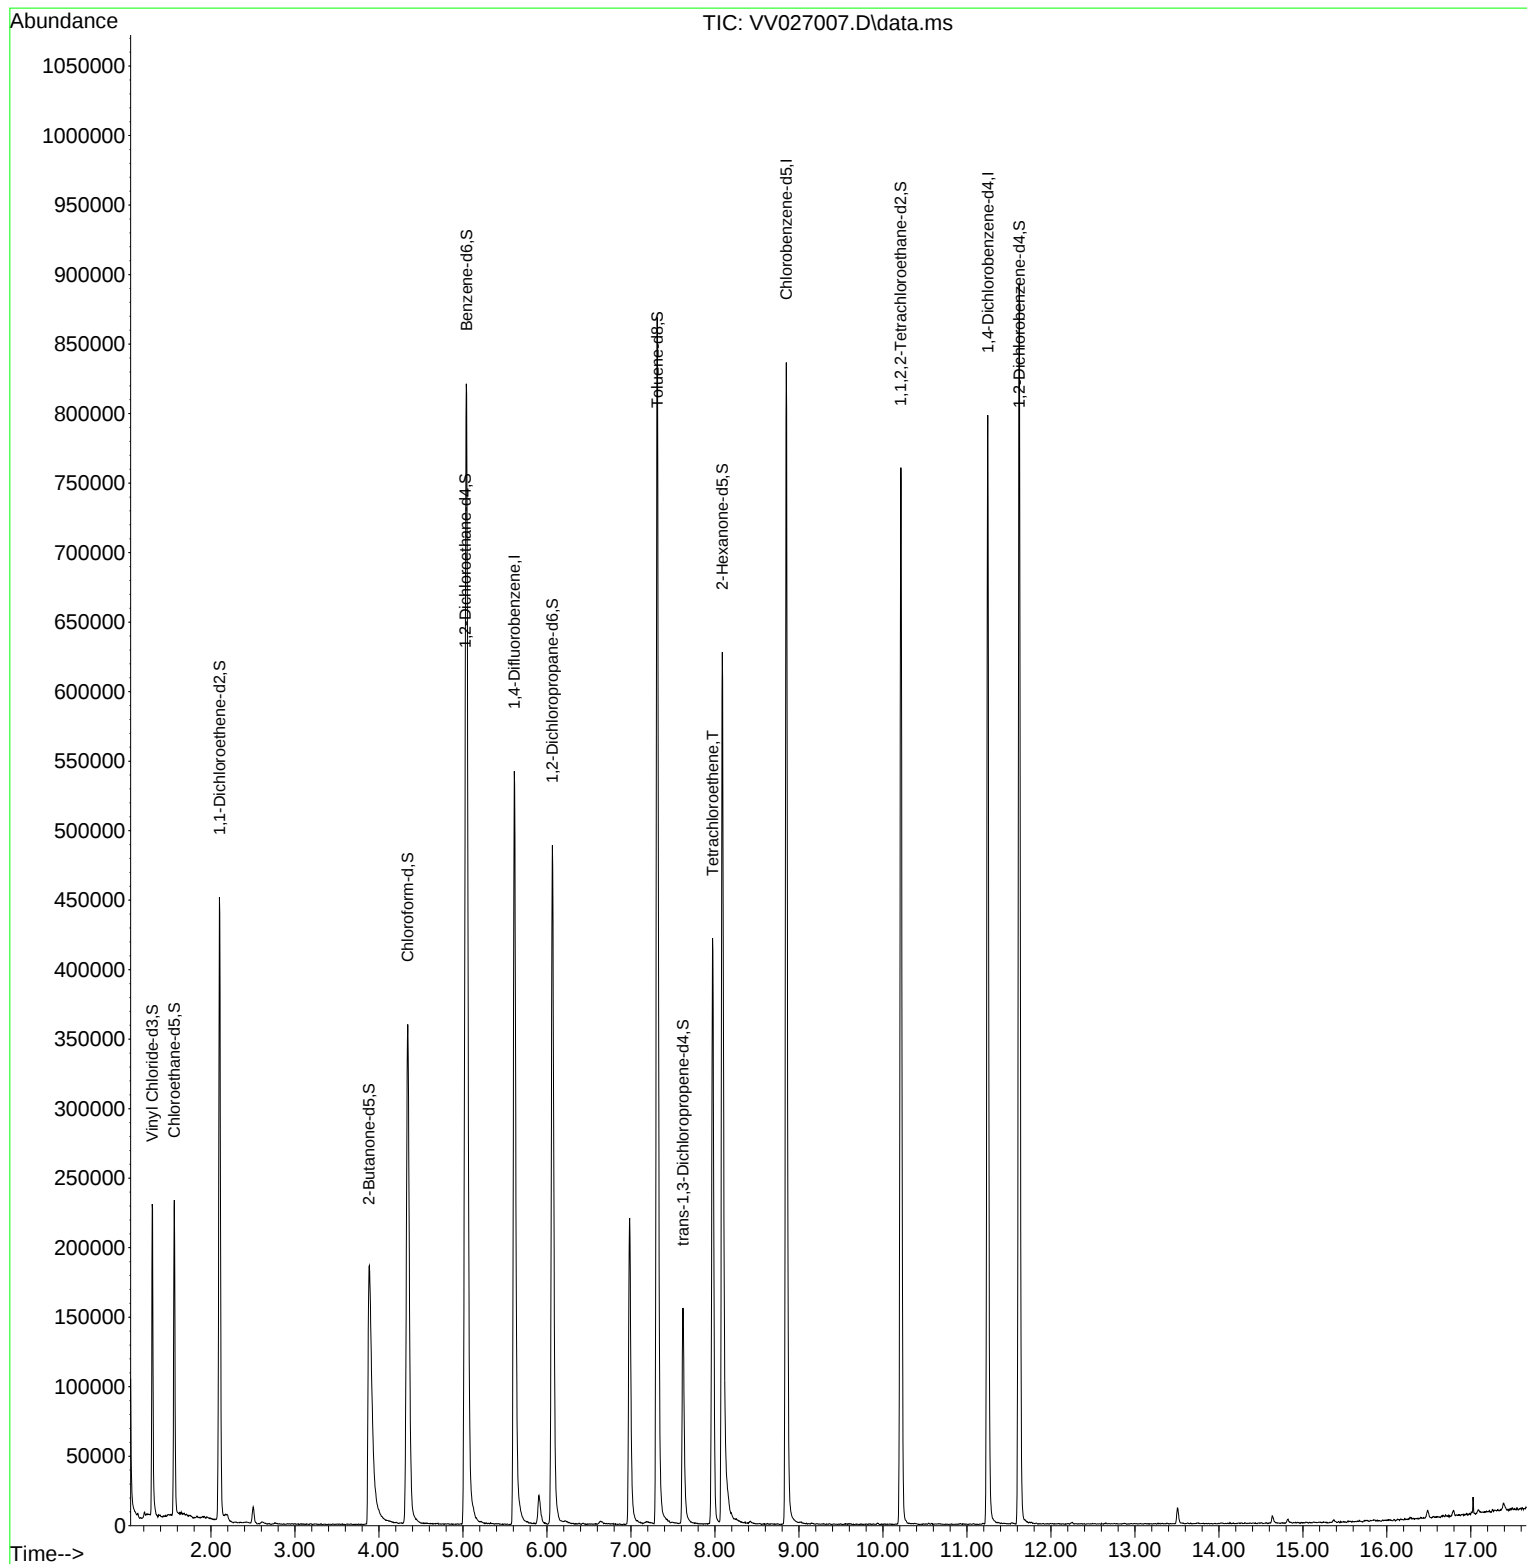

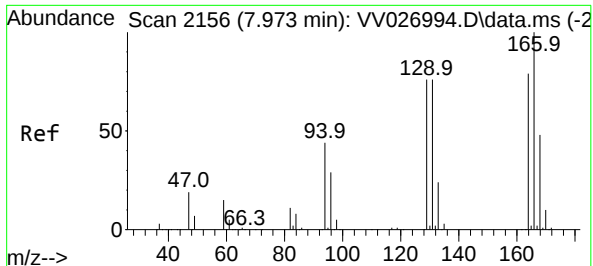

#46
 Tetrachloroethene
 Concen: 30.769 ug/L
 RT: 7.973 min Scan# 2156
 Delta R.T. 0.000 min
 Lab File: VV027007.D
 Acq: 27 Jul 2022 18:36

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF6DL

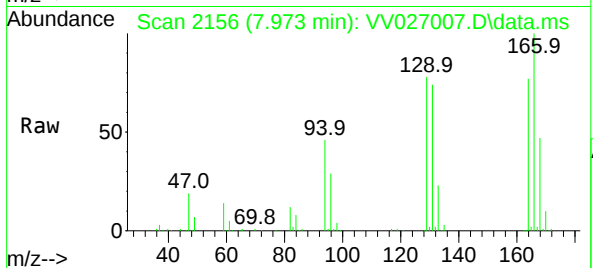

Tgt Ion:	164	Resp:	96101
Ion	Ratio	Lower	Upper
164	100		
129	101.1	66.3	123.1
131	95.1	63.1	117.3
166	129.4	86.2	160.2

