

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072722\
 Data File : VW027027.D
 Acq On : 28 Jul 2022 03:11
 Operator : SY/MD
 Sample : N3897-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ3

Quant Time: Jul 28 06:19:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 28 02:51:09 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	433882	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	447054	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	187548	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	199690	54.875	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	109.740%	
7) Chloroethane-d5	1.564	69	166409	56.526	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	113.060%	
11) 1,1-Dichloroethene-d2	2.101	63	268097	40.951	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.900%	
21) 2-Butanone-d5	3.892	46	172875	70.479	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	70.480%	
24) Chloroform-d	4.342	84	367047	51.251	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.500%	
26) 1,2-Dichloroethane-d4	5.027	65	213322	52.072	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.140%	
32) Benzene-d6	5.046	84	737208	54.554	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	109.100%	
36) 1,2-Dichloropropane-d6	6.066	67	231720	53.209	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.420%	
41) Toluene-d8	7.313	98	595409	50.357	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.720%	
43) trans-1,3-Dichloroprop...	7.619	79	87422	47.909	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	95.820%	
47) 2-Hexanone-d5	8.088	63	169341	89.306	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.310%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	330553	49.965	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.940%	
66) 1,2-Dichlorobenzene-d4	11.622	152	216144	61.430	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	122.860%#	
Target Compounds						
13) Acetone	2.185	43	60812	35.309	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV0727027.D
Acq On : 28 Jul 2022 03:11
Operator : SY/MD
Sample : N3897-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ3

Quant Time: Jul 28 06:19:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 28 02:51:09 2022
Response via : Initial Calibration

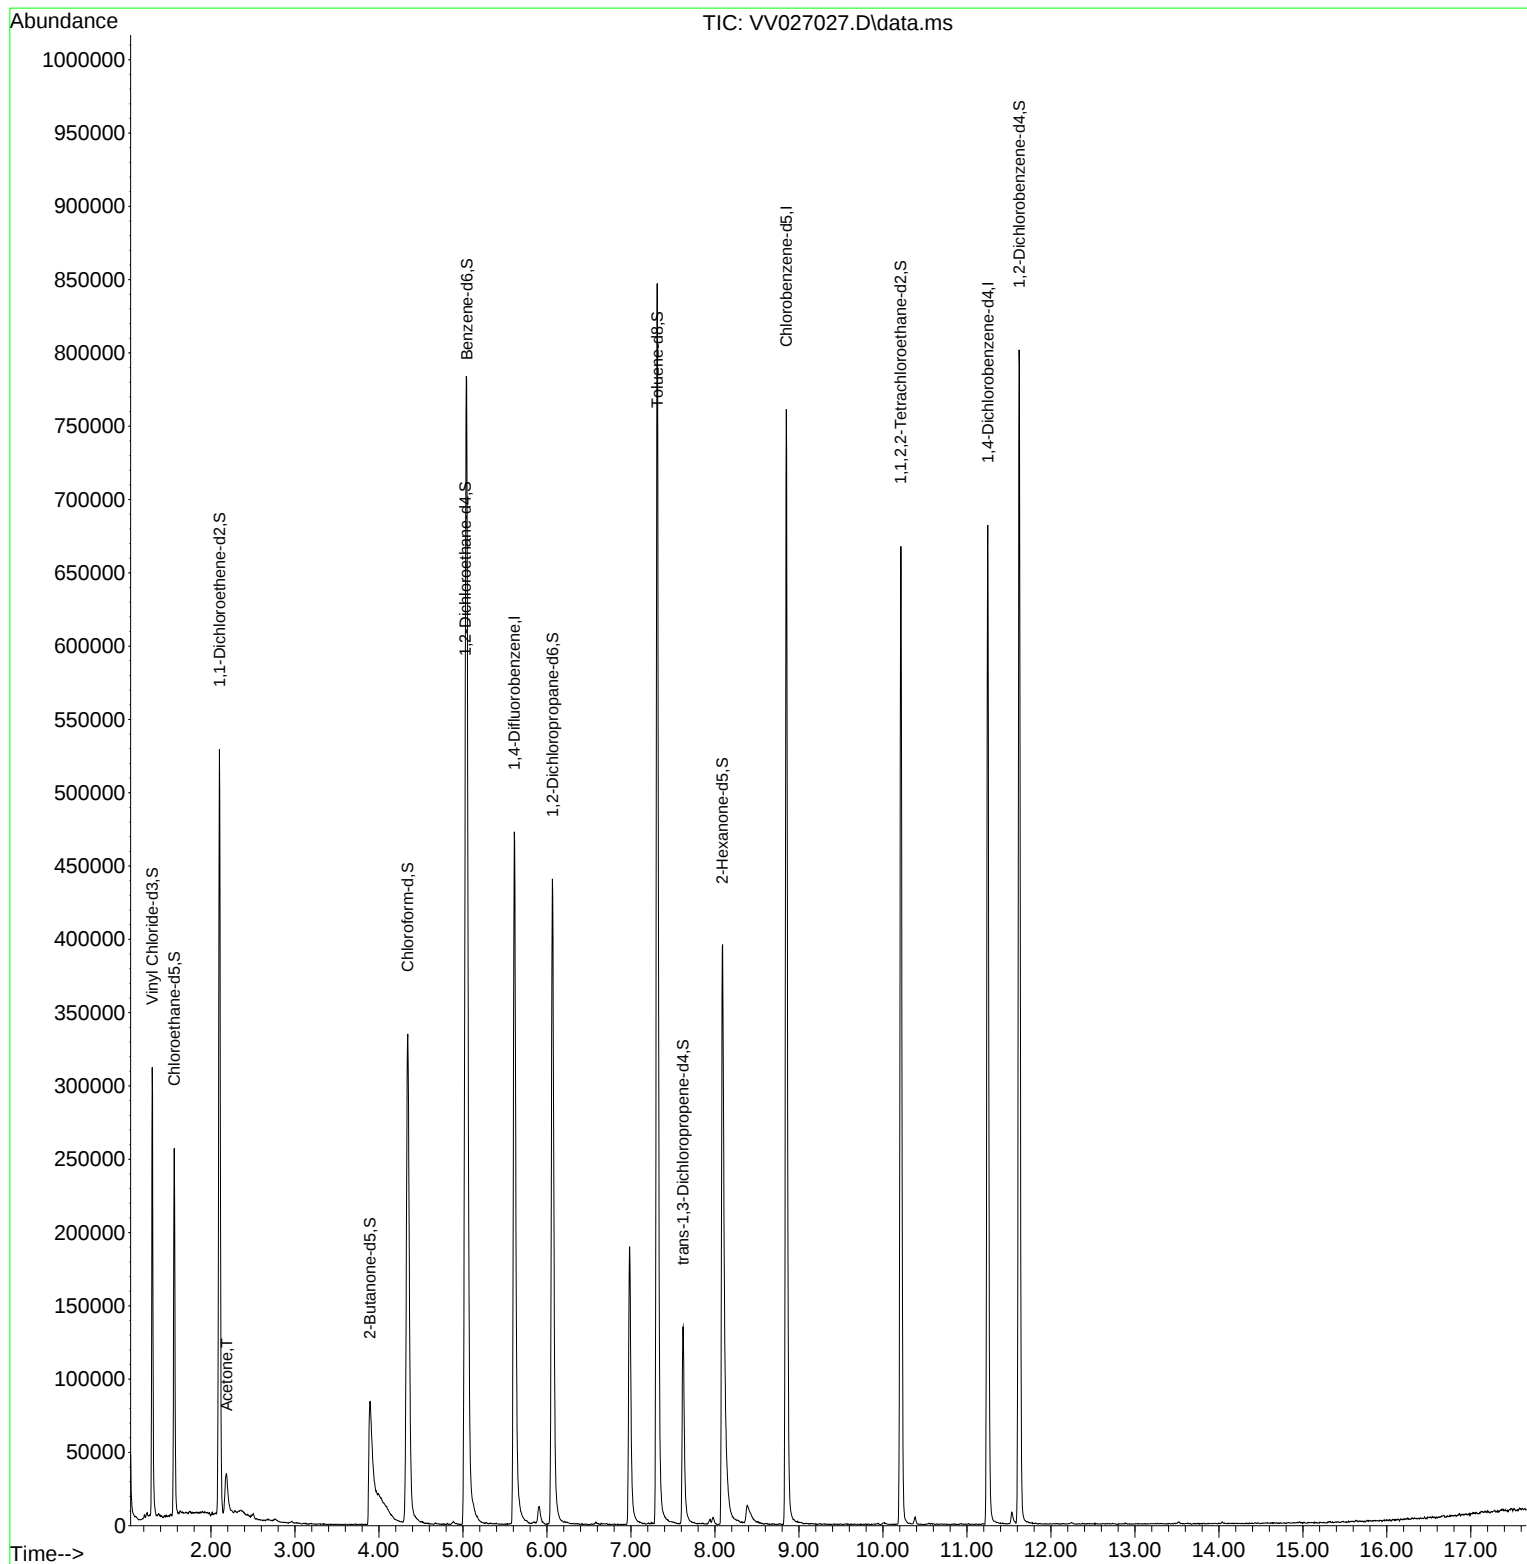

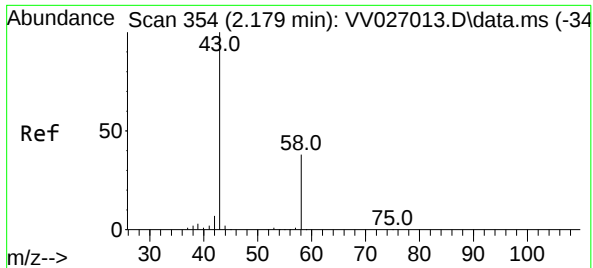

#13
 Acetone
 Concen: 35.309 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV027027.D
 Acq: 28 Jul 2022 03:11

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ3

Tgt Ion: 43 Resp: 60812
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 72.6

