

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026995.D
 Acq On : 27 Jul 2022 13:07
 Operator : SY/MD
 Sample : VV0727WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	347284	367316	17.05%	2.282%
2	1.564	155	163	176	rBV	274794	318505	14.79%	1.979%
3	2.101	320	330	345	rBV	586182	829123	38.49%	5.151%
4	2.500	447	454	470	rVB2	15449	25128	1.17%	0.156%
5	2.851	561	563	564	rBV	259	114	0.01%	0.001%
6	2.928	585	587	594	rBV3	414	334	0.02%	0.002%
7	3.079	632	634	635	rBV	466	119	0.01%	0.001%
8	3.098	638	640	643	rVV	267	169	0.01%	0.001%
9	3.240	682	684	685	rBV	179	72	0.00%	0.000%
10	3.375	720	726	728	rBV3	280	284	0.01%	0.002%
11	3.400	732	734	735	rBV2	324	78	0.00%	0.000%
12	3.561	781	784	789	rBV2	234	203	0.01%	0.001%
13	3.638	805	808	810	rBV2	242	157	0.01%	0.001%
14	3.696	822	826	830	rBV	378	341	0.02%	0.002%
15	3.780	848	852	855	rBV3	299	248	0.01%	0.002%
16	3.812	860	862	863	rBV3	167	49	0.00%	0.000%
17	3.844	870	872	875	rBV	161	94	0.00%	0.001%
18	3.886	875	885	938	rBV	113528	414284	19.23%	2.574%
19	4.339	1010	1026	1060	rBV	351168	875165	40.63%	5.437%
20	4.748	1149	1153	1154	rBV2	199	149	0.01%	0.001%
21	4.760	1154	1157	1161	rVB3	601	386	0.02%	0.002%
22	4.780	1162	1163	1169	rVB2	286	245	0.01%	0.002%
23	4.809	1169	1172	1173	rBV2	412	223	0.01%	0.001%
24	4.844	1181	1183	1184	rBV	252	102	0.00%	0.001%
25	4.854	1184	1186	1189	rVV2	199	106	0.00%	0.001%
26	4.892	1197	1198	1201	rBV	290	180	0.01%	0.001%
27	4.924	1206	1208	1210	rBV2	468	161	0.01%	0.001%
28	5.040	1225	1244	1274	rBV2	840384	2154106	100.00%	13.382%
29	5.551	1401	1403	1404	rBV	299	95	0.00%	0.001%
30	5.609	1409	1421	1456	rBV	632021	1313244	60.96%	8.158%
31	6.063	1549	1562	1596	rBV	469355	972763	45.16%	6.043%
32	6.301	1634	1636	1638	rVB2	735	295	0.01%	0.002%
33	6.320	1638	1642	1644	rBV2	449	348	0.02%	0.002%
34	6.394	1663	1665	1667	rBV	390	175	0.01%	0.001%
35	6.436	1676	1678	1681	rBV3	300	114	0.01%	0.001%
36	6.481	1689	1692	1696	rBV3	275	199	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026995.D
 Acq On : 27 Jul 2022 13:07
 Operator : SY/MD
 Sample : VV0727WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.506	1696	1700	1702	rBV3	435	329	0.02%	0.002%
38	6.564	1716	1718	1721	rBV3	268	149	0.01%	0.001%
39	6.587	1721	1725	1726	rVB	232	149	0.01%	0.001%
40	6.600	1726	1729	1731	rBV2	198	126	0.01%	0.001%
41	6.616	1731	1734	1735	rBV2	280	146	0.01%	0.001%
42	6.641	1740	1742	1745	rVB2	304	176	0.01%	0.001%
43	6.664	1745	1749	1750	rBV2	273	192	0.01%	0.001%
44	6.738	1770	1772	1773	rBV2	210	64	0.00%	0.000%
45	6.789	1785	1788	1793	rVB3	334	277	0.01%	0.002%
46	6.812	1793	1795	1796	rBV	124	33	0.00%	0.000%
47	6.870	1810	1813	1815	rBV	150	80	0.00%	0.000%
48	6.883	1815	1817	1819	rBV	136	78	0.00%	0.000%
49	6.918	1825	1828	1831	rBV	416	219	0.01%	0.001%
50	6.982	1835	1848	1883	rBV	225207	421870	19.58%	2.621%
51	7.313	1938	1951	1976	rBV	928833	1653620	76.77%	10.273%
52	7.619	2036	2046	2080	rBV	158182	284219	13.19%	1.766%
53	7.976	2148	2157	2173	rVB4	11826	21860	1.01%	0.136%
54	8.088	2182	2192	2235	rBV	421236	857008	39.78%	5.324%
55	8.677	2372	2375	2380	rVB	508	387	0.02%	0.002%
56	8.706	2380	2384	2388	rBV2	597	639	0.03%	0.004%
57	8.760	2397	2401	2404	rVB3	554	439	0.02%	0.003%
58	8.786	2404	2409	2414	rBV3	514	562	0.03%	0.003%
59	8.850	2416	2429	2469	rBV	1014638	1661032	77.11%	10.319%
60	9.262	2554	2557	2562	rVB2	466	320	0.01%	0.002%
61	9.291	2562	2566	2569	rBV2	560	406	0.02%	0.003%
62	9.349	2579	2584	2589	rBV4	462	477	0.02%	0.003%
63	9.509	2633	2634	2637	rVB	342	126	0.01%	0.001%
64	9.622	2663	2669	2673	rBV3	438	535	0.02%	0.003%
65	9.741	2701	2706	2711	rBV2	371	574	0.03%	0.004%
66	9.821	2728	2731	2735	rBV2	396	309	0.01%	0.002%
67	9.889	2750	2752	2754	rBV2	261	122	0.01%	0.001%
68	10.214	2841	2853	2879	rBV	660421	1042588	48.40%	6.477%
69	10.452	2924	2927	2928	rBV2	259	169	0.01%	0.001%
70	10.734	3012	3015	3017	rBV	223	113	0.01%	0.001%
71	10.744	3017	3018	3020	rBV	212	84	0.00%	0.001%
72	10.902	3065	3067	3069	rBV	302	148	0.01%	0.001%
73	10.992	3093	3095	3100	rVB2	317	203	0.01%	0.001%
74	11.246	3163	3174	3197	rBV	954009	1481407	68.77%	9.203%
75	11.622	3279	3291	3319	rBV	883694	1391532	64.60%	8.644%
76	12.590	3590	3592	3594	rBV	315	88	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026995.D
Acq On : 27 Jul 2022 13:07
Operator : SY/MD
Sample : VV0727WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis




Sum of corrected areas: 16097529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026995.D
Acq On : 27 Jul 2022 13:07
Operator : SY/MD
Sample : VV0727WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

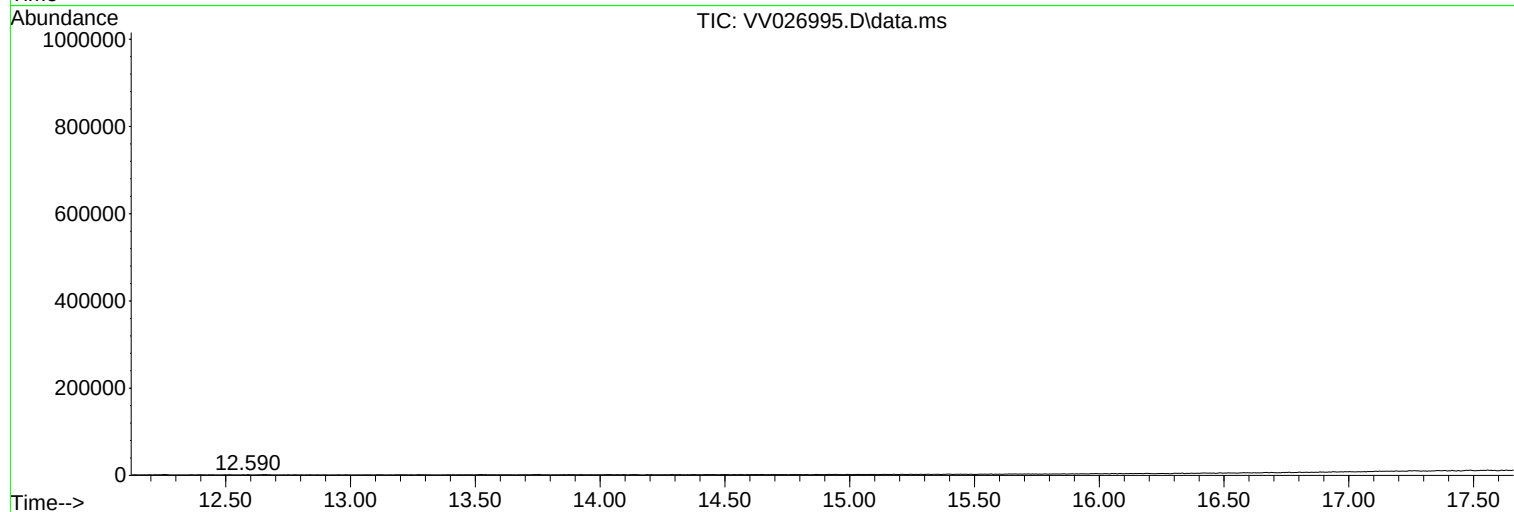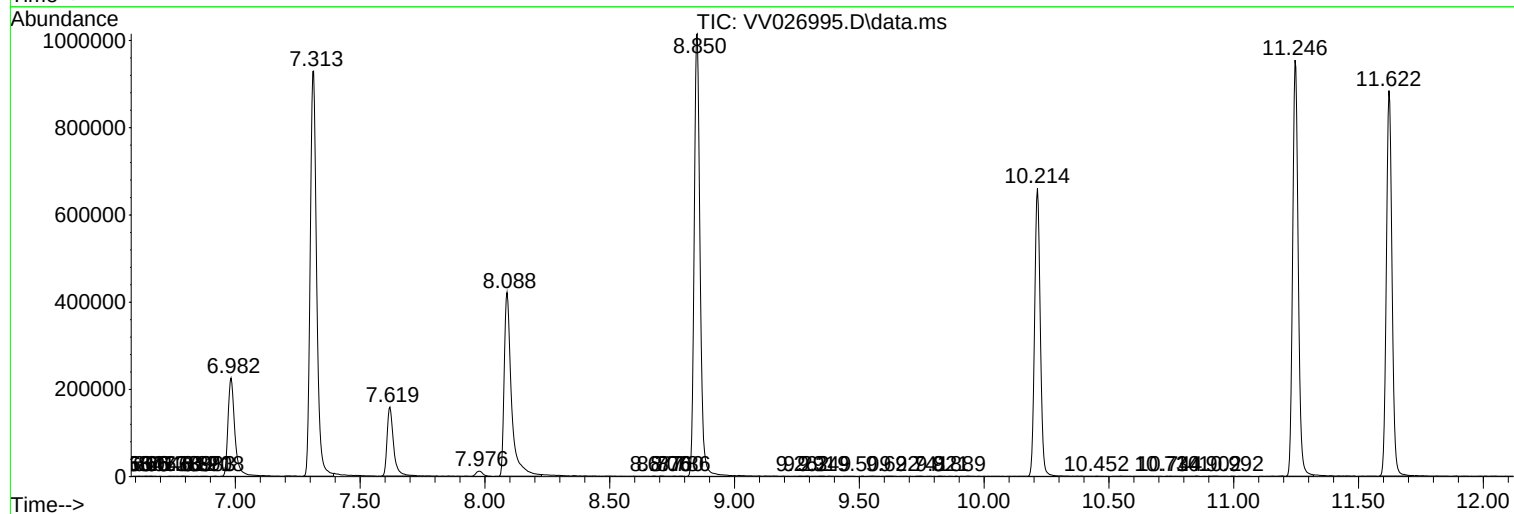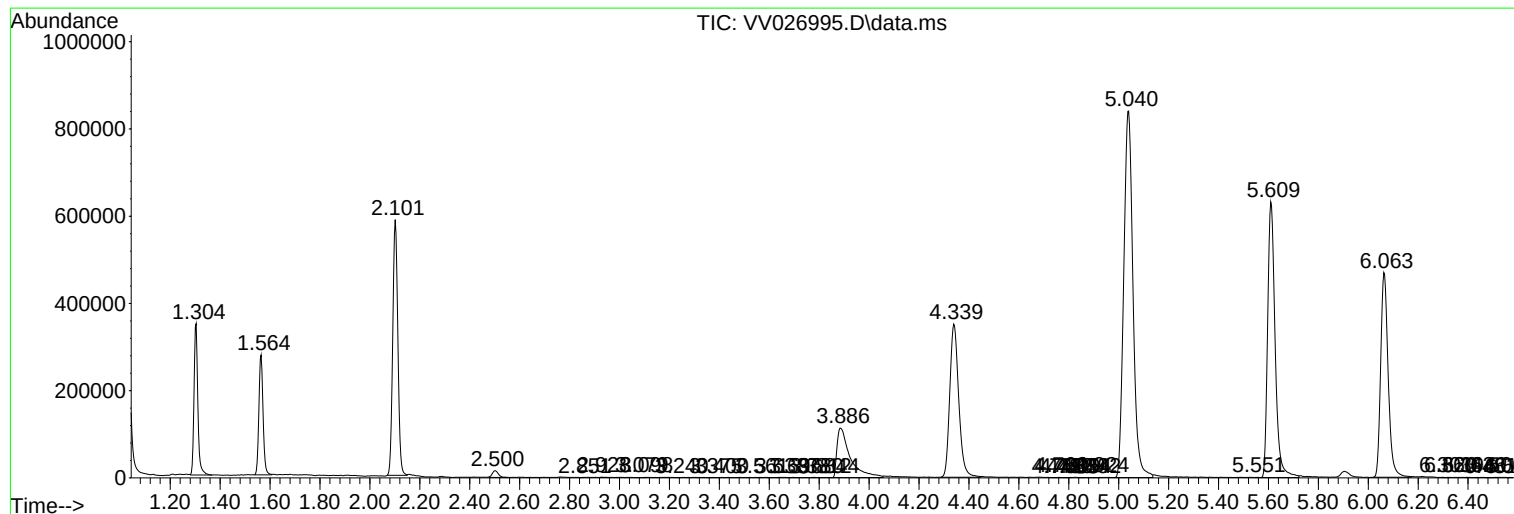

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026995.D
Acq On : 27 Jul 2022 13:07
Operator : SY/MD
Sample : VV0727WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026995.D
Acq On : 27 Jul 2022 13:07
Operator : SY/MD
Sample : VV0727WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc