

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026996.D
 Acq On : 27 Jul 2022 14:03
 Operator : SY/MD
 Sample : VV0727WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	100	rVB	360082	379412	16.76%	2.400%
2	1.564	155	163	176	rBV	295067	334060	14.76%	2.113%
3	2.101	320	330	348	rBV	612758	872952	38.57%	5.522%
4	2.298	381	391	396	rVB4	1496	2219	0.10%	0.014%
5	2.503	445	455	468	rVB	10551	17629	0.78%	0.112%
6	2.764	531	536	539	rBV4	757	557	0.02%	0.004%
7	2.812	547	551	557	rBV2	419	389	0.02%	0.002%
8	2.844	557	561	565	rBV2	464	392	0.02%	0.002%
9	2.957	592	596	598	rBV2	398	280	0.01%	0.002%
10	3.182	663	666	671	rBV3	383	421	0.02%	0.003%
11	3.272	690	694	699	rVB2	404	351	0.02%	0.002%
12	3.478	753	758	761	rVB3	303	305	0.01%	0.002%
13	3.584	787	791	794	rVB2	427	407	0.02%	0.003%
14	3.738	836	839	844	rBV2	352	302	0.01%	0.002%
15	3.805	857	860	866	rVB2	338	363	0.02%	0.002%
16	3.841	866	871	872	rBV2	415	322	0.01%	0.002%
17	3.889	875	886	937	rBV	122315	459101	20.28%	2.904%
18	4.230	989	992	996	rVB2	842	601	0.03%	0.004%
19	4.252	996	999	1002	rBV2	567	383	0.02%	0.002%
20	4.339	1009	1026	1055	rBV	365798	916365	40.48%	5.797%
21	4.561	1094	1095	1100	rVB	499	286	0.01%	0.002%
22	4.600	1105	1107	1110	rBV2	433	306	0.01%	0.002%
23	4.638	1115	1119	1123	rBV4	340	359	0.02%	0.002%
24	4.674	1127	1130	1132	rBV2	373	296	0.01%	0.002%
25	4.760	1154	1157	1163	rVB4	392	392	0.02%	0.002%
26	4.838	1179	1181	1186	rVB3	705	529	0.02%	0.003%
27	4.899	1194	1200	1203	rBV3	448	460	0.02%	0.003%
28	4.921	1203	1207	1213	rBV4	561	752	0.03%	0.005%
29	5.040	1225	1244	1280	rBV2	877808	2263482	100.00%	14.319%
30	5.426	1362	1364	1370	rVB2	469	295	0.01%	0.002%
31	5.500	1384	1387	1391	rBV3	432	334	0.01%	0.002%
32	5.558	1399	1405	1409	rBV3	341	346	0.02%	0.002%
33	5.612	1409	1422	1459	rBV	501992	1043119	46.08%	6.599%
34	5.834	1489	1491	1496	rVB4	746	483	0.02%	0.003%
35	5.905	1502	1513	1531	rBV3	14334	31893	1.41%	0.202%
36	5.992	1537	1540	1544	rVB2	619	404	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026996.D
 Acq On : 27 Jul 2022 14:03
 Operator : SY/MD
 Sample : VV0727WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.066	1548	1563	1594	rBV	488897	1017301	44.94%	6.435%
38	6.294	1632	1634	1638	rBV5	407	334	0.01%	0.002%
39	6.458	1682	1685	1687	rBV2	454	330	0.01%	0.002%
40	6.539	1708	1710	1714	rVB2	715	384	0.02%	0.002%
41	6.648	1740	1744	1746	rVV3	535	408	0.02%	0.003%
42	6.664	1746	1749	1753	rVV3	487	400	0.02%	0.003%
43	6.757	1772	1778	1783	rBV3	406	439	0.02%	0.003%
44	6.982	1837	1848	1874	rBV	230767	435584	19.24%	2.755%
45	7.204	1913	1917	1919	rBV2	393	317	0.01%	0.002%
46	7.313	1939	1951	1979	rBV	996886	1737352	76.76%	10.990%
47	7.619	2032	2046	2072	rBV	169243	301105	13.30%	1.905%
48	7.866	2119	2123	2128	rBV4	686	685	0.03%	0.004%
49	7.940	2141	2146	2149	rVV4	556	519	0.02%	0.003%
50	7.979	2149	2158	2169	rVB3	9639	16906	0.75%	0.107%
51	8.088	2179	2192	2229	rBV	462851	928526	41.02%	5.874%
52	8.355	2273	2275	2278	rVB3	858	355	0.02%	0.002%
53	8.503	2318	2321	2323	rBV2	510	326	0.01%	0.002%
54	8.706	2381	2384	2387	rBV3	529	443	0.02%	0.003%
55	8.850	2417	2429	2451	rBV	803999	1310231	57.89%	8.288%
56	9.027	2477	2484	2491	rVV5	907	1816	0.08%	0.011%
57	9.072	2495	2498	2501	rVV2	610	442	0.02%	0.003%
58	9.124	2511	2514	2517	rVB4	500	332	0.01%	0.002%
59	9.162	2523	2526	2529	rBV2	410	314	0.01%	0.002%
60	9.188	2533	2534	2541	rVB2	460	447	0.02%	0.003%
61	9.368	2586	2590	2595	rBV2	485	386	0.02%	0.002%
62	9.442	2610	2613	2618	rBV2	329	427	0.02%	0.003%
63	9.503	2629	2632	2636	rBV2	310	302	0.01%	0.002%
64	9.548	2643	2646	2651	rBV4	773	761	0.03%	0.005%
65	9.667	2679	2683	2687	rBV3	279	376	0.02%	0.002%
66	9.979	2777	2780	2785	rBV2	403	325	0.01%	0.002%
67	10.062	2804	2806	2810	rBV3	295	283	0.01%	0.002%
68	10.133	2822	2828	2832	rBV2	437	487	0.02%	0.003%
69	10.214	2841	2853	2874	rBV	713355	1107739	48.94%	7.007%
70	10.423	2914	2918	2919	rBV2	475	313	0.01%	0.002%
71	10.509	2939	2945	2949	rBV2	405	428	0.02%	0.003%
72	10.847	3049	3050	3053	rVB2	661	331	0.01%	0.002%
73	10.921	3070	3073	3079	rVB3	618	606	0.03%	0.004%
74	11.191	3153	3157	3163	rVB3	587	631	0.03%	0.004%
75	11.246	3163	3174	3204	rBV	734590	1157999	51.16%	7.325%
76	11.442	3233	3235	3241	rVB2	484	395	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026996.D
 Acq On : 27 Jul 2022 14:03
 Operator : SY/MD
 Sample : VV0727WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.506	3250	3255	3256	rBV2	431	304	0.01%	0.002%
78	11.622	3278	3291	3312	rBV	908193	1439014	63.58%	9.103%
79	11.863	3363	3366	3370	rBV2	521	367	0.02%	0.002%
80	12.017	3411	3414	3417	rBV2	412	287	0.01%	0.002%
81	12.252	3480	3487	3488	rBV	1111	1160	0.05%	0.007%
82	12.657	3610	3613	3614	rBV2	478	287	0.01%	0.002%
83	12.808	3657	3660	3663	rBV3	432	294	0.01%	0.002%
84	12.902	3684	3689	3691	rBV2	507	456	0.02%	0.003%
85	12.988	3712	3716	3719	rBV3	396	374	0.02%	0.002%
86	13.049	3729	3735	3739	rBV3	559	590	0.03%	0.004%
87	13.172	3771	3773	3778	rVB2	707	452	0.02%	0.003%
88	13.284	3804	3808	3811	rVB2	531	400	0.02%	0.003%
89	13.342	3823	3826	3829	rVB	918	538	0.02%	0.003%
90	13.374	3829	3836	3839	rBV3	449	494	0.02%	0.003%
91	13.400	3839	3844	3845	rBV2	492	449	0.02%	0.003%
92	13.818	3971	3974	3978	rBV2	503	460	0.02%	0.003%
93	13.860	3980	3987	3990	rBV2	523	777	0.03%	0.005%
94	13.947	4012	4014	4019	rVB3	528	337	0.01%	0.002%
95	13.976	4020	4023	4025	rBV	527	306	0.01%	0.002%
96	14.728	4254	4257	4260	rBV3	819	602	0.03%	0.004%
97	15.172	4392	4395	4399	rBV4	824	684	0.03%	0.004%
98	15.236	4412	4415	4417	rBV2	760	431	0.02%	0.003%
99	15.316	4438	4440	4445	rBV4	764	606	0.03%	0.004%
100	15.393	4461	4464	4467	rBV2	1130	778	0.03%	0.005%




Sum of corrected areas: 15808079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026996.D
Acq On : 27 Jul 2022 14:03
Operator : SY/MD
Sample : VV0727WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

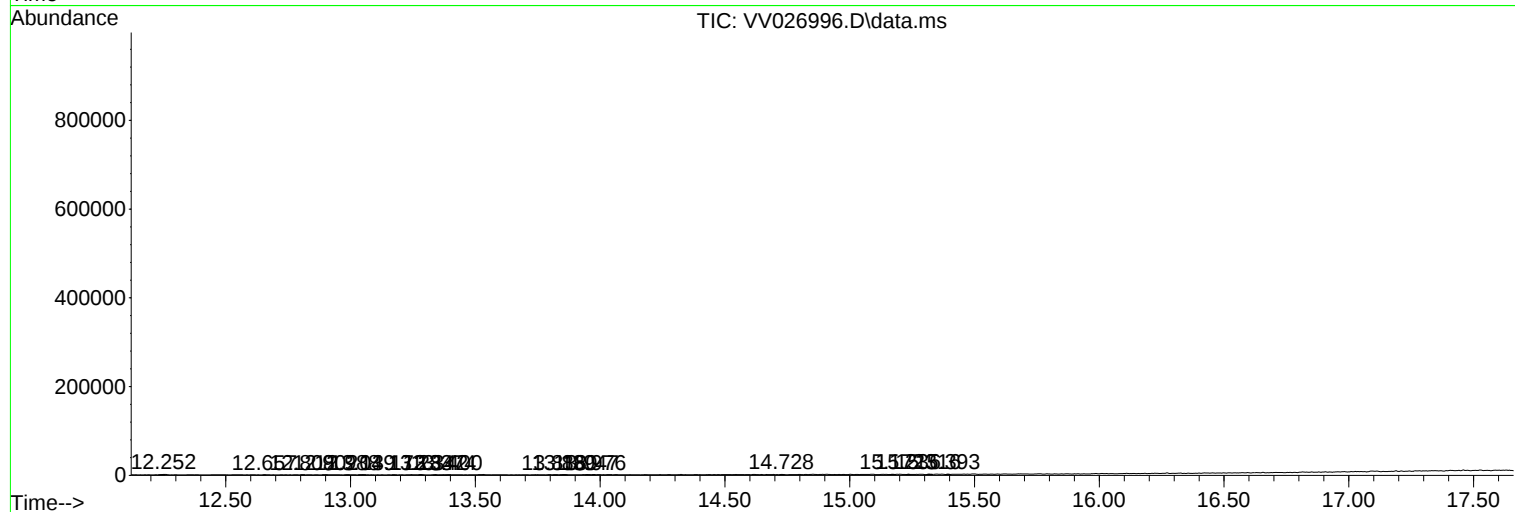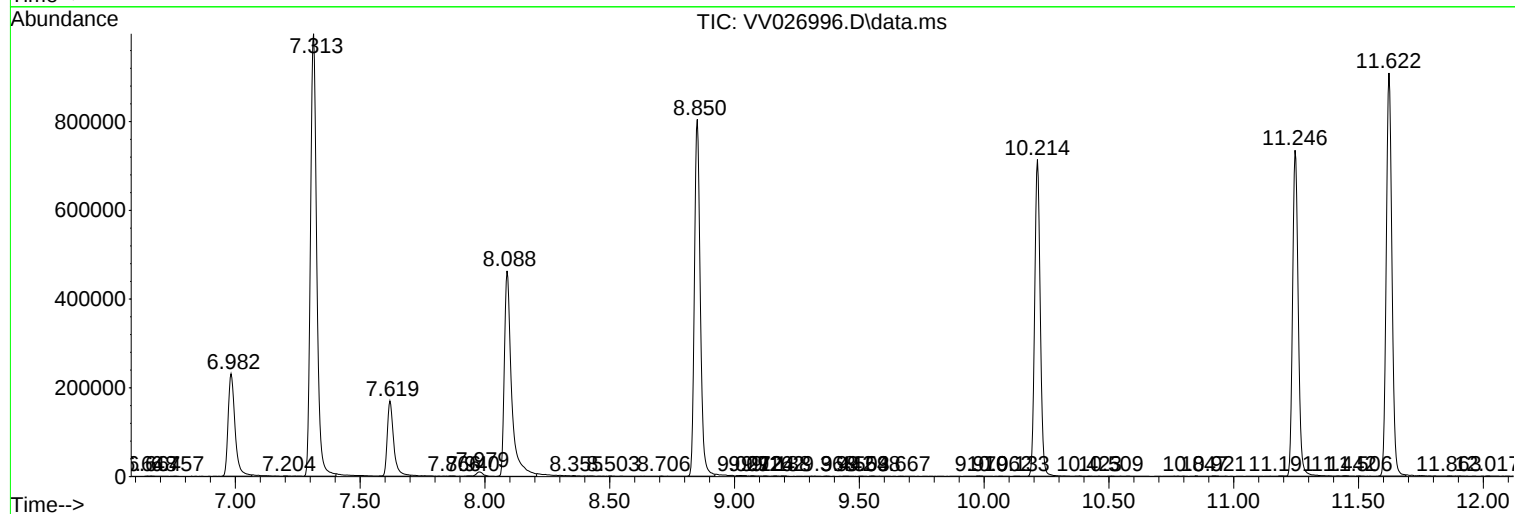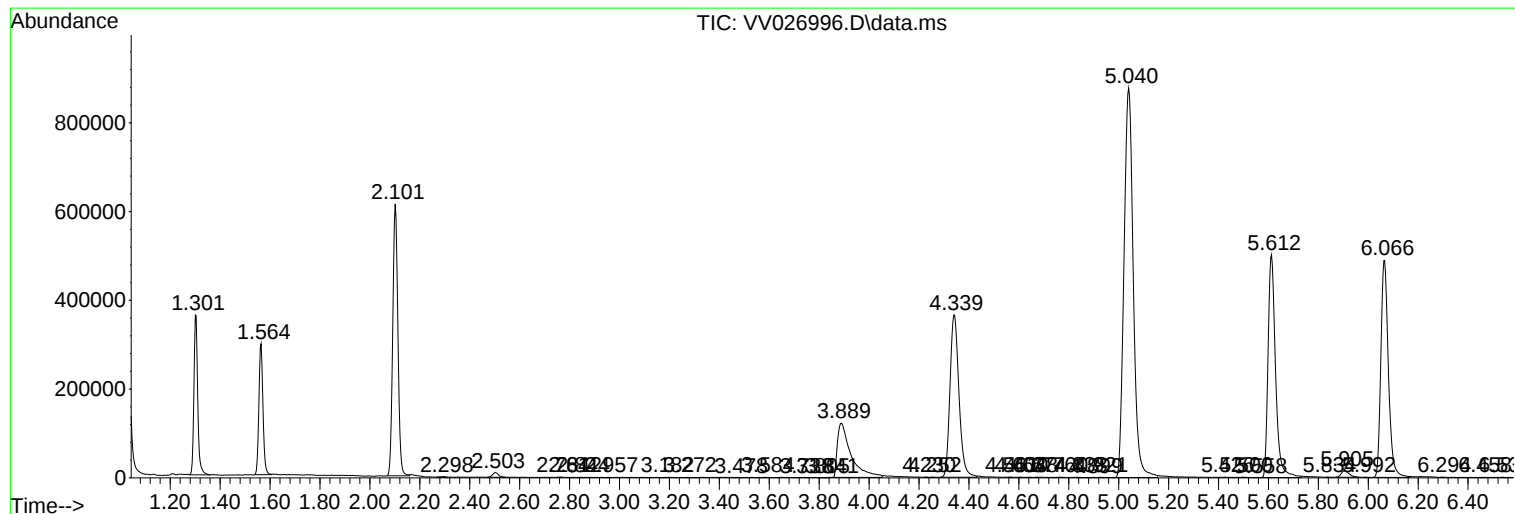

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026996.D
Acq On : 27 Jul 2022 14:03
Operator : SY/MD
Sample : VV0727WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026996.D
Acq On : 27 Jul 2022 14:03
Operator : SY/MD
Sample : VV0727WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------