

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026997.D
 Acq On : 27 Jul 2022 14:30
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV026997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	105	rVB	346724	371571	16.92%	2.382%
2	1.564	155	163	177	rBV	281327	323075	14.71%	2.071%
3	2.101	319	330	345	rBV	603467	854324	38.91%	5.477%
4	2.233	369	371	378	rVB3	733	594	0.03%	0.004%
5	2.413	425	427	433	rVB3	697	565	0.03%	0.004%
6	2.465	440	443	445	rBV2	428	312	0.01%	0.002%
7	2.503	445	455	467	rVB3	13270	22181	1.01%	0.142%
8	2.638	494	497	503	rBV3	323	331	0.02%	0.002%
9	2.696	512	515	519	rBV2	355	326	0.01%	0.002%
10	2.754	529	533	534	rBV2	507	344	0.02%	0.002%
11	2.802	546	548	556	rVB2	510	466	0.02%	0.003%
12	2.966	596	599	603	rBV2	431	366	0.02%	0.002%
13	3.188	663	668	671	rBV2	471	454	0.02%	0.003%
14	3.272	692	694	701	rVB2	345	289	0.01%	0.002%
15	3.349	714	718	724	rVB3	417	504	0.02%	0.003%
16	3.410	735	737	742	rVB2	341	328	0.01%	0.002%
17	3.519	768	771	775	rVV2	355	333	0.02%	0.002%
18	3.638	804	808	812	rBV5	359	321	0.01%	0.002%
19	3.690	819	824	833	rBV3	387	635	0.03%	0.004%
20	3.789	849	855	859	rBV3	290	383	0.02%	0.002%
21	3.886	875	885	931	rBV2	123313	442732	20.16%	2.838%
22	4.342	1007	1027	1061	rBV	354792	898395	40.92%	5.759%
23	4.584	1098	1102	1104	rBV3	587	467	0.02%	0.003%
24	4.815	1168	1174	1177	rBV4	357	458	0.02%	0.003%
25	5.040	1227	1244	1281	rBV2	857433	2195586	100.00%	14.075%
26	5.346	1337	1339	1343	rVV3	588	467	0.02%	0.003%
27	5.439	1366	1368	1372	rVB3	551	323	0.01%	0.002%
28	5.477	1377	1380	1381	rBV3	633	411	0.02%	0.003%
29	5.535	1394	1398	1401	rBV4	399	293	0.01%	0.002%
30	5.613	1409	1422	1462	rBV	523366	1084225	49.38%	6.951%
31	5.844	1492	1494	1499	rBV5	542	428	0.02%	0.003%
32	5.905	1502	1513	1529	rBV4	15085	34060	1.55%	0.218%
33	6.014	1543	1547	1549	rBV3	535	413	0.02%	0.003%
34	6.066	1549	1563	1597	rBV	480549	992833	45.22%	6.365%
35	6.297	1633	1635	1638	rVB3	691	375	0.02%	0.002%
36	6.317	1638	1641	1646	rVB3	744	687	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026997.D
 Acq On : 27 Jul 2022 14:30
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.339	1646	1648	1650	rBV2	592	359	0.02%	0.002%
38	6.407	1667	1669	1673	rBV3	412	314	0.01%	0.002%
39	6.442	1678	1680	1686	rVB4	343	304	0.01%	0.002%
40	6.722	1762	1767	1769	rBV2	516	416	0.02%	0.003%
41	6.735	1769	1771	1778	rVB2	406	364	0.02%	0.002%
42	6.815	1790	1796	1802	rBV4	549	669	0.03%	0.004%
43	6.854	1802	1808	1813	rVB3	399	594	0.03%	0.004%
44	6.883	1813	1817	1821	rBV2	321	296	0.01%	0.002%
45	6.982	1837	1848	1875	rBV	223267	424150	19.32%	2.719%
46	7.201	1914	1916	1920	rVB4	445	339	0.02%	0.002%
47	7.239	1925	1928	1929	rBV3	735	368	0.02%	0.002%
48	7.313	1937	1951	1992	rBV	957248	1686413	76.81%	10.811%
49	7.535	2018	2020	2024	rVB3	902	514	0.02%	0.003%
50	7.619	2036	2046	2074	rBV	160045	290694	13.24%	1.864%
51	7.818	2106	2108	2112	rVB5	538	390	0.02%	0.003%
52	7.931	2140	2143	2146	rBV3	545	360	0.02%	0.002%
53	7.976	2148	2157	2169	rVB2	9710	16680	0.76%	0.107%
54	8.088	2180	2192	2226	rBV	451244	900325	41.01%	5.772%
55	8.368	2277	2279	2282	rVB4	541	313	0.01%	0.002%
56	8.484	2312	2315	2323	rVB5	685	839	0.04%	0.005%
57	8.609	2352	2354	2358	rBV3	737	335	0.02%	0.002%
58	8.741	2391	2395	2402	rBV3	497	562	0.03%	0.004%
59	8.773	2402	2405	2407	rBV2	457	384	0.02%	0.002%
60	8.850	2417	2429	2457	rBV	828853	1361314	62.00%	8.727%
61	9.130	2512	2516	2519	rBV4	590	373	0.02%	0.002%
62	9.149	2519	2522	2524	rBV3	460	311	0.01%	0.002%
63	9.259	2554	2556	2559	rBV2	431	304	0.01%	0.002%
64	9.378	2589	2593	2597	rVB3	425	357	0.02%	0.002%
65	9.503	2629	2632	2636	rVB2	443	309	0.01%	0.002%
66	9.667	2679	2683	2691	rBV3	405	551	0.03%	0.004%
67	9.931	2760	2765	2769	rBV3	316	356	0.02%	0.002%
68	10.040	2794	2799	2801	rBV2	390	320	0.01%	0.002%
69	10.075	2806	2810	2813	rBV2	356	291	0.01%	0.002%
70	10.214	2839	2853	2880	rBV	695600	1083307	49.34%	6.945%
71	10.545	2951	2956	2964	rVB4	649	873	0.04%	0.006%
72	10.583	2964	2968	2974	rBV3	314	374	0.02%	0.002%
73	10.931	3072	3076	3080	rVB2	721	588	0.03%	0.004%
74	11.050	3109	3113	3116	rBV	294	283	0.01%	0.002%
75	11.194	3152	3158	3161	rBV3	812	763	0.03%	0.005%
76	11.246	3163	3174	3194	rBV	763354	1187855	54.10%	7.615%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV026997.D
 Acq On : 27 Jul 2022 14:30
 Operator : SY/MD
 Sample : N3766-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3313	rBV	886002	1394330	63.51%	8.939%
78	11.998	3404	3408	3412	rBV3	304	336	0.02%	0.002%
79	12.426	3537	3541	3545	rBV	387	371	0.02%	0.002%
80	12.535	3572	3575	3580	rVB2	482	355	0.02%	0.002%
81	12.574	3584	3587	3590	rVV3	581	406	0.02%	0.003%
82	12.609	3594	3598	3603	rVB2	580	554	0.03%	0.004%
83	12.635	3603	3606	3609	rBV2	489	288	0.01%	0.002%
84	12.654	3609	3612	3617	rBV3	942	794	0.04%	0.005%
85	12.960	3705	3707	3713	rVB3	503	361	0.02%	0.002%
86	13.233	3784	3792	3797	rBV3	529	863	0.04%	0.006%
87	13.513	3874	3879	3881	rBV4	589	480	0.02%	0.003%
88	13.535	3883	3886	3891	rVB2	574	536	0.02%	0.003%
89	13.702	3935	3938	3940	rBV2	435	313	0.01%	0.002%
90	13.972	4019	4022	4025	rBV3	433	337	0.02%	0.002%
91	14.088	4054	4058	4060	rBV3	586	398	0.02%	0.003%
92	14.271	4112	4115	4117	rBV2	514	390	0.02%	0.003%
93	14.342	4135	4137	4142	rVB4	480	364	0.02%	0.002%
94	14.435	4163	4166	4170	rBV3	672	412	0.02%	0.003%
95	14.519	4190	4192	4196	rVB3	481	297	0.01%	0.002%
96	14.644	4227	4231	4233	rBV3	591	493	0.02%	0.003%
97	14.876	4299	4303	4308	rVB4	692	745	0.03%	0.005%
98	14.914	4310	4315	4316	rBV	570	477	0.02%	0.003%
99	14.976	4331	4334	4335	rBV2	491	297	0.01%	0.002%
100	15.217	4406	4409	4412	rBV2	752	504	0.02%	0.003%




Sum of corrected areas: 15599067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026997.D
Acq On : 27 Jul 2022 14:30
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

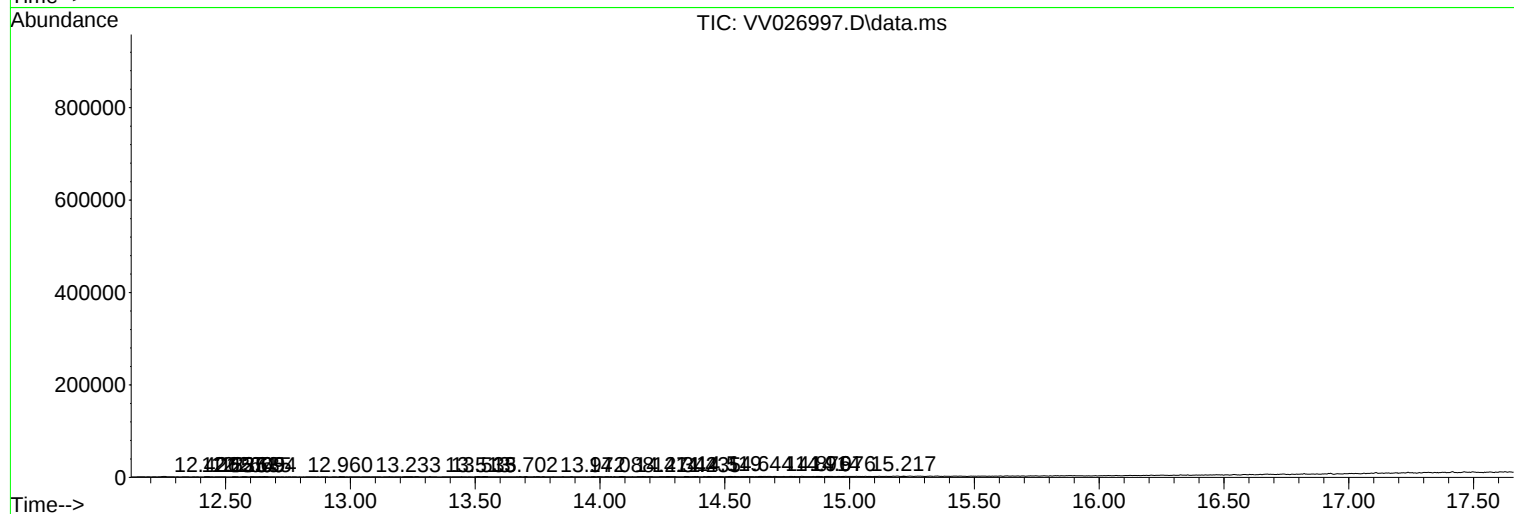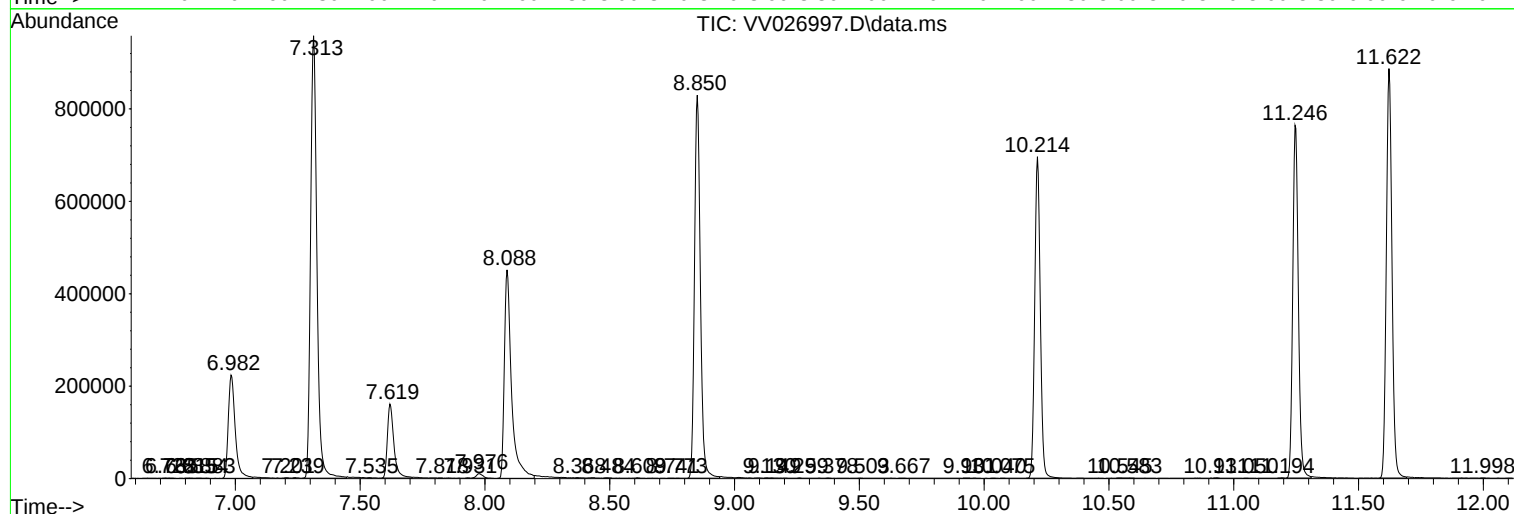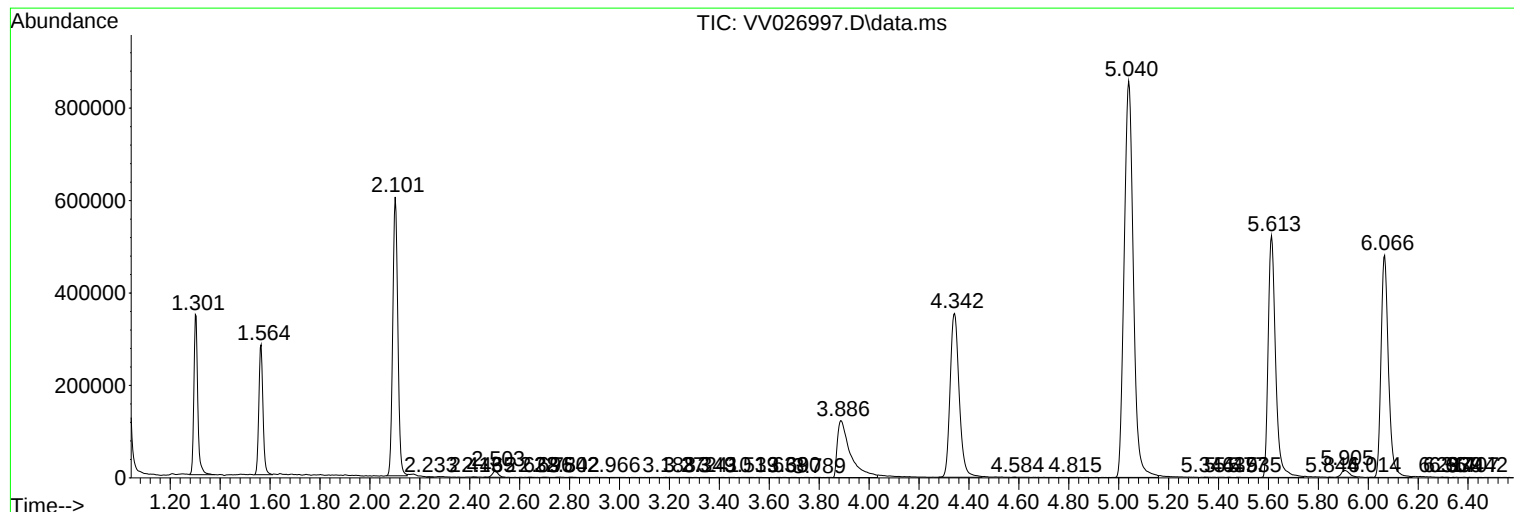

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026997.D
Acq On : 27 Jul 2022 14:30
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026997.D
Acq On : 27 Jul 2022 14:30
Operator : SY/MD
Sample : N3766-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc