

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027006.D
 Acq On : 27 Jul 2022 18:12
 Operator : SY/MD
 Sample : N3880-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV027006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	230108	243233	11.41%	1.364%
2	1.564	156	163	176	rBV	227832	258846	12.14%	1.451%
3	2.101	321	330	347	rBV	445980	630236	29.56%	3.534%
4	2.503	448	455	467	rVB2	13946	22279	1.04%	0.125%
5	3.095	636	639	641	rBV	269	169	0.01%	0.001%
6	3.105	641	642	646	rVB2	392	219	0.01%	0.001%
7	3.159	658	659	660	rBV	351	98	0.00%	0.001%
8	3.297	699	702	704	rBV2	329	237	0.01%	0.001%
9	3.381	723	728	730	rBV2	540	436	0.02%	0.002%
10	3.404	730	735	739	rVV2	352	434	0.02%	0.002%
11	3.513	766	769	771	rBV	246	175	0.01%	0.001%
12	3.648	807	811	815	rBV	258	286	0.01%	0.002%
13	3.732	834	837	838	rBV	156	77	0.00%	0.000%
14	3.834	867	869	871	rBV2	271	134	0.01%	0.001%
15	3.892	874	887	922	rBV3	207286	756508	35.48%	4.242%
16	4.342	1012	1027	1068	rVB	350998	876250	41.10%	4.913%
17	4.603	1104	1108	1111	rBV3	577	480	0.02%	0.003%
18	4.683	1126	1133	1137	rBV5	765	1069	0.05%	0.006%
19	4.748	1150	1153	1154	rBV3	372	176	0.01%	0.001%
20	4.850	1184	1185	1189	rBV2	370	168	0.01%	0.001%
21	4.905	1198	1202	1205	rBV3	519	508	0.02%	0.003%
22	5.040	1228	1244	1280	rBV2	825406	2132054	100.00%	11.954%
23	5.413	1358	1360	1362	rBV	518	161	0.01%	0.001%
24	5.445	1369	1370	1372	rVB2	351	90	0.00%	0.001%
25	5.461	1372	1375	1377	rVB2	298	162	0.01%	0.001%
26	5.477	1377	1380	1381	rBV	541	255	0.01%	0.001%
27	5.500	1385	1387	1389	rBV3	284	143	0.01%	0.001%
28	5.516	1389	1392	1394	rBV2	412	265	0.01%	0.001%
29	5.571	1408	1409	1410	rVB	351	68	0.00%	0.000%
30	5.612	1410	1422	1458	rBV	555317	1142011	53.56%	6.403%
31	5.911	1503	1515	1539	rBV4	120759	266851	12.52%	1.496%
32	6.066	1550	1563	1590	rBV	486772	998463	46.83%	5.598%
33	6.410	1667	1670	1671	rBV	600	370	0.02%	0.002%
34	6.468	1682	1688	1692	rBV4	806	715	0.03%	0.004%
35	6.490	1693	1695	1700	rBV3	666	587	0.03%	0.003%
36	6.538	1707	1710	1712	rBV2	464	336	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027006.D
 Acq On : 27 Jul 2022 18:12
 Operator : SY/MD
 Sample : N3880-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.567	1717	1719	1720	rBV	363	109	0.01%	0.001%
38	6.632	1732	1739	1740	rBV3	2484	2526	0.12%	0.014%
39	6.899	1816	1822	1824	rBV2	364	332	0.02%	0.002%
40	6.985	1837	1849	1880	rBV	220605	419209	19.66%	2.350%
41	7.313	1939	1951	1984	rBV	877393	1555334	72.95%	8.720%
42	7.619	2037	2046	2068	rBV	156556	277006	12.99%	1.553%
43	7.972	2143	2156	2178	rBV	1005672	1679601	78.78%	9.417%
44	8.088	2182	2192	2226	rBV	645480	1213983	56.94%	6.807%
45	8.850	2415	2429	2458	rBV	856902	1412225	66.24%	7.918%
46	9.265	2555	2558	2559	rBV2	276	171	0.01%	0.001%
47	9.378	2590	2593	2598	rBV4	319	333	0.02%	0.002%
48	9.419	2603	2606	2608	rBV	280	220	0.01%	0.001%
49	9.455	2615	2617	2620	rBV2	296	168	0.01%	0.001%
50	9.673	2682	2685	2686	rBV	466	277	0.01%	0.002%
51	9.744	2702	2707	2708	rBV2	459	310	0.01%	0.002%
52	9.776	2714	2717	2721	rBV	327	266	0.01%	0.001%
53	9.834	2732	2735	2737	rBV2	257	144	0.01%	0.001%
54	9.866	2742	2745	2749	rVV2	413	281	0.01%	0.002%
55	9.940	2763	2768	2776	rVB4	881	1109	0.05%	0.006%
56	10.088	2810	2814	2816	rBV	247	234	0.01%	0.001%
57	10.124	2822	2825	2827	rBV2	536	248	0.01%	0.001%
58	10.140	2827	2830	2831	rBV	319	184	0.01%	0.001%
59	10.214	2841	2853	2875	rBV	768500	1196450	56.12%	6.708%
60	10.587	2967	2969	2973	rVB3	701	395	0.02%	0.002%
61	10.641	2985	2986	2987	rBV	331	100	0.00%	0.001%
62	10.683	2997	2999	3003	rVB3	313	221	0.01%	0.001%
63	10.712	3003	3008	3012	rBV2	450	465	0.02%	0.003%
64	10.731	3012	3014	3020	rBV2	336	330	0.02%	0.002%
65	10.821	3040	3042	3043	rBV	210	80	0.00%	0.000%
66	10.905	3065	3068	3070	rBV2	473	272	0.01%	0.002%
67	11.040	3107	3110	3113	rBV2	236	152	0.01%	0.001%
68	11.146	3139	3143	3146	rBV2	468	425	0.02%	0.002%
69	11.181	3150	3154	3156	rBV3	594	435	0.02%	0.002%
70	11.249	3163	3175	3203	rBV	821108	1269597	59.55%	7.118%
71	11.622	3278	3291	3319	rBV	916754	1430192	67.08%	8.019%
72	12.580	3587	3589	3590	rBV	359	164	0.01%	0.001%
73	12.757	3642	3644	3646	rBV	324	148	0.01%	0.001%
74	13.133	3757	3761	3762	rBV2	563	447	0.02%	0.003%
75	13.275	3799	3805	3808	rBV4	915	1090	0.05%	0.006%
76	13.506	3869	3877	3892	rVB	21475	35136	1.65%	0.197%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027006.D
Acq On : 27 Jul 2022 18:12
Operator : SY/MD
Sample : N3880-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis

77	14.011	4032	4034	4038	rbV3	685	478	0.02%	0.003%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 17835396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027006.D
Acq On : 27 Jul 2022 18:12
Operator : SY/MD
Sample : N3880-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

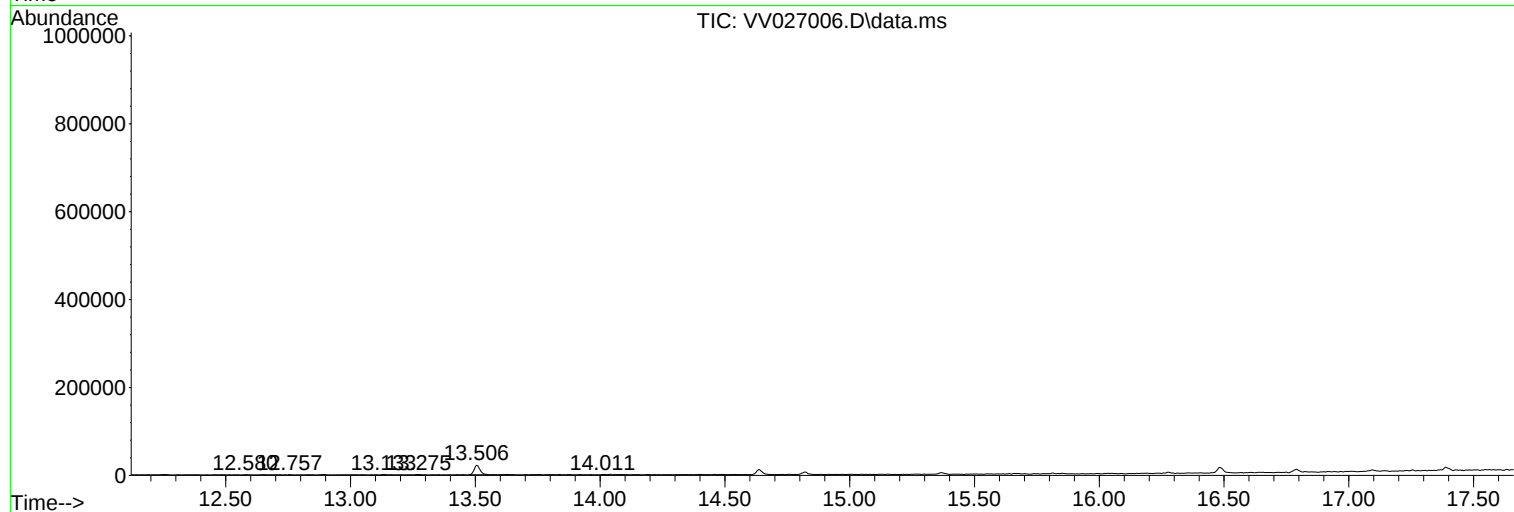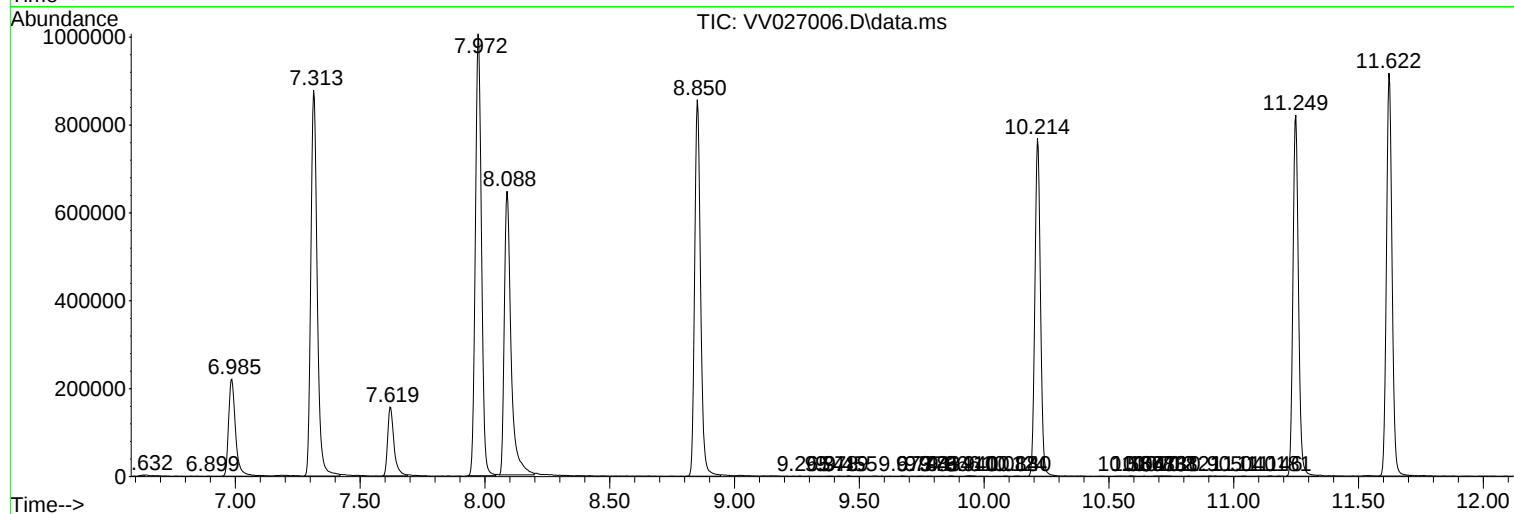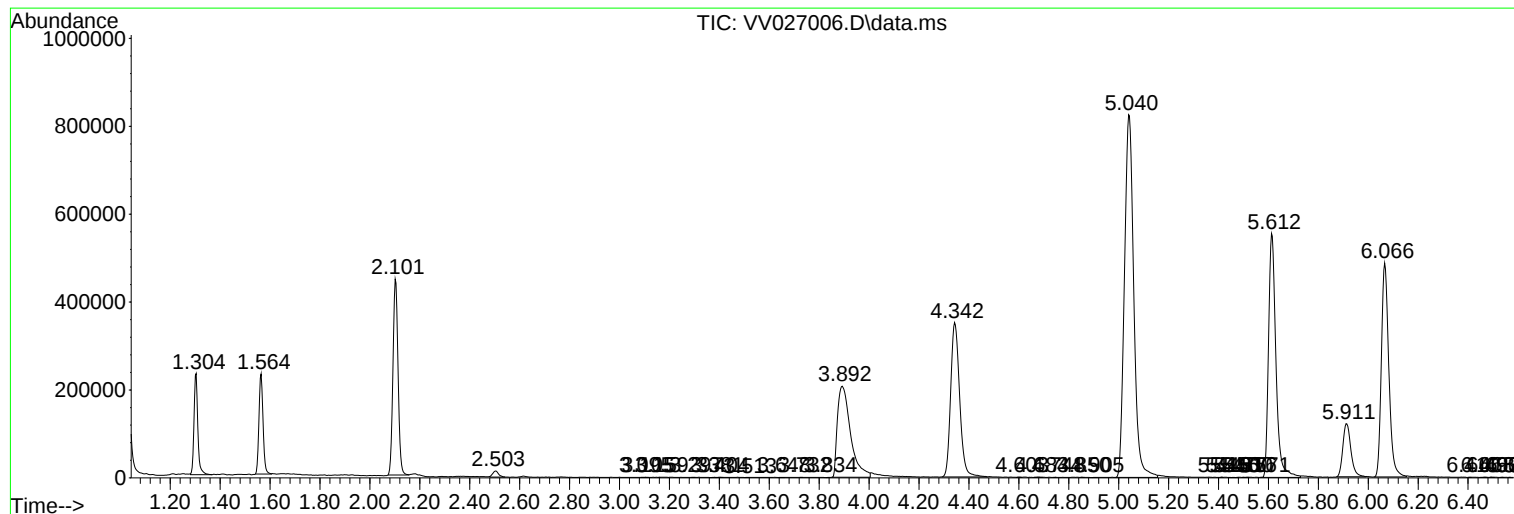

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027006.D
Acq On : 27 Jul 2022 18:12
Operator : SY/MD
Sample : N3880-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027006.D
Acq On : 27 Jul 2022 18:12
Operator : SY/MD
Sample : N3880-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------