

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027007.D
 Acq On : 27 Jul 2022 18:36
 Operator : SY/MD
 Sample : N3880-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	225315	244731	11.50%	1.489%
2	1.565	155	163	178	rBV	226250	259831	12.21%	1.581%
3	2.101	320	330	346	rBV	446779	638581	30.00%	3.885%
4	2.503	445	455	463	rBV2	11576	17830	0.84%	0.108%
5	2.564	470	474	475	rBV	440	281	0.01%	0.002%
6	2.732	522	526	529	rBV2	367	341	0.02%	0.002%
7	2.757	529	534	535	rBV2	831	529	0.02%	0.003%
8	2.973	597	601	604	rVB2	542	426	0.02%	0.003%
9	3.185	663	667	673	rVB2	655	897	0.04%	0.005%
10	3.314	703	707	710	rVB	399	299	0.01%	0.002%
11	3.452	746	750	755	rVB3	391	346	0.02%	0.002%
12	3.490	758	762	766	rVV2	307	302	0.01%	0.002%
13	3.532	772	775	779	rBV3	364	268	0.01%	0.002%
14	3.619	796	802	804	rBV2	397	365	0.02%	0.002%
15	3.754	840	844	847	rBV	425	293	0.01%	0.002%
16	3.886	874	885	935	rBV	185806	644717	30.29%	3.922%
17	4.343	1011	1027	1058	rBV	358532	885910	41.62%	5.390%
18	4.616	1110	1112	1115	rBV3	526	377	0.02%	0.002%
19	4.703	1137	1139	1141	rVB2	689	302	0.01%	0.002%
20	4.863	1187	1189	1192	rVB3	492	270	0.01%	0.002%
21	5.040	1227	1244	1280	rBV2	820290	2128555	100.00%	12.950%
22	5.330	1331	1334	1338	rBV4	783	473	0.02%	0.003%
23	5.423	1359	1363	1367	rVB4	432	416	0.02%	0.003%
24	5.500	1382	1387	1392	rBV4	371	436	0.02%	0.003%
25	5.526	1392	1395	1402	rVB4	442	435	0.02%	0.003%
26	5.613	1410	1422	1459	rBV	541584	1116447	52.45%	6.793%
27	5.905	1501	1513	1534	rBV5	20453	46726	2.20%	0.284%
28	6.066	1545	1563	1600	rBV	488553	1016441	47.75%	6.184%
29	6.336	1644	1647	1650	rBV2	560	358	0.02%	0.002%
30	6.352	1650	1652	1657	rBV3	438	375	0.02%	0.002%
31	6.384	1657	1662	1670	rVB6	830	1018	0.05%	0.006%
32	6.426	1670	1675	1676	rBV3	770	642	0.03%	0.004%
33	6.487	1691	1694	1697	rBV3	451	343	0.02%	0.002%
34	6.503	1697	1699	1703	rVV5	418	264	0.01%	0.002%
35	6.587	1723	1725	1728	rVB3	553	331	0.02%	0.002%
36	6.638	1728	1741	1746	rBV6	2249	4851	0.23%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027007.D
 Acq On : 27 Jul 2022 18:36
 Operator : SY/MD
 Sample : N3880-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.867	1809	1812	1815	rVB3	432	284	0.01%	0.002%
38	6.879	1815	1816	1822	rVB	422	326	0.02%	0.002%
39	6.912	1822	1826	1828	rBV2	538	449	0.02%	0.003%
40	6.986	1832	1849	1873	rBV	220318	415197	19.51%	2.526%
41	7.313	1939	1951	1986	rBV	867734	1553275	72.97%	9.450%
42	7.619	2036	2046	2076	rBV	154926	279619	13.14%	1.701%
43	7.931	2137	2143	2144	rBV3	669	555	0.03%	0.003%
44	7.973	2144	2156	2181	rBV	421106	711813	33.44%	4.331%
45	8.088	2182	2192	2223	rBV	625533	1186242	55.73%	7.217%
46	8.410	2289	2292	2293	rBV2	1242	684	0.03%	0.004%
47	8.590	2347	2348	2353	rVB4	526	275	0.01%	0.002%
48	8.677	2370	2375	2377	rBV2	363	338	0.02%	0.002%
49	8.850	2416	2429	2467	rBV	835543	1377739	64.73%	8.382%
50	9.092	2501	2504	2508	rVB3	624	400	0.02%	0.002%
51	9.111	2508	2510	2513	rBV2	367	275	0.01%	0.002%
52	9.146	2518	2521	2522	rBV	648	350	0.02%	0.002%
53	9.214	2536	2542	2543	rBV2	458	371	0.02%	0.002%
54	9.329	2575	2578	2582	rBV3	384	301	0.01%	0.002%
55	9.358	2585	2587	2596	rVB3	654	683	0.03%	0.004%
56	9.407	2598	2602	2605	rBV3	353	323	0.02%	0.002%
57	9.477	2619	2624	2627	rBV3	324	278	0.01%	0.002%
58	9.497	2627	2630	2637	rVB2	501	537	0.03%	0.003%
59	9.548	2643	2646	2648	rBV3	459	271	0.01%	0.002%
60	9.561	2648	2650	2655	rVB3	616	486	0.02%	0.003%
61	9.583	2655	2657	2661	rBV3	614	449	0.02%	0.003%
62	9.606	2661	2664	2667	rVV3	463	310	0.01%	0.002%
63	9.677	2680	2686	2687	rBV2	337	287	0.01%	0.002%
64	9.731	2698	2703	2705	rBV2	386	320	0.02%	0.002%
65	9.747	2705	2708	2713	rVB3	455	338	0.02%	0.002%
66	10.214	2841	2853	2879	rBV	759917	1194358	56.11%	7.267%
67	10.484	2933	2937	2942	rBV2	439	439	0.02%	0.003%
68	10.548	2952	2957	2962	rVB3	704	713	0.03%	0.004%
69	10.580	2963	2967	2970	rVB4	680	492	0.02%	0.003%
70	10.619	2976	2979	2982	rBV2	276	271	0.01%	0.002%
71	10.918	3067	3072	3073	rBV	409	327	0.02%	0.002%
72	10.992	3091	3095	3099	rVB2	376	383	0.02%	0.002%
73	11.191	3152	3157	3160	rBV2	669	701	0.03%	0.004%
74	11.249	3163	3175	3206	rBV	797577	1222714	57.44%	7.439%
75	11.535	3259	3264	3265	rBV3	901	803	0.04%	0.005%
76	11.622	3279	3291	3310	rBV	892407	1419906	66.71%	8.639%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027007.D
 Acq On : 27 Jul 2022 18:36
 Operator : SY/MD
 Sample : N3880-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.911	3374	3381	3384	rVB2	555	533	0.03%	0.003%
78	11.963	3394	3397	3402	rVB3	443	426	0.02%	0.003%
79	11.995	3402	3407	3411	rBV4	523	600	0.03%	0.004%
80	12.021	3413	3415	3420	rVB	558	402	0.02%	0.002%
81	12.043	3420	3422	3426	rBV2	382	291	0.01%	0.002%
82	12.255	3478	3488	3495	rBV4	1303	2351	0.11%	0.014%
83	12.300	3495	3502	3507	rVV3	373	464	0.02%	0.003%
84	12.493	3560	3562	3566	rBV4	351	263	0.01%	0.002%
85	12.641	3604	3608	3610	rBV2	687	581	0.03%	0.004%
86	12.654	3610	3612	3617	rVB	777	574	0.03%	0.003%
87	12.786	3649	3653	3655	rBV2	451	269	0.01%	0.002%
88	13.175	3772	3774	3778	rBV2	371	306	0.01%	0.002%
89	13.275	3799	3805	3808	rBV5	682	526	0.02%	0.003%
90	13.381	3835	3838	3841	rBV4	557	408	0.02%	0.002%
91	13.426	3849	3852	3857	rBV3	401	331	0.02%	0.002%
92	13.509	3869	3878	3891	rBV2	11276	18436	0.87%	0.112%
93	13.664	3924	3926	3930	rVB2	559	285	0.01%	0.002%
94	14.635	4222	4228	4242	rBV4	5295	8594	0.40%	0.052%
95	14.824	4280	4287	4295	rBV7	2418	3169	0.15%	0.019%
96	14.979	4332	4335	4336	rBV2	544	298	0.01%	0.002%
97	15.361	4450	4454	4455	rBV3	1538	1045	0.05%	0.006%
98	15.451	4480	4482	4484	rBV2	920	366	0.02%	0.002%
99	15.673	4548	4551	4553	rBV3	1006	548	0.03%	0.003%
100	17.027	4969	4972	4977	rVB	11923	6450	0.30%	0.039%




Sum of corrected areas: 16436405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027007.D
Acq On : 27 Jul 2022 18:36
Operator : SY/MD
Sample : N3880-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

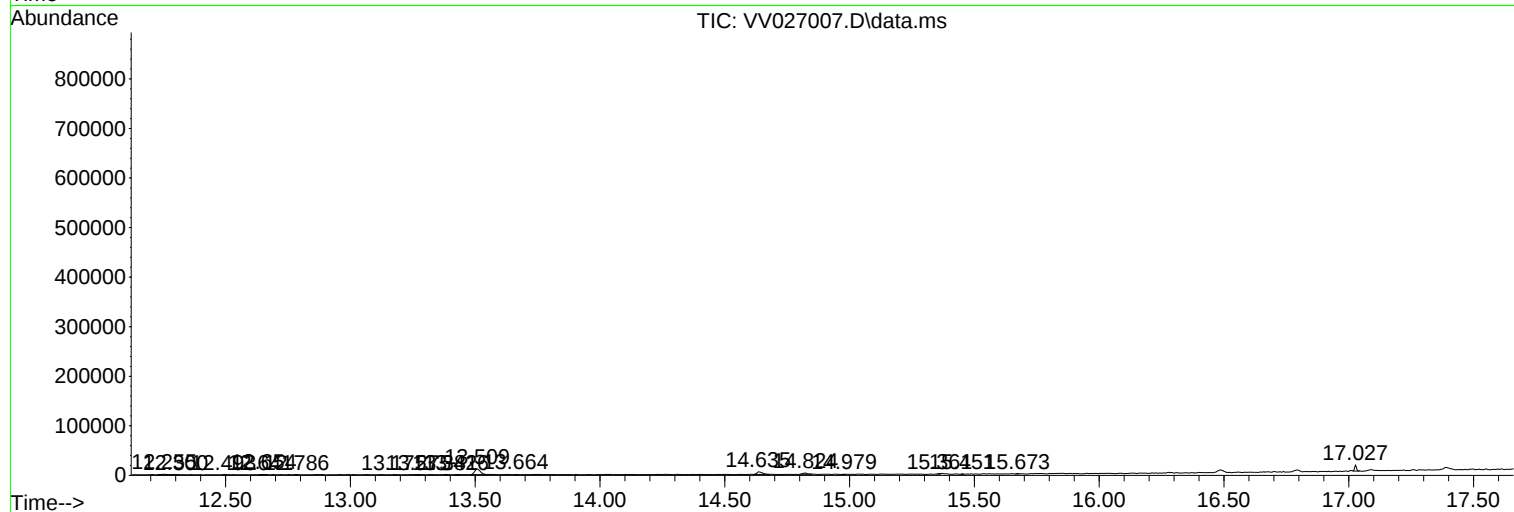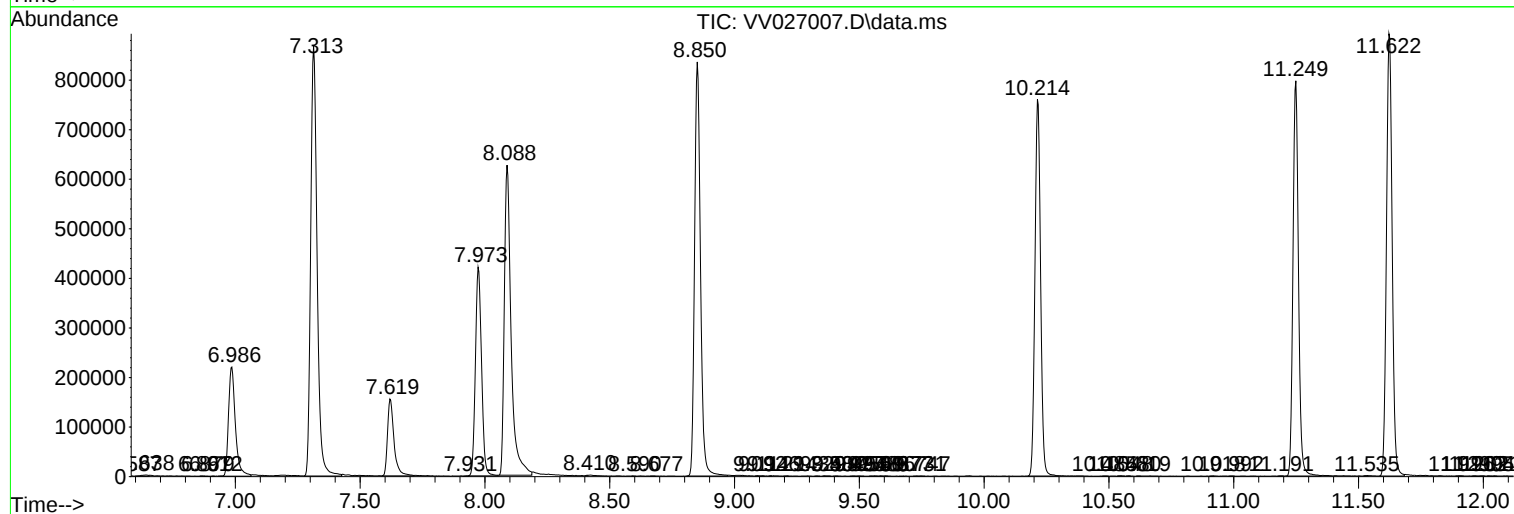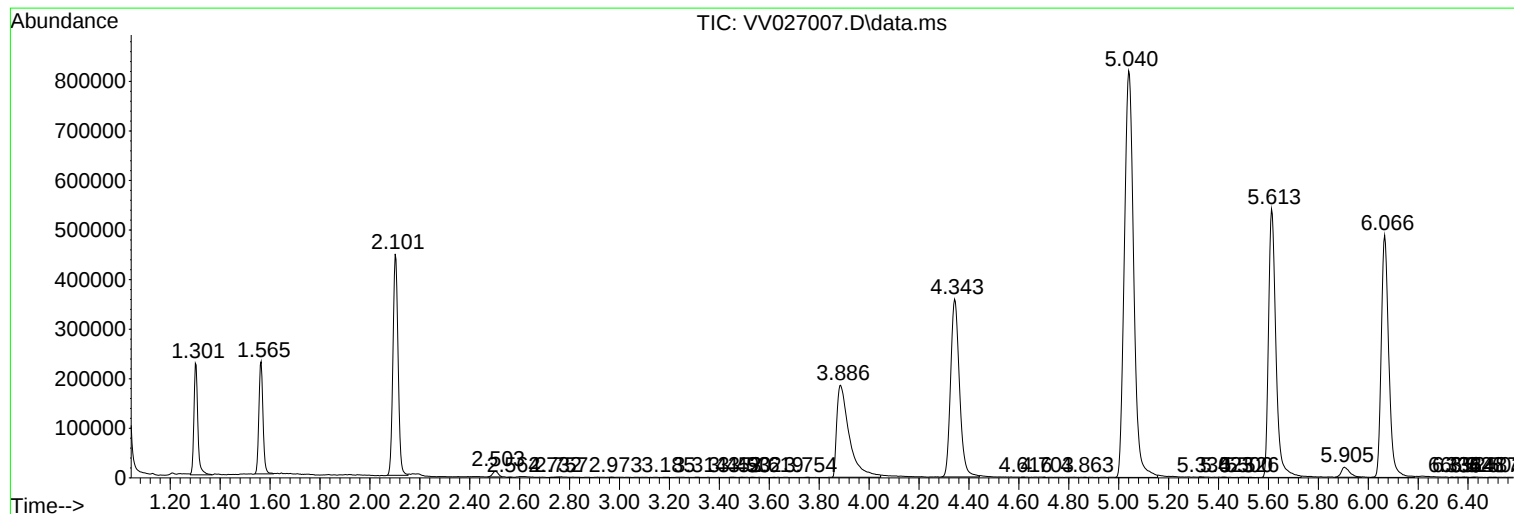

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027007.D
Acq On : 27 Jul 2022 18:36
Operator : SY/MD
Sample : N3880-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027007.D
Acq On : 27 Jul 2022 18:36
Operator : SY/MD
Sample : N3880-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------