

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027008.D
 Acq On : 27 Jul 2022 19:01
 Operator : SY/MD
 Sample : N3880-04DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	222383	235846	11.16%	1.437%
2	1.565	156	163	176	rVB	225499	255929	12.11%	1.559%
3	2.101	321	330	349	rVB	441961	627818	29.71%	3.825%
4	2.503	448	455	465	rVB2	11874	18012	0.85%	0.110%
5	2.793	543	545	546	rVB2	599	143	0.01%	0.001%
6	2.812	546	551	553	rBV	280	222	0.01%	0.001%
7	2.857	561	565	567	rBV	344	260	0.01%	0.002%
8	3.002	608	610	612	rBV2	286	116	0.01%	0.001%
9	3.175	662	664	672	rVB2	413	356	0.02%	0.002%
10	3.407	735	736	737	rBV	266	59	0.00%	0.000%
11	3.420	737	740	742	rVB2	296	171	0.01%	0.001%
12	3.529	772	774	776	rBV2	117	57	0.00%	0.000%
13	3.545	776	779	780	rBV2	174	74	0.00%	0.000%
14	3.667	810	817	820	rVB3	368	404	0.02%	0.002%
15	3.683	820	822	825	rVB2	194	99	0.00%	0.001%
16	3.699	825	827	829	rBV	97	39	0.00%	0.000%
17	3.712	829	831	835	rBV	183	123	0.01%	0.001%
18	3.744	835	841	843	rBV2	200	210	0.01%	0.001%
19	3.754	843	844	847	rBV2	235	132	0.01%	0.001%
20	3.812	860	862	863	rBV	162	66	0.00%	0.000%
21	3.886	874	885	926	rBV	175739	595340	28.17%	3.627%
22	4.343	1010	1027	1053	rBV	354788	883437	41.80%	5.382%
23	4.606	1107	1109	1112	rBV3	460	314	0.01%	0.002%
24	4.648	1119	1122	1127	rBV3	370	410	0.02%	0.002%
25	4.780	1159	1163	1166	rVB3	409	294	0.01%	0.002%
26	4.812	1166	1173	1174	rBV3	637	541	0.03%	0.003%
27	4.876	1190	1193	1196	rBV2	235	158	0.01%	0.001%
28	4.973	1220	1223	1225	rBV2	204	119	0.01%	0.001%
29	5.040	1228	1244	1292	rVV2	809861	2113248	100.00%	12.874%
30	5.474	1376	1379	1382	rBV4	457	296	0.01%	0.002%
31	5.555	1399	1404	1406	rVB2	432	346	0.02%	0.002%
32	5.568	1406	1408	1409	rBV2	163	58	0.00%	0.000%
33	5.613	1410	1422	1454	rBV	556116	1143150	54.09%	6.964%
34	5.908	1503	1514	1535	rVB6	19294	45167	2.14%	0.275%
35	6.066	1549	1563	1598	rBV	490445	1007876	47.69%	6.140%
36	6.375	1657	1659	1663	rBV2	421	291	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027008.D
 Acq On : 27 Jul 2022 19:01
 Operator : SY/MD
 Sample : N3880-04DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.452	1681	1683	1688	rVB	448	268	0.01%	0.002%
38	6.513	1700	1702	1704	rVB2	273	80	0.00%	0.000%
39	6.532	1707	1708	1713	rVB2	199	100	0.00%	0.001%
40	6.555	1713	1715	1720	rVB3	510	317	0.02%	0.002%
41	6.580	1720	1723	1724	rBV2	212	104	0.00%	0.001%
42	6.609	1728	1732	1733	rBV2	360	284	0.01%	0.002%
43	6.638	1734	1741	1747	rBV5	2383	3521	0.17%	0.021%
44	6.831	1798	1801	1802	rBV2	291	162	0.01%	0.001%
45	6.873	1811	1814	1818	rVB2	293	197	0.01%	0.001%
46	6.915	1823	1827	1832	rBV2	161	174	0.01%	0.001%
47	6.937	1832	1834	1837	rBV	181	91	0.00%	0.001%
48	6.986	1837	1849	1870	rBV	217926	408298	19.32%	2.487%
49	7.313	1938	1951	1979	rBV	870640	1537606	72.76%	9.367%
50	7.619	2036	2046	2071	rBV	151309	274295	12.98%	1.671%
51	7.857	2117	2120	2125	rVB5	755	605	0.03%	0.004%
52	7.905	2132	2135	2137	rBV3	469	302	0.01%	0.002%
53	7.973	2144	2156	2181	rBV	466596	785885	37.19%	4.788%
54	8.088	2182	2192	2230	rBV	615249	1183281	55.99%	7.209%
55	8.593	2346	2349	2351	rBV	373	293	0.01%	0.002%
56	8.625	2357	2359	2366	rVB3	466	395	0.02%	0.002%
57	8.677	2373	2375	2379	rVB4	347	233	0.01%	0.001%
58	8.699	2379	2382	2384	rBV	533	306	0.01%	0.002%
59	8.773	2402	2405	2406	rBV	188	99	0.00%	0.001%
60	8.799	2409	2413	2415	rBV3	836	407	0.02%	0.002%
61	8.850	2417	2429	2456	rBV	860610	1411816	66.81%	8.601%
62	9.120	2511	2513	2514	rBV	534	218	0.01%	0.001%
63	9.249	2549	2553	2554	rBV2	204	121	0.01%	0.001%
64	9.278	2560	2562	2566	rBV	321	215	0.01%	0.001%
65	9.310	2566	2572	2573	rBV	412	347	0.02%	0.002%
66	9.474	2621	2623	2625	rBV2	243	155	0.01%	0.001%
67	9.503	2630	2632	2635	rBV3	317	222	0.01%	0.001%
68	9.529	2637	2640	2641	rBV2	382	175	0.01%	0.001%
69	9.545	2642	2645	2654	rVB5	751	925	0.04%	0.006%
70	9.583	2654	2657	2659	rBV2	322	251	0.01%	0.002%
71	9.609	2663	2665	2668	rBV	202	130	0.01%	0.001%
72	9.645	2673	2676	2678	rVB2	356	168	0.01%	0.001%
73	9.683	2686	2688	2690	rBV2	154	76	0.00%	0.000%
74	9.719	2696	2699	2700	rBV	232	115	0.01%	0.001%
75	9.760	2708	2712	2714	rBV	400	257	0.01%	0.002%
76	9.866	2741	2745	2750	rVB3	499	557	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027008.D
 Acq On : 27 Jul 2022 19:01
 Operator : SY/MD
 Sample : N3880-04DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.895	2750	2754	2757	rBV2	409	381	0.02%	0.002%
78	9.915	2757	2760	2761	rBV	435	253	0.01%	0.002%
79	9.995	2783	2785	2789	rBV2	225	122	0.01%	0.001%
80	10.034	2792	2797	2798	rBV3	301	187	0.01%	0.001%
81	10.043	2798	2800	2804	rVB	217	115	0.01%	0.001%
82	10.063	2804	2806	2810	rBV2	299	164	0.01%	0.001%
83	10.214	2841	2853	2877	rBV	764022	1188858	56.26%	7.242%
84	10.583	2964	2968	2972	rVB2	840	567	0.03%	0.003%
85	10.686	2997	3000	3002	rBV2	333	220	0.01%	0.001%
86	10.767	3021	3025	3028	rBV	574	447	0.02%	0.003%
87	10.799	3033	3035	3036	rBV	229	68	0.00%	0.000%
88	10.870	3053	3057	3058	rBV	310	206	0.01%	0.001%
89	10.924	3072	3074	3079	rVB2	602	316	0.01%	0.002%
90	11.024	3102	3105	3110	rVB	582	447	0.02%	0.003%
91	11.056	3110	3115	3118	rBV2	454	535	0.03%	0.003%
92	11.091	3124	3126	3128	rBV	302	134	0.01%	0.001%
93	11.149	3142	3144	3146	rBV	186	73	0.00%	0.000%
94	11.249	3163	3175	3200	rBV	812096	1260162	59.63%	7.677%
95	11.622	3279	3291	3314	rBV	898558	1405359	66.50%	8.561%
96	12.239	3480	3483	3485	rBV2	728	537	0.03%	0.003%
97	12.763	3644	3646	3648	rBV2	418	160	0.01%	0.001%
98	13.278	3803	3806	3811	rBV3	737	646	0.03%	0.004%
99	13.506	3872	3877	3890	rVB2	6601	10350	0.49%	0.063%
100	13.677	3927	3930	3933	rBV4	643	531	0.03%	0.003%




Sum of corrected areas: 16415070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027008.D
Acq On : 27 Jul 2022 19:01
Operator : SY/MD
Sample : N3880-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

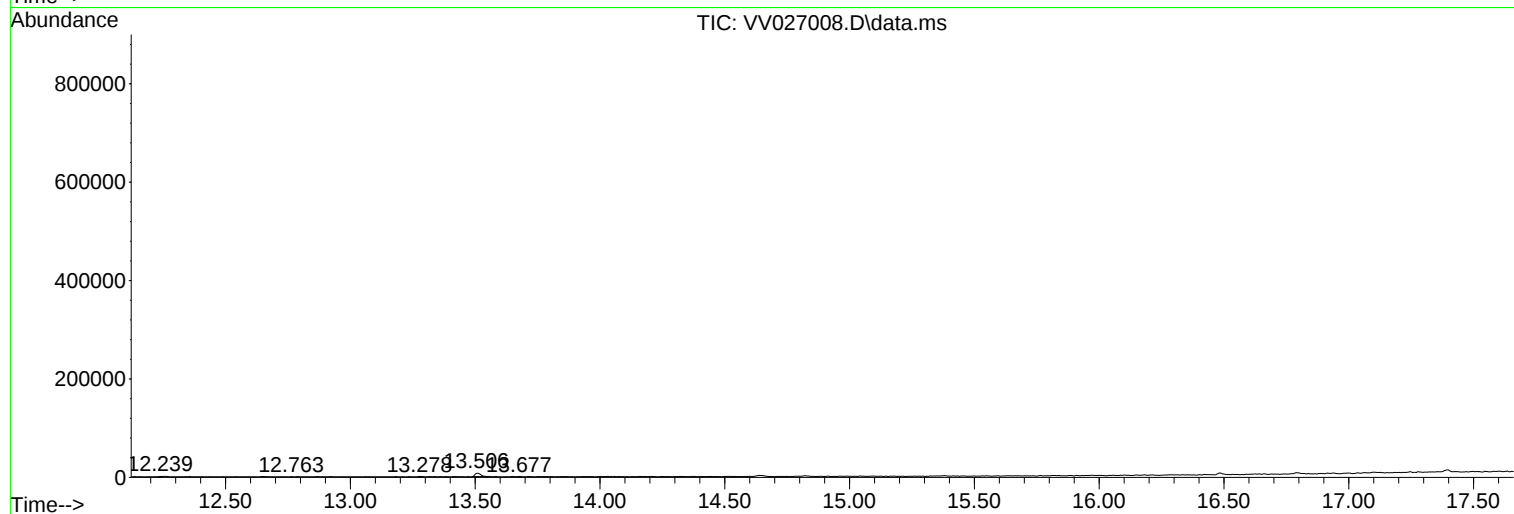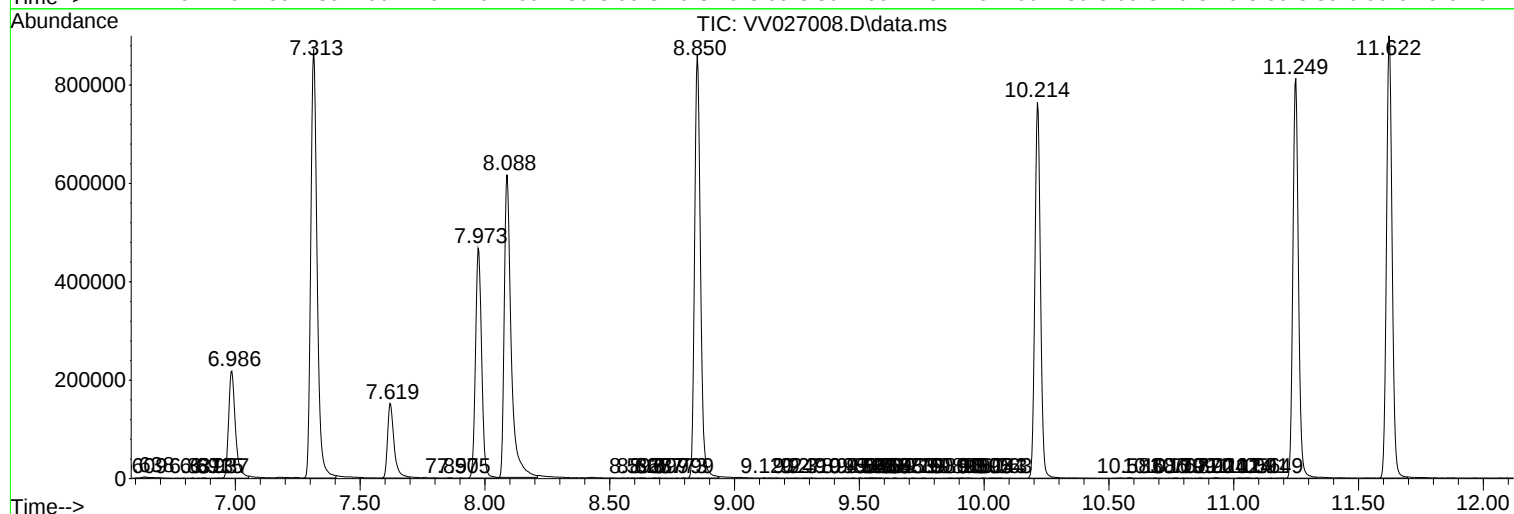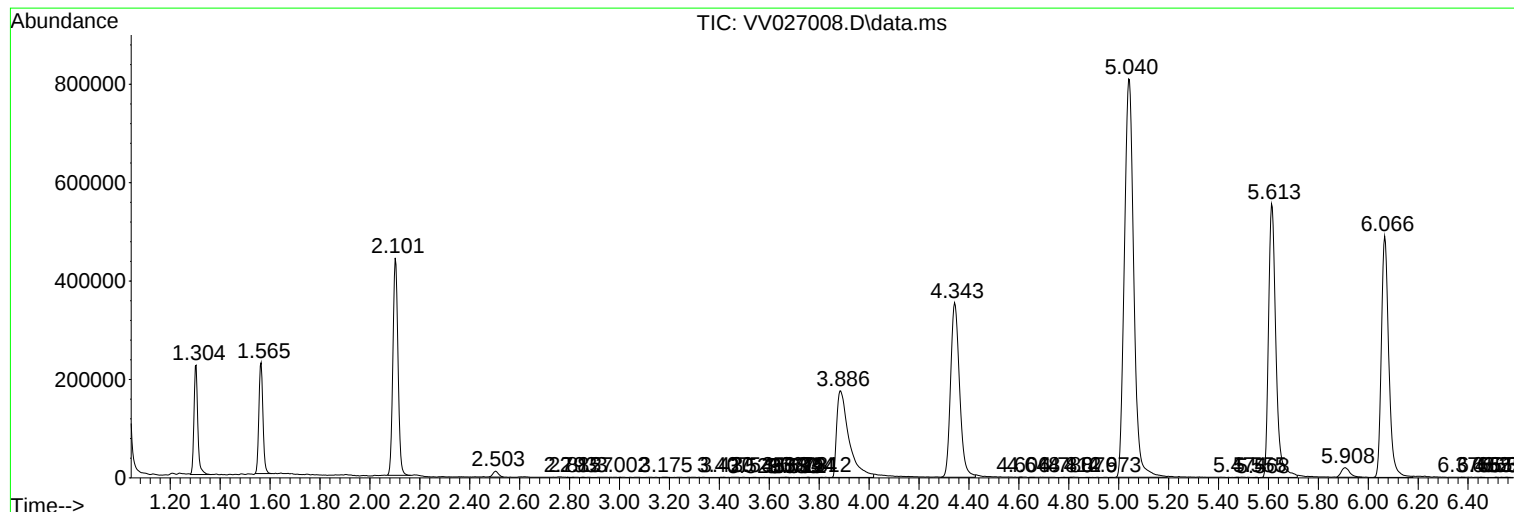

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027008.D
Acq On : 27 Jul 2022 19:01
Operator : SY/MD
Sample : N3880-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027008.D
Acq On : 27 Jul 2022 19:01
Operator : SY/MD
Sample : N3880-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------