

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027009.D
 Acq On : 27 Jul 2022 19:25
 Operator : SY/MD
 Sample : N3880-06DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	221249	234040	11.22%	1.491%
2	1.564	156	163	179	rVB	222370	252696	12.12%	1.610%
3	2.101	321	330	349	rBV	432654	619119	29.69%	3.944%
4	2.503	448	455	466	rVB3	10740	18276	0.88%	0.116%
5	2.876	568	571	572	rBV	310	162	0.01%	0.001%
6	3.002	606	610	612	rBV3	458	367	0.02%	0.002%
7	3.050	623	625	627	rBV	243	103	0.00%	0.001%
8	3.371	716	725	726	rBV	373	400	0.02%	0.003%
9	3.449	744	749	753	rBV3	324	318	0.02%	0.002%
10	3.468	753	755	758	rVV2	185	132	0.01%	0.001%
11	3.490	758	762	764	rVB	411	271	0.01%	0.002%
12	3.513	767	769	772	rBV	266	157	0.01%	0.001%
13	3.645	808	810	811	rBV	205	92	0.00%	0.001%
14	3.658	811	814	817	rVB	331	216	0.01%	0.001%
15	3.706	827	829	831	rBV	197	83	0.00%	0.001%
16	3.773	847	850	853	rBV	282	205	0.01%	0.001%
17	3.793	853	856	860	rVB2	380	251	0.01%	0.002%
18	3.815	860	863	865	rBV2	182	108	0.01%	0.001%
19	3.889	874	886	947	rBV2	187148	694061	33.28%	4.421%
20	4.342	1011	1027	1055	rBV	351918	873283	41.87%	5.563%
21	4.764	1155	1158	1164	rVB2	379	317	0.02%	0.002%
22	4.786	1164	1165	1167	rVB	364	119	0.01%	0.001%
23	4.870	1189	1191	1193	rBV	237	99	0.00%	0.001%
24	4.911	1200	1204	1208	rBV2	220	213	0.01%	0.001%
25	4.937	1209	1212	1215	rBV4	224	221	0.01%	0.001%
26	5.040	1228	1244	1274	rBV2	803285	2085496	100.00%	13.284%
27	5.442	1367	1369	1373	rVB2	360	202	0.01%	0.001%
28	5.493	1383	1385	1389	rVB4	530	214	0.01%	0.001%
29	5.612	1410	1422	1459	rBV	535708	1110882	53.27%	7.076%
30	5.911	1501	1515	1540	rBV5	49149	120884	5.80%	0.770%
31	6.066	1548	1563	1591	rBV	482404	991468	47.54%	6.315%
32	6.413	1670	1671	1673	rBV	273	69	0.00%	0.000%
33	6.455	1681	1684	1685	rBV2	354	201	0.01%	0.001%
34	6.481	1689	1692	1694	rBV2	362	137	0.01%	0.001%
35	6.493	1694	1696	1697	rBV2	282	147	0.01%	0.001%
36	6.513	1700	1702	1704	rBV3	253	136	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027009.D
 Acq On : 27 Jul 2022 19:25
 Operator : SY/MD
 Sample : N3880-06DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.577	1721	1722	1726	rBV3	250	136	0.01%	0.001%
38	6.628	1731	1738	1742	rBV4	2077	2994	0.14%	0.019%
39	6.837	1801	1803	1805	rBV2	293	137	0.01%	0.001%
40	6.860	1809	1810	1813	rVB	511	188	0.01%	0.001%
41	6.985	1837	1849	1877	rBV	215740	405069	19.42%	2.580%
42	7.313	1939	1951	1985	rBV	866266	1515633	72.67%	9.654%
43	7.619	2036	2046	2067	rBV	149962	270346	12.96%	1.722%
44	7.853	2116	2119	2125	rVB5	911	601	0.03%	0.004%
45	7.937	2143	2145	2147	rBV2	556	332	0.02%	0.002%
46	7.976	2147	2157	2178	rVB2	63409	111556	5.35%	0.711%
47	8.088	2182	2192	2233	rBV	623812	1211625	58.10%	7.718%
48	8.670	2369	2373	2378	rBV2	627	551	0.03%	0.004%
49	8.744	2394	2396	2397	rBV	432	189	0.01%	0.001%
50	8.770	2401	2404	2405	rBV	289	153	0.01%	0.001%
51	8.850	2417	2429	2458	rBV	832806	1370880	65.73%	8.732%
52	9.140	2517	2519	2521	rBV3	662	342	0.02%	0.002%
53	9.239	2547	2550	2552	rBV3	350	222	0.01%	0.001%
54	9.345	2577	2583	2585	rBV3	602	624	0.03%	0.004%
55	9.400	2595	2600	2604	rBV3	383	344	0.02%	0.002%
56	9.551	2642	2647	2655	rBV3	642	788	0.04%	0.005%
57	9.622	2666	2669	2672	rVB	461	287	0.01%	0.002%
58	9.644	2673	2676	2680	rBV	288	246	0.01%	0.002%
59	9.731	2701	2703	2704	rBV	241	100	0.00%	0.001%
60	9.789	2718	2721	2722	rBV2	349	208	0.01%	0.001%
61	9.860	2741	2743	2744	rBV	168	71	0.00%	0.000%
62	9.873	2744	2747	2751	rVV2	453	333	0.02%	0.002%
63	9.931	2761	2765	2768	rBV2	522	458	0.02%	0.003%
64	9.972	2773	2778	2780	rBV	377	284	0.01%	0.002%
65	10.011	2787	2790	2791	rBV	214	134	0.01%	0.001%
66	10.114	2819	2822	2828	rBV3	479	560	0.03%	0.004%
67	10.149	2831	2833	2835	rBB	211	91	0.00%	0.001%
68	10.214	2836	2853	2876	rBV	762580	1189585	57.04%	7.577%
69	10.410	2911	2914	2916	rBV2	429	215	0.01%	0.001%
70	10.628	2977	2982	2984	rBV	547	463	0.02%	0.003%
71	10.847	3047	3050	3053	rBV2	335	225	0.01%	0.001%
72	10.863	3053	3055	3058	rBV2	439	272	0.01%	0.002%
73	10.924	3070	3074	3077	rBV3	571	476	0.02%	0.003%
74	10.988	3093	3094	3096	rVB	312	110	0.01%	0.001%
75	11.249	3162	3175	3200	rBV	775220	1218540	58.43%	7.762%
76	11.622	3279	3291	3314	rBV	882712	1387592	66.54%	8.839%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027009.D
Acq On : 27 Jul 2022 19:25
Operator : SY/MD
Sample : N3880-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis

77	11.879	3369	3371	3374	rBV2	429	302	0.01%	0.002%
78	12.950	3702	3704	3707	rBV2	367	241	0.01%	0.002%
79	13.008	3719	3722	3727	rBV2	449	490	0.02%	0.003%
80	13.773	3958	3960	3961	rBV	309	122	0.01%	0.001%




Sum of corrected areas: 15699260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027009.D
Acq On : 27 Jul 2022 19:25
Operator : SY/MD
Sample : N3880-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

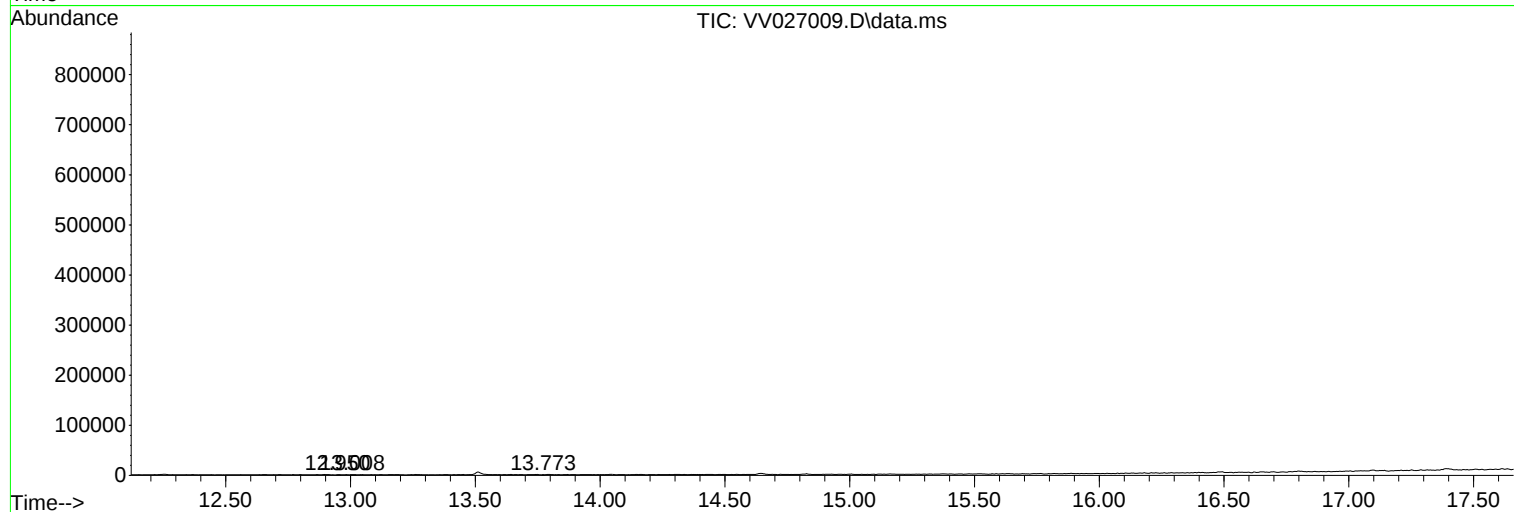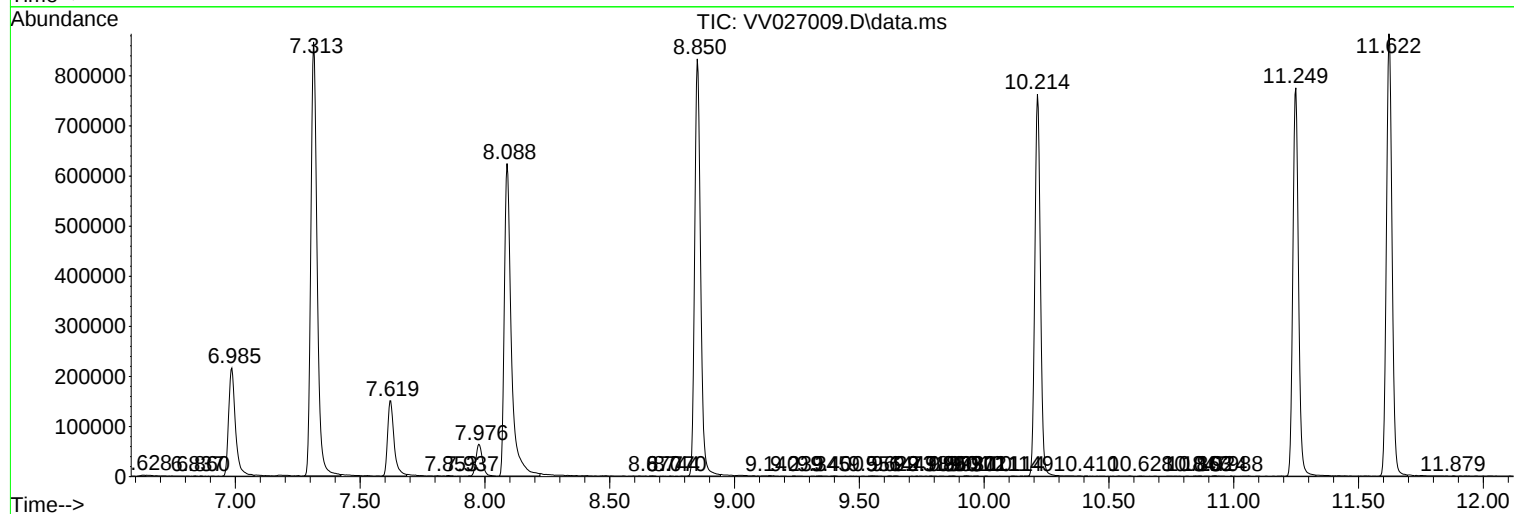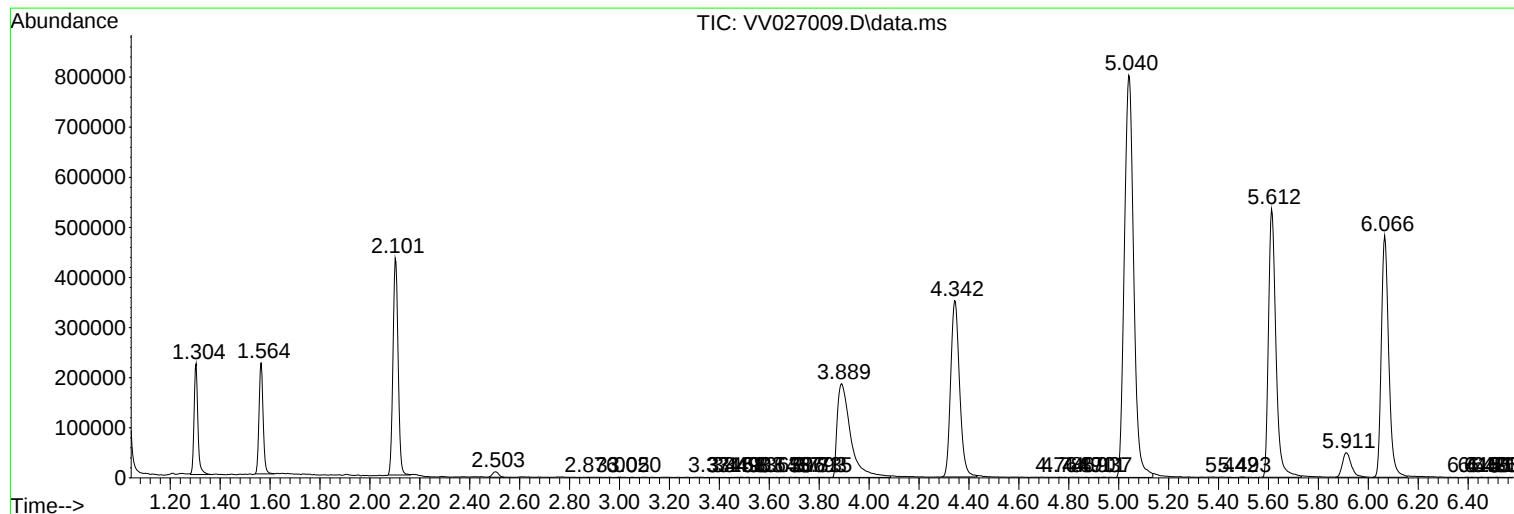

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027009.D
Acq On : 27 Jul 2022 19:25
Operator : SY/MD
Sample : N3880-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027009.D
Acq On : 27 Jul 2022 19:25
Operator : SY/MD
Sample : N3880-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------