

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027011.D
 Acq On : 27 Jul 2022 20:15
 Operator : SY/MD
 Sample : N3880-08DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.207	49	52	57	rBV2	3654	3101	0.15%	0.020%
2	1.304	75	82	95	rVB	215309	221637	10.92%	1.401%
3	1.564	155	163	175	rBV	212787	242602	11.96%	1.533%
4	2.101	320	330	347	rBV	417705	594111	29.28%	3.755%
5	2.278	383	385	392	rVB3	976	878	0.04%	0.006%
6	2.503	446	455	466	rVB3	11341	18360	0.90%	0.116%
7	2.613	480	489	502	rVB4	2479	5150	0.25%	0.033%
8	2.722	518	523	526	rBV2	416	325	0.02%	0.002%
9	2.841	558	560	564	rVB2	741	458	0.02%	0.003%
10	2.863	564	567	572	rBV2	318	298	0.01%	0.002%
11	3.121	642	647	650	rBV2	298	325	0.02%	0.002%
12	3.268	689	693	696	rBV3	344	354	0.02%	0.002%
13	3.304	701	704	708	rBV2	355	313	0.02%	0.002%
14	3.490	755	762	766	rBV2	348	498	0.02%	0.003%
15	3.886	873	885	937	rBV2	173663	629021	31.00%	3.975%
16	4.342	1010	1027	1061	rBV	345946	859015	42.33%	5.429%
17	4.574	1092	1099	1104	rVB3	614	780	0.04%	0.005%
18	4.661	1122	1126	1128	rBV4	459	301	0.01%	0.002%
19	4.712	1139	1142	1145	rVB3	684	507	0.02%	0.003%
20	4.764	1152	1158	1161	rBV2	368	350	0.02%	0.002%
21	4.934	1208	1211	1215	rBV3	415	354	0.02%	0.002%
22	5.040	1227	1244	1283	rBV2	775935	2029129	100.00%	12.824%
23	5.336	1333	1336	1341	rVB3	639	488	0.02%	0.003%
24	5.381	1347	1350	1356	rVB4	570	569	0.03%	0.004%
25	5.413	1358	1360	1364	rVB3	545	328	0.02%	0.002%
26	5.493	1382	1385	1388	rBV3	632	342	0.02%	0.002%
27	5.612	1409	1422	1451	rBV	535902	1102783	54.35%	6.970%
28	5.821	1484	1487	1490	rVB3	523	325	0.02%	0.002%
29	5.841	1490	1493	1496	rBV2	452	388	0.02%	0.002%
30	5.908	1502	1514	1531	rBV4	19402	43225	2.13%	0.273%
31	6.066	1550	1563	1595	rBV	471276	968200	47.72%	6.119%
32	6.526	1702	1706	1710	rVB3	474	387	0.02%	0.002%
33	6.638	1731	1741	1748	rBV5	2410	5285	0.26%	0.033%
34	6.985	1838	1849	1878	rBV	205511	389687	19.20%	2.463%
35	7.169	1903	1906	1907	rBV	677	395	0.02%	0.002%
36	7.252	1929	1932	1936	rVB4	1050	739	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027011.D
 Acq On : 27 Jul 2022 20:15
 Operator : SY/MD
 Sample : N3880-08DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	7.313	1939	1951	1977	rBV	831695	1456046	71.76%	9.202%
38	7.619	2036	2046	2078	rVV	145704	264104	13.02%	1.669%
39	7.818	2104	2108	2111	rBV4	344	309	0.02%	0.002%
40	7.847	2114	2117	2121	rVB3	684	539	0.03%	0.003%
41	7.870	2121	2124	2127	rVB2	773	474	0.02%	0.003%
42	7.924	2137	2141	2144	rBV4	620	477	0.02%	0.003%
43	7.972	2144	2156	2178	rBV	396127	672038	33.12%	4.247%
44	8.088	2181	2192	2237	rBV	599421	1156515	57.00%	7.309%
45	8.603	2349	2352	2353	rBV2	529	313	0.02%	0.002%
46	8.673	2368	2374	2377	rBV4	449	427	0.02%	0.003%
47	8.715	2384	2387	2395	rVV4	505	571	0.03%	0.004%
48	8.850	2417	2429	2456	rBV	857664	1384582	68.24%	8.751%
49	9.143	2516	2520	2528	rBV5	639	917	0.05%	0.006%
50	9.242	2549	2551	2555	rVB2	415	319	0.02%	0.002%
51	9.275	2555	2561	2565	rBV5	731	794	0.04%	0.005%
52	9.320	2573	2575	2579	rVB2	429	304	0.01%	0.002%
53	9.551	2642	2647	2651	rVV2	1116	1029	0.05%	0.007%
54	9.580	2654	2656	2661	rVB5	599	415	0.02%	0.003%
55	9.635	2669	2673	2675	rBV2	362	351	0.02%	0.002%
56	9.802	2722	2725	2729	rBV2	432	380	0.02%	0.002%
57	9.889	2746	2752	2755	rBV3	330	330	0.02%	0.002%
58	9.934	2760	2766	2767	rBV2	559	587	0.03%	0.004%
59	10.214	2840	2853	2878	rBV	742864	1164781	57.40%	7.361%
60	10.522	2944	2949	2951	rBV3	308	301	0.01%	0.002%
61	10.545	2952	2956	2960	rVV2	568	546	0.03%	0.003%
62	10.570	2962	2964	2970	rVB3	629	617	0.03%	0.004%
63	10.767	3019	3025	3026	rBV3	325	353	0.02%	0.002%
64	10.799	3031	3035	3038	rBV3	356	300	0.01%	0.002%
65	10.902	3063	3067	3069	rBV3	460	381	0.02%	0.002%
66	11.152	3140	3145	3148	rBV2	489	481	0.02%	0.003%
67	11.191	3155	3157	3162	rVB3	580	333	0.02%	0.002%
68	11.249	3162	3175	3194	rBV	786404	1210950	59.68%	7.653%
69	11.525	3254	3261	3263	rBV3	613	707	0.03%	0.004%
70	11.622	3279	3291	3315	rBV	863669	1361928	67.12%	8.607%
71	11.802	3345	3347	3351	rBV2	480	346	0.02%	0.002%
72	11.873	3366	3369	3376	rVB3	699	680	0.03%	0.004%
73	12.062	3425	3428	3431	rBV3	534	376	0.02%	0.002%
74	12.252	3472	3487	3492	rBV5	1539	2914	0.14%	0.018%
75	12.316	3501	3507	3508	rBV2	402	357	0.02%	0.002%
76	12.644	3606	3609	3613	rBV2	382	358	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027011.D
 Acq On : 27 Jul 2022 20:15
 Operator : SY/MD
 Sample : N3880-08DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.879	3678	3682	3684	rBV2	528	377	0.02%	0.002%
78	13.046	3731	3734	3739	rVV2	578	555	0.03%	0.004%
79	13.104	3749	3752	3756	rVB2	634	511	0.03%	0.003%
80	13.168	3769	3772	3778	rVB	524	478	0.02%	0.003%
81	13.201	3778	3782	3785	rBV2	437	406	0.02%	0.003%
82	13.226	3785	3790	3792	rBV2	440	372	0.02%	0.002%
83	13.265	3798	3802	3804	rBV3	620	474	0.02%	0.003%
84	13.487	3867	3871	3872	rBV2	380	299	0.01%	0.002%
85	13.509	3874	3878	3883	rBV4	1971	2178	0.11%	0.014%
86	13.577	3896	3899	3902	rVB2	614	378	0.02%	0.002%
87	13.615	3907	3911	3913	rBV3	590	475	0.02%	0.003%
88	13.699	3930	3937	3938	rBV3	472	557	0.03%	0.004%
89	13.776	3959	3961	3966	rVB3	660	562	0.03%	0.004%
90	13.866	3986	3989	3992	rBV2	468	346	0.02%	0.002%
91	14.011	4032	4034	4038	rVB2	590	331	0.02%	0.002%
92	14.033	4038	4041	4044	rBV	590	525	0.03%	0.003%
93	14.477	4175	4179	4183	rVB4	507	397	0.02%	0.003%
94	14.538	4196	4198	4202	rBV3	391	299	0.01%	0.002%
95	14.699	4244	4248	4250	rBV2	852	668	0.03%	0.004%
96	15.146	4385	4387	4391	rVB3	857	541	0.03%	0.003%
97	15.168	4391	4394	4397	rBV4	972	712	0.04%	0.004%
98	15.329	4440	4444	4447	rBV3	779	750	0.04%	0.005%
99	15.393	4460	4464	4466	rBV3	909	721	0.04%	0.005%
100	15.525	4503	4505	4506	rBV	707	330	0.02%	0.002%




Sum of corrected areas: 15822780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027011.D
Acq On : 27 Jul 2022 20:15
Operator : SY/MD
Sample : N3880-08DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

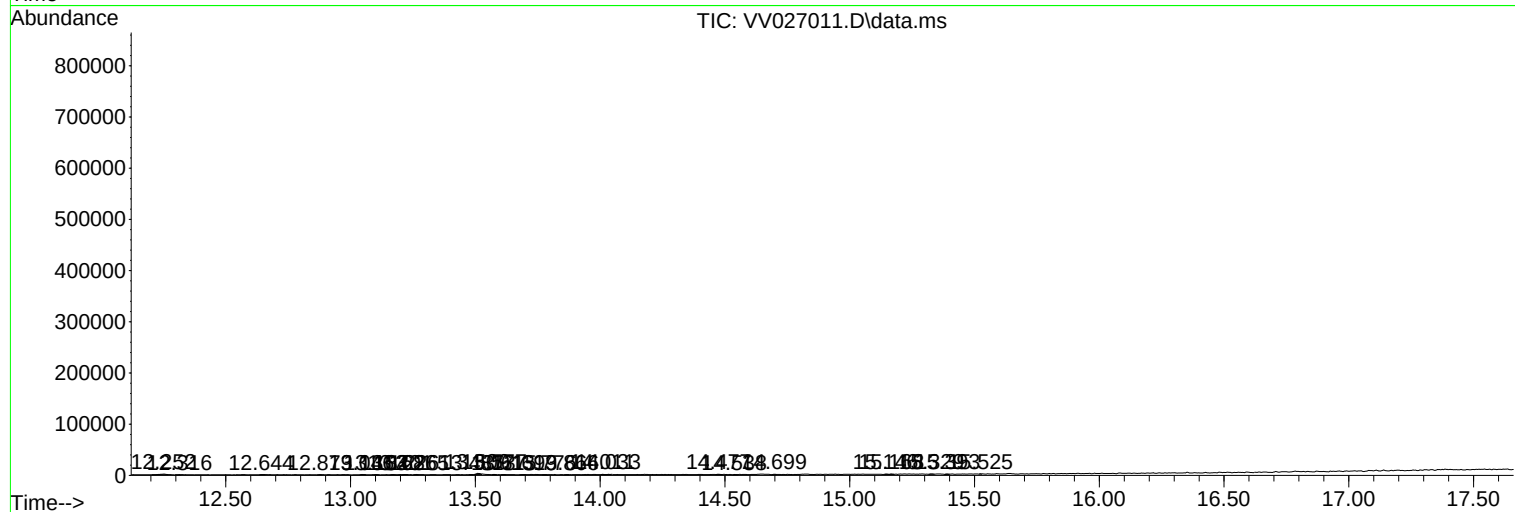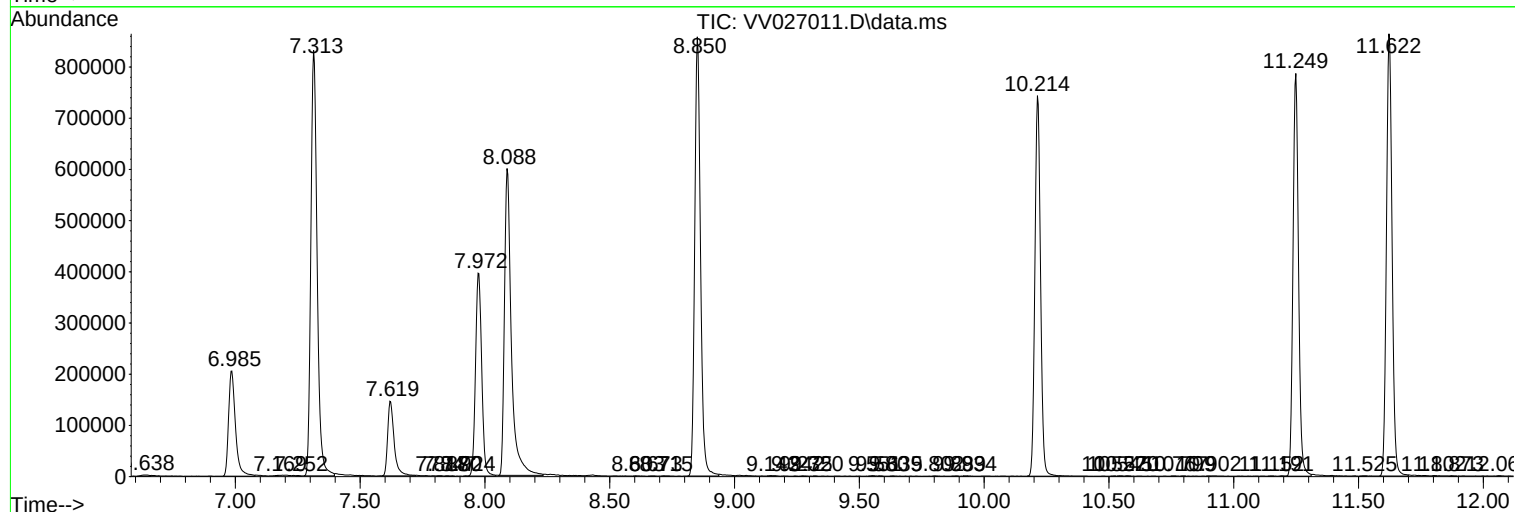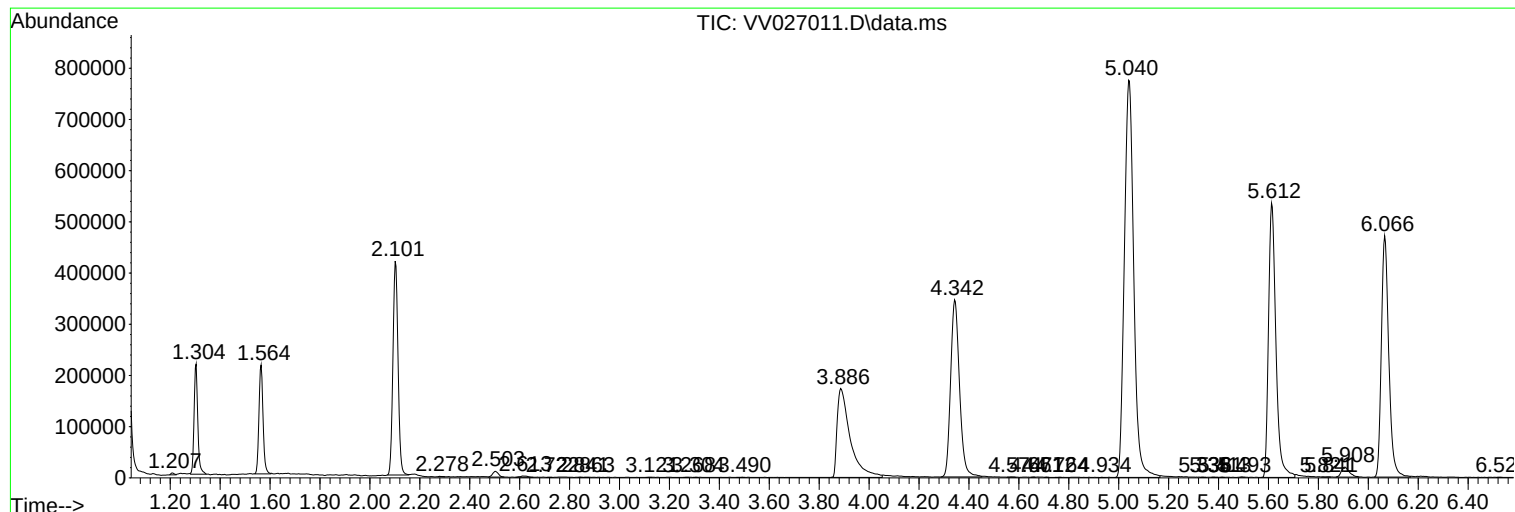

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027011.D
Acq On : 27 Jul 2022 20:15
Operator : SY/MD
Sample : N3880-08DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DEBUG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027011.D
Acq On : 27 Jul 2022 20:15
Operator : SY/MD
Sample : N3880-08DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------