

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027012.D
 Acq On : 27 Jul 2022 20:39
 Operator : SY/MD
 Sample : N3880-07DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	206886	218975	10.98%	1.426%
2	1.565	155	163	175	rBV	211145	240490	12.06%	1.566%
3	2.102	320	330	343	rBV	406384	575550	28.86%	3.747%
4	2.349	403	407	409	rBV2	491	426	0.02%	0.003%
5	2.503	446	455	466	rVB2	11552	17701	0.89%	0.115%
6	2.610	481	488	497	rBV4	1624	2819	0.14%	0.018%
7	2.764	532	536	540	rBV4	806	721	0.04%	0.005%
8	2.851	559	563	566	rBV2	361	331	0.02%	0.002%
9	3.024	612	617	623	rBV3	424	580	0.03%	0.004%
10	3.188	664	668	671	rBV2	423	301	0.02%	0.002%
11	3.291	697	700	706	rVB	397	359	0.02%	0.002%
12	3.323	706	710	716	rVB2	481	453	0.02%	0.003%
13	3.500	757	765	769	rBV2	434	542	0.03%	0.004%
14	3.761	844	846	851	rVB2	415	325	0.02%	0.002%
15	3.809	856	861	864	rBV2	500	382	0.02%	0.002%
16	3.886	874	885	941	rBV	168877	591075	29.64%	3.848%
17	4.343	1007	1027	1051	rBV	339384	842391	42.24%	5.484%
18	4.651	1121	1123	1127	rBV3	482	335	0.02%	0.002%
19	5.040	1224	1244	1280	rBV2	767533	1994418	100.00%	12.984%
20	5.349	1335	1340	1343	rBV3	670	603	0.03%	0.004%
21	5.368	1344	1346	1349	rVB3	723	299	0.01%	0.002%
22	5.500	1385	1387	1391	rVB4	392	324	0.02%	0.002%
23	5.519	1391	1393	1396	rBV2	465	298	0.01%	0.002%
24	5.613	1410	1422	1459	rBV	512854	1067380	53.52%	6.949%
25	5.905	1501	1513	1534	rVV4	19688	44516	2.23%	0.290%
26	6.066	1549	1563	1600	rBV	459884	954949	47.88%	6.217%
27	6.204	1604	1606	1612	rVV6	1732	2048	0.10%	0.013%
28	6.230	1612	1614	1621	rVB5	1388	1186	0.06%	0.008%
29	6.372	1656	1658	1662	rVV3	717	429	0.02%	0.003%
30	6.445	1678	1681	1685	rBV2	528	307	0.02%	0.002%
31	6.497	1694	1697	1699	rBV2	462	332	0.02%	0.002%
32	6.548	1711	1713	1719	rVB2	535	381	0.02%	0.002%
33	6.642	1731	1742	1748	rBV7	2408	4942	0.25%	0.032%
34	6.735	1766	1771	1773	rBV3	658	414	0.02%	0.003%
35	6.880	1809	1816	1819	rBV3	390	414	0.02%	0.003%
36	6.931	1827	1832	1835	rBV3	318	328	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027012.D
 Acq On : 27 Jul 2022 20:39
 Operator : SY/MD
 Sample : N3880-07DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.986	1837	1849	1879	rBV	200726	383290	19.22%	2.495%
38	7.162	1902	1904	1906	rBV2	630	384	0.02%	0.002%
39	7.314	1939	1951	1975	rBV	806652	1406396	70.52%	9.156%
40	7.571	2028	2031	2036	rBV3	506	543	0.03%	0.004%
41	7.619	2036	2046	2067	rBV	141877	257159	12.89%	1.674%
42	7.799	2099	2102	2106	rVB3	654	385	0.02%	0.003%
43	7.857	2117	2120	2127	rVB6	745	804	0.04%	0.005%
44	7.973	2143	2156	2179	rBV	363933	629923	31.58%	4.101%
45	8.088	2182	2192	2241	rVV	599595	1144838	57.40%	7.453%
46	8.426	2290	2297	2304	rVB6	1400	1914	0.10%	0.012%
47	8.474	2309	2312	2317	rVB3	785	598	0.03%	0.004%
48	8.497	2317	2319	2322	rBV2	546	325	0.02%	0.002%
49	8.535	2327	2331	2333	rBV	354	307	0.02%	0.002%
50	8.632	2357	2361	2364	rBV4	543	417	0.02%	0.003%
51	8.738	2388	2394	2395	rBV4	398	335	0.02%	0.002%
52	8.851	2417	2429	2454	rBV	797790	1318699	66.12%	8.585%
53	9.146	2519	2521	2526	rVB4	514	303	0.02%	0.002%
54	9.175	2526	2530	2535	rBV2	380	293	0.01%	0.002%
55	9.252	2550	2554	2557	rBV	471	414	0.02%	0.003%
56	9.487	2624	2627	2633	rVV3	447	485	0.02%	0.003%
57	9.513	2633	2635	2641	rVB3	369	305	0.02%	0.002%
58	9.558	2645	2649	2653	rVV2	719	575	0.03%	0.004%
59	9.857	2738	2742	2748	rVB3	488	412	0.02%	0.003%
60	10.014	2788	2791	2796	rVB	466	351	0.02%	0.002%
61	10.214	2841	2853	2877	rVV	733025	1156659	57.99%	7.530%
62	10.378	2900	2904	2906	rBV3	589	423	0.02%	0.003%
63	10.455	2919	2928	2933	rBV3	457	757	0.04%	0.005%
64	10.487	2933	2938	2940	rBV2	373	289	0.01%	0.002%
65	10.539	2950	2954	2956	rBV4	393	359	0.02%	0.002%
66	10.555	2956	2959	2963	rVB3	573	420	0.02%	0.003%
67	10.764	3021	3024	3027	rBV3	436	300	0.02%	0.002%
68	10.924	3069	3074	3079	rVB4	661	808	0.04%	0.005%
69	10.998	3091	3097	3101	rBV3	345	412	0.02%	0.003%
70	11.047	3109	3112	3118	rVB3	494	496	0.02%	0.003%
71	11.166	3143	3149	3153	rBV3	400	403	0.02%	0.003%
72	11.191	3153	3157	3163	rBV4	730	588	0.03%	0.004%
73	11.249	3163	3175	3208	rBV	747561	1158326	58.08%	7.541%
74	11.477	3242	3246	3252	rVB4	573	582	0.03%	0.004%
75	11.622	3279	3291	3319	rBV	834725	1304589	65.41%	8.493%
76	11.847	3358	3361	3368	rBV4	425	364	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027012.D
 Acq On : 27 Jul 2022 20:39
 Operator : SY/MD
 Sample : N3880-07DL 400X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.905	3376	3379	3383	rVB	612	387	0.02%	0.003%
78	12.259	3479	3489	3498	rBV4	1361	2511	0.13%	0.016%
79	12.436	3541	3544	3547	rVV2	544	434	0.02%	0.003%
80	12.503	3562	3565	3574	rVB3	487	648	0.03%	0.004%
81	12.542	3574	3577	3580	rBV	335	285	0.01%	0.002%
82	12.625	3598	3603	3607	rBV3	430	590	0.03%	0.004%
83	12.699	3624	3626	3632	rVB	477	430	0.02%	0.003%
84	12.731	3632	3636	3638	rBV2	423	372	0.02%	0.002%
85	12.802	3656	3658	3663	rBV3	458	354	0.02%	0.002%
86	12.828	3663	3666	3673	rVB3	509	580	0.03%	0.004%
87	13.111	3751	3754	3761	rBV3	377	327	0.02%	0.002%
88	13.159	3767	3769	3774	rVB2	390	338	0.02%	0.002%
89	13.204	3779	3783	3785	rBV	410	348	0.02%	0.002%
90	13.336	3822	3824	3828	rVB2	434	359	0.02%	0.002%
91	13.513	3867	3879	3884	rBV4	3200	4787	0.24%	0.031%
92	13.696	3931	3936	3942	rBV2	644	566	0.03%	0.004%
93	13.718	3942	3943	3946	rBV3	523	312	0.02%	0.002%
94	13.857	3983	3986	3991	rVB4	659	503	0.03%	0.003%
95	14.104	4061	4063	4065	rBV2	537	291	0.01%	0.002%
96	14.641	4227	4230	4234	rBV4	1250	999	0.05%	0.007%
97	14.757	4262	4266	4269	rBV4	769	690	0.03%	0.004%
98	14.825	4284	4287	4293	rVB4	921	882	0.04%	0.006%
99	15.143	4384	4386	4388	rBV2	779	365	0.02%	0.002%
100	15.349	4447	4450	4452	rBV3	663	417	0.02%	0.003%

Sum of corrected areas: 15360329




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027012.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3880-07DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

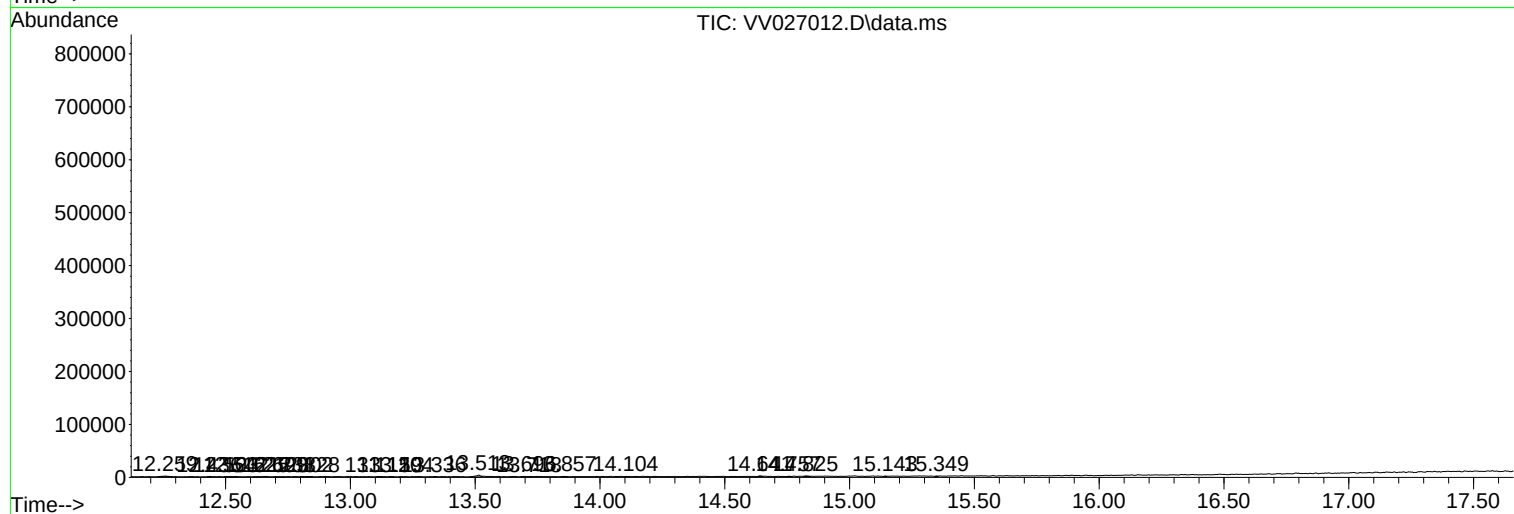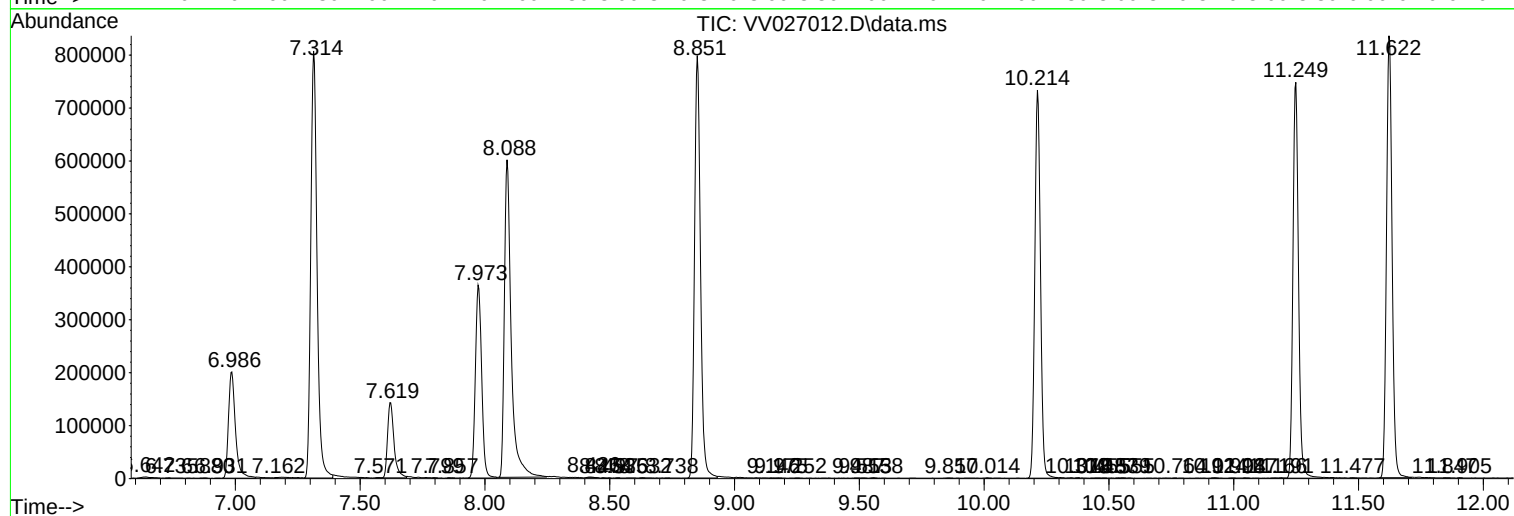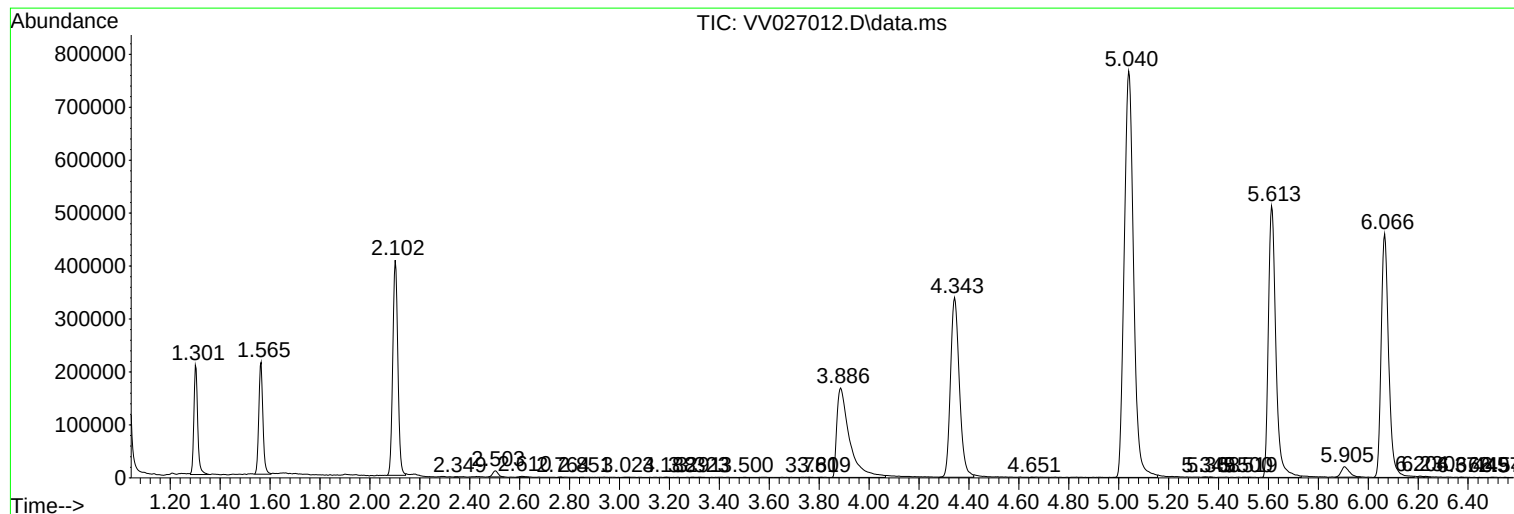

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027012.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3880-07DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DEBUG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027012.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3880-07DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DEBUG0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------