

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027014.D
 Acq On : 27 Jul 2022 21:53
 Operator : SY/MD
 Sample : VV0727WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	326313	346118	16.21%	2.260%
2	1.564	156	163	174	rVB	265390	299512	14.03%	1.955%
3	2.101	320	330	346	rBV	552172	783347	36.69%	5.114%
4	2.503	448	455	466	rVB	8392	13681	0.64%	0.089%
5	2.738	525	528	529	rBV	395	215	0.01%	0.001%
6	2.754	529	533	541	rVB5	1045	1741	0.08%	0.011%
7	2.847	560	562	566	rVB	379	241	0.01%	0.002%
8	3.153	655	657	659	rBV2	387	152	0.01%	0.001%
9	3.172	659	663	664	rBV	469	307	0.01%	0.002%
10	3.256	687	689	693	rVB	292	149	0.01%	0.001%
11	3.291	693	700	703	rBV3	309	354	0.02%	0.002%
12	3.381	723	728	729	rBV	375	279	0.01%	0.002%
13	3.439	743	746	748	rBV2	382	272	0.01%	0.002%
14	3.545	776	779	782	rVB2	327	178	0.01%	0.001%
15	3.567	782	786	789	rBV2	313	326	0.02%	0.002%
16	3.651	810	812	814	rVB	216	86	0.00%	0.001%
17	3.715	829	832	835	rVB3	372	219	0.01%	0.001%
18	3.735	835	838	844	rBV3	401	417	0.02%	0.003%
19	3.834	866	869	873	rBV	196	179	0.01%	0.001%
20	3.886	875	885	929	rBV	142740	481942	22.57%	3.146%
21	4.342	1012	1027	1051	rBV	346925	856283	40.10%	5.590%
22	4.760	1155	1157	1158	rBV	418	186	0.01%	0.001%
23	4.786	1162	1165	1166	rBV	335	170	0.01%	0.001%
24	4.818	1172	1175	1177	rBV2	640	468	0.02%	0.003%
25	4.944	1211	1214	1217	rBV3	459	253	0.01%	0.002%
26	4.966	1217	1221	1224	rBV3	318	230	0.01%	0.002%
27	5.040	1227	1244	1285	rBV2	830149	2135167	100.00%	13.939%
28	5.448	1370	1371	1377	rBV2	247	156	0.01%	0.001%
29	5.538	1394	1399	1402	rBV3	470	460	0.02%	0.003%
30	5.612	1410	1422	1455	rBV	529685	1092775	51.18%	7.134%
31	5.908	1503	1514	1532	rBV2	14509	31905	1.49%	0.208%
32	5.995	1537	1541	1547	rVB6	554	636	0.03%	0.004%
33	6.066	1549	1563	1594	rBV	471239	966442	45.26%	6.309%
34	6.342	1647	1649	1653	rVB2	293	116	0.01%	0.001%
35	6.429	1674	1676	1679	rVB2	352	135	0.01%	0.001%
36	6.487	1690	1694	1697	rBV2	403	371	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027014.D
 Acq On : 27 Jul 2022 21:53
 Operator : SY/MD
 Sample : VV0727WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.587	1723	1725	1727	rBV2	246	125	0.01%	0.001%
38	6.606	1729	1731	1735	rBV	411	291	0.01%	0.002%
39	6.641	1735	1742	1745	rBV2	543	646	0.03%	0.004%
40	6.747	1773	1775	1776	rBV2	241	95	0.00%	0.001%
41	6.770	1780	1782	1786	rVB2	350	193	0.01%	0.001%
42	6.792	1786	1789	1790	rBV	185	88	0.00%	0.001%
43	6.805	1791	1793	1795	rVB2	427	178	0.01%	0.001%
44	6.841	1801	1804	1807	rBV	306	217	0.01%	0.001%
45	6.902	1819	1823	1825	rBV2	301	251	0.01%	0.002%
46	6.931	1829	1832	1834	rBV2	341	198	0.01%	0.001%
47	6.985	1838	1849	1874	rBV2	210636	402532	18.85%	2.628%
48	7.313	1939	1951	1990	rBV	909270	1612276	75.51%	10.526%
49	7.622	2034	2047	2072	rBV	147870	274394	12.85%	1.791%
50	7.982	2149	2159	2169	rVB5	8330	14746	0.69%	0.096%
51	8.053	2178	2181	2182	rBV	393	168	0.01%	0.001%
52	8.088	2182	2192	2230	rBV	487103	966920	45.29%	6.312%
53	8.480	2310	2314	2315	rBV2	619	434	0.02%	0.003%
54	8.574	2339	2343	2350	rVB3	887	713	0.03%	0.005%
55	8.603	2350	2352	2354	rVB	355	148	0.01%	0.001%
56	8.622	2354	2358	2362	rBV3	893	998	0.05%	0.007%
57	8.850	2416	2429	2459	rBV	829792	1367393	64.04%	8.927%
58	9.101	2505	2507	2510	rBV2	468	297	0.01%	0.002%
59	9.149	2516	2522	2525	rBV5	1043	1159	0.05%	0.008%
60	9.239	2545	2550	2551	rBV	545	393	0.02%	0.003%
61	9.262	2554	2557	2562	rVB2	679	560	0.03%	0.004%
62	9.297	2566	2568	2569	rBV2	210	94	0.00%	0.001%
63	9.352	2583	2585	2586	rBV	340	111	0.01%	0.001%
64	9.432	2605	2610	2612	rBV3	356	411	0.02%	0.003%
65	9.513	2630	2635	2637	rBV3	313	251	0.01%	0.002%
66	9.541	2641	2644	2645	rBV	453	232	0.01%	0.002%
67	9.558	2646	2649	2653	rVB3	690	601	0.03%	0.004%
68	9.641	2673	2675	2678	rBV2	259	146	0.01%	0.001%
69	9.840	2734	2737	2738	rBV	198	100	0.00%	0.001%
70	9.866	2742	2745	2749	rBV2	366	239	0.01%	0.002%
71	9.886	2749	2751	2752	rBV	276	141	0.01%	0.001%
72	9.931	2759	2765	2766	rBV2	1041	738	0.03%	0.005%
73	10.008	2784	2789	2790	rBV2	342	208	0.01%	0.001%
74	10.053	2798	2803	2806	rBV2	308	347	0.02%	0.002%
75	10.114	2818	2822	2826	rVB2	416	398	0.02%	0.003%
76	10.140	2826	2830	2833	rBV2	525	355	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027014.D
 Acq On : 27 Jul 2022 21:53
 Operator : SY/MD
 Sample : VV0727WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.213	2841	2853	2878	rBV	681129	1086805	50.90%	7.095%
78	10.442	2920	2924	2929	rBV2	545	679	0.03%	0.004%
79	10.545	2952	2956	2958	rBV	631	534	0.03%	0.003%
80	10.631	2981	2983	2986	rBV2	248	201	0.01%	0.001%
81	10.683	2997	2999	3002	rVB2	392	174	0.01%	0.001%
82	10.712	3007	3008	3009	rBV	371	110	0.01%	0.001%
83	10.763	3020	3024	3028	rVV2	504	410	0.02%	0.003%
84	10.824	3038	3043	3046	rBV	260	230	0.01%	0.002%
85	10.853	3049	3052	3053	rBV	327	184	0.01%	0.001%
86	10.966	3085	3087	3090	rVB	402	198	0.01%	0.001%
87	11.004	3095	3099	3102	rBV2	428	366	0.02%	0.002%
88	11.133	3136	3139	3144	rBV2	273	235	0.01%	0.002%
89	11.249	3163	3175	3200	rBV	759069	1188852	55.68%	7.761%
90	11.574	3274	3276	3279	rBV2	298	207	0.01%	0.001%
91	11.622	3279	3291	3316	rBV	858132	1340966	62.80%	8.754%
92	12.197	3467	3470	3472	rBV	374	232	0.01%	0.002%
93	12.467	3552	3554	3562	rBV3	436	521	0.02%	0.003%
94	12.619	3598	3601	3604	rBV3	356	207	0.01%	0.001%
95	12.651	3605	3611	3621	rBV3	1777	2655	0.12%	0.017%
96	13.265	3797	3802	3803	rBV2	2057	1630	0.08%	0.011%
97	13.438	3853	3856	3861	rBV3	491	411	0.02%	0.003%
98	13.512	3871	3879	3890	rBV2	7013	11858	0.56%	0.077%
99	13.747	3944	3952	3965	rBV7	3146	5098	0.24%	0.033%
100	16.438	4786	4789	4793	rVB	17592	9545	0.45%	0.062%




Sum of corrected areas: 15317561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027014.D
Acq On : 27 Jul 2022 21:53
Operator : SY/MD
Sample : VV0727WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

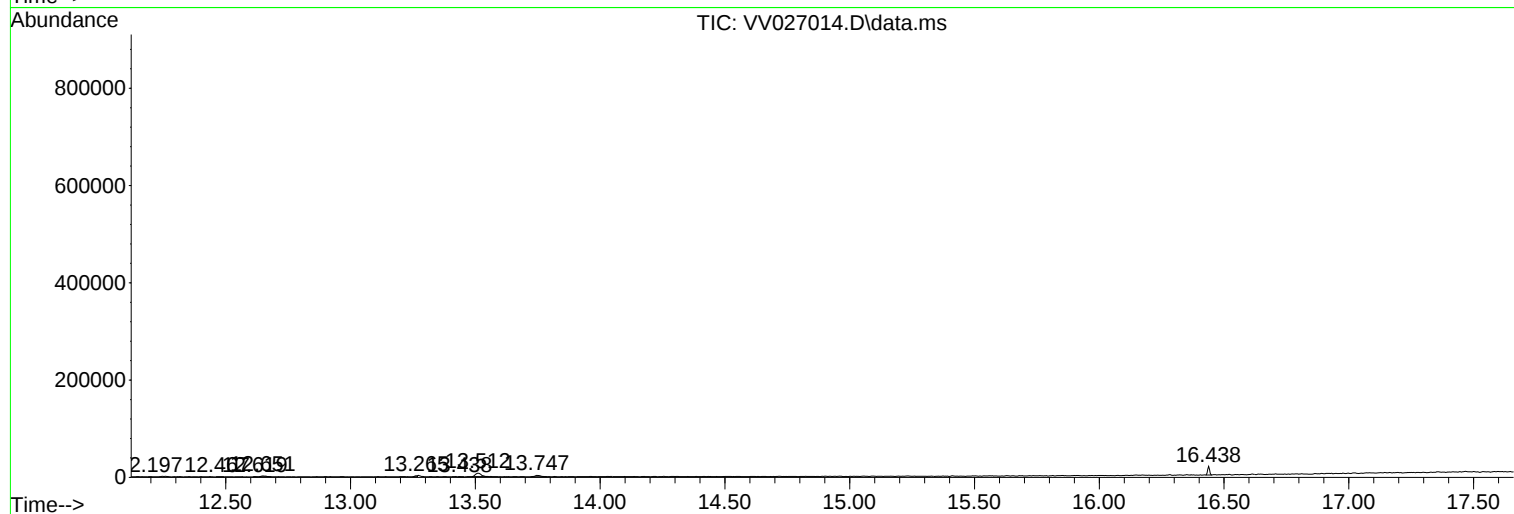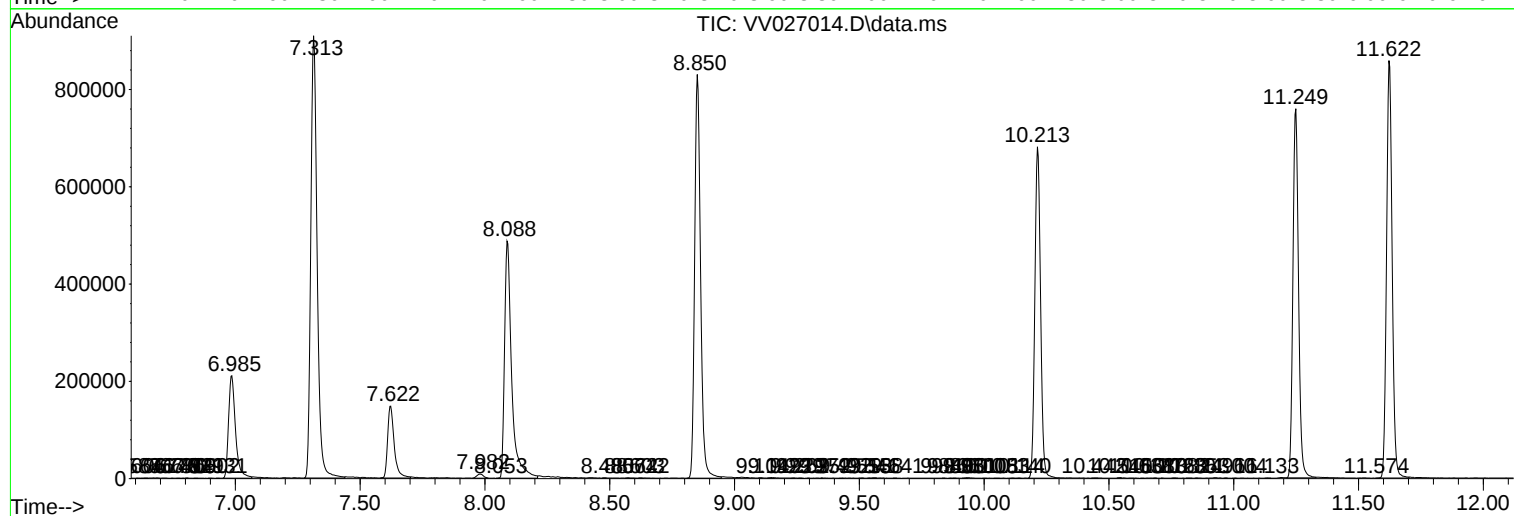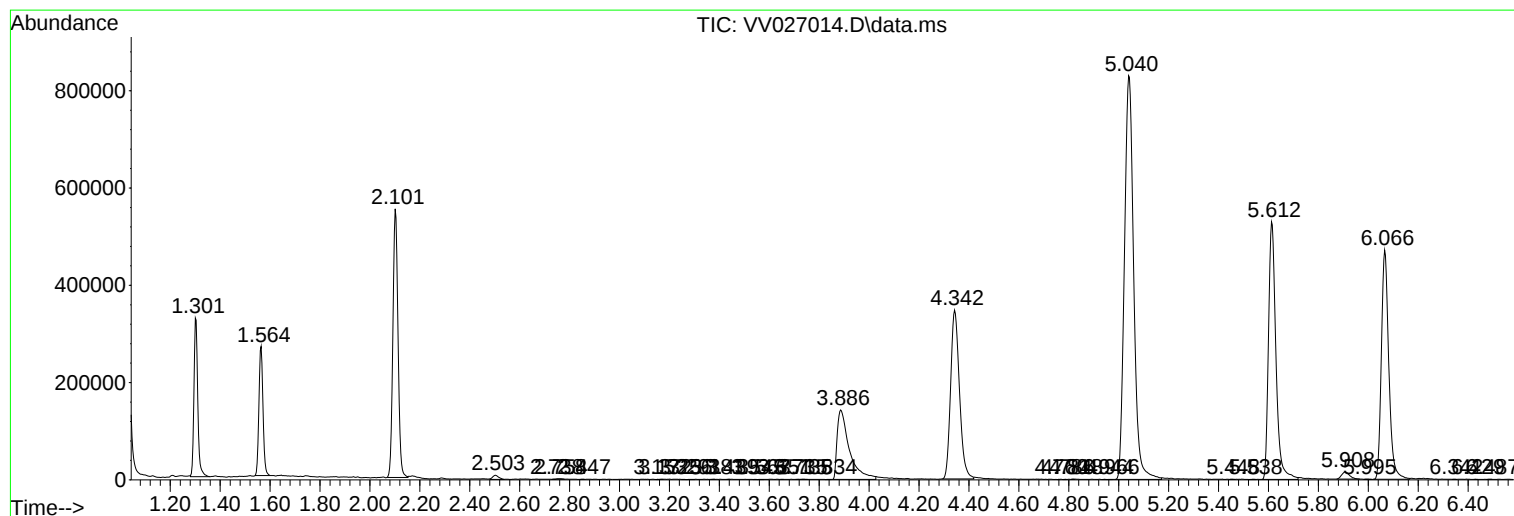

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027014.D
Acq On : 27 Jul 2022 21:53
Operator : SY/MD
Sample : VV0727WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027014.D
Acq On : 27 Jul 2022 21:53
Operator : SY/MD
Sample : VV0727WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc