

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027015.D
 Acq On : 27 Jul 2022 22:17
 Operator : SY/MD
 Sample : N3897-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV027015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	318407	327685	15.68%	2.230%
2	1.564	155	163	178	rBV	259077	297830	14.25%	2.027%
3	2.101	320	330	352	rVB	539234	764453	36.58%	5.202%
4	2.741	525	529	531	rBV2	796	645	0.03%	0.004%
5	2.921	583	585	588	rVB	379	202	0.01%	0.001%
6	2.941	588	591	594	rBV3	390	287	0.01%	0.002%
7	2.963	594	598	600	rBV2	440	343	0.02%	0.002%
8	3.034	617	620	623	rVB2	426	293	0.01%	0.002%
9	3.053	623	626	628	rBV	185	116	0.01%	0.001%
10	3.066	628	630	632	rBV2	325	224	0.01%	0.002%
11	3.105	640	642	644	rBV	241	166	0.01%	0.001%
12	3.137	650	652	658	rVB2	297	174	0.01%	0.001%
13	3.169	658	662	665	rBV	487	339	0.02%	0.002%
14	3.185	665	667	669	rBV2	324	212	0.01%	0.001%
15	3.224	676	679	685	rBV2	287	292	0.01%	0.002%
16	3.253	685	688	690	rVV2	213	126	0.01%	0.001%
17	3.269	690	693	696	rVB	299	218	0.01%	0.001%
18	3.285	696	698	701	rBV	284	129	0.01%	0.001%
19	3.410	735	737	740	rBV2	238	126	0.01%	0.001%
20	3.442	744	747	749	rBV	266	160	0.01%	0.001%
21	3.539	775	777	784	rVB3	386	297	0.01%	0.002%
22	3.629	799	805	807	rBV	278	369	0.02%	0.003%
23	3.671	813	818	822	rBV	414	358	0.02%	0.002%
24	3.732	833	837	838	rBV2	236	163	0.01%	0.001%
25	3.815	861	863	866	rVB2	352	202	0.01%	0.001%
26	3.851	870	874	876	rBV2	256	185	0.01%	0.001%
27	3.892	876	887	917	rBV	102385	354425	16.96%	2.412%
28	4.343	1012	1027	1053	rBV	338181	836334	40.02%	5.691%
29	4.667	1126	1128	1129	rBV	423	161	0.01%	0.001%
30	4.770	1157	1160	1163	rBV3	341	251	0.01%	0.002%
31	4.828	1176	1178	1181	rBV2	409	230	0.01%	0.002%
32	4.941	1210	1213	1215	rVB	253	136	0.01%	0.001%
33	4.957	1215	1218	1220	rBV2	321	207	0.01%	0.001%
34	5.040	1227	1244	1282	rBV2	812802	2089779	100.00%	14.220%
35	5.481	1380	1381	1382	rBV	459	167	0.01%	0.001%
36	5.558	1402	1405	1408	rBV	271	208	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027015.D
 Acq On : 27 Jul 2022 22:17
 Operator : SY/MD
 Sample : N3897-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	5.613	1409	1422	1451	rBV	509118	1042178	49.87%	7.092%
38	5.905	1501	1513	1534	rBV3	21108	49330	2.36%	0.336%
39	6.066	1550	1563	1601	rBV	457952	951730	45.54%	6.476%
40	6.355	1650	1653	1658	rVB3	689	540	0.03%	0.004%
41	6.416	1670	1672	1673	rBV	306	151	0.01%	0.001%
42	6.458	1682	1685	1687	rBV2	352	214	0.01%	0.001%
43	6.497	1693	1697	1702	rBV3	401	491	0.02%	0.003%
44	6.564	1714	1718	1720	rBV	239	217	0.01%	0.001%
45	6.613	1731	1733	1736	rBV2	611	362	0.02%	0.002%
46	6.735	1769	1771	1775	rVB2	404	184	0.01%	0.001%
47	6.760	1775	1779	1781	rBV2	520	404	0.02%	0.003%
48	6.799	1789	1791	1793	rBV	217	137	0.01%	0.001%
49	6.857	1807	1809	1812	rVB	378	199	0.01%	0.001%
50	6.876	1812	1815	1817	rBV2	234	146	0.01%	0.001%
51	6.912	1820	1826	1828	rBV2	225	260	0.01%	0.002%
52	6.982	1837	1848	1876	rBV	206781	398973	19.09%	2.715%
53	7.313	1939	1951	1989	rBV	880338	1559179	74.61%	10.610%
54	7.619	2037	2046	2072	rBV	146031	267490	12.80%	1.820%
55	7.847	2114	2117	2121	rBV4	621	500	0.02%	0.003%
56	7.908	2133	2136	2138	rBV3	961	640	0.03%	0.004%
57	8.050	2177	2180	2182	rBV3	563	413	0.02%	0.003%
58	8.088	2182	2192	2233	rBV	424748	956628	45.78%	6.509%
59	8.567	2340	2341	2343	rBV	387	139	0.01%	0.001%
60	8.580	2343	2345	2349	rVB3	594	346	0.02%	0.002%
61	8.619	2355	2357	2363	rVB5	873	784	0.04%	0.005%
62	8.654	2366	2368	2372	rVV2	293	132	0.01%	0.001%
63	8.696	2377	2381	2385	rBV5	536	415	0.02%	0.003%
64	8.715	2385	2387	2390	rBV2	541	287	0.01%	0.002%
65	8.776	2402	2406	2408	rBV2	230	189	0.01%	0.001%
66	8.802	2409	2414	2416	rBV3	341	229	0.01%	0.002%
67	8.850	2417	2429	2452	rBV	810906	1300629	62.24%	8.850%
68	9.095	2501	2505	2508	rBV3	815	699	0.03%	0.005%
69	9.214	2539	2542	2544	rBV3	363	238	0.01%	0.002%
70	9.281	2561	2563	2568	rBV2	470	352	0.02%	0.002%
71	9.384	2593	2595	2597	rBV	358	153	0.01%	0.001%
72	9.481	2619	2625	2628	rBV2	382	409	0.02%	0.003%
73	9.542	2640	2644	2646	rBV3	418	364	0.02%	0.002%
74	9.600	2659	2662	2667	rVB3	636	659	0.03%	0.004%
75	9.625	2667	2670	2672	rBV2	359	211	0.01%	0.001%
76	9.641	2672	2675	2677	rBV2	471	272	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027015.D
 Acq On : 27 Jul 2022 22:17
 Operator : SY/MD
 Sample : N3897-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.844	2737	2738	2741	rBV2	287	156	0.01%	0.001%
78	9.905	2754	2757	2760	rVB2	419	197	0.01%	0.001%
79	9.928	2760	2764	2766	rBV3	937	616	0.03%	0.004%
80	9.976	2777	2779	2783	rVV	168	117	0.01%	0.001%
81	9.995	2783	2785	2788	rVB	308	171	0.01%	0.001%
82	10.214	2841	2853	2882	rVV	662989	1050405	50.26%	7.148%
83	10.362	2895	2899	2900	rBV2	697	497	0.02%	0.003%
84	10.378	2900	2904	2905	rBV	2621	1688	0.08%	0.011%
85	10.580	2963	2967	2970	rBV4	423	348	0.02%	0.002%
86	10.699	3002	3004	3007	rVV	226	119	0.01%	0.001%
87	10.760	3021	3023	3028	rBV2	365	337	0.02%	0.002%
88	10.860	3050	3054	3059	rVB4	510	429	0.02%	0.003%
89	11.008	3098	3100	3104	rVB	370	186	0.01%	0.001%
90	11.124	3133	3136	3138	rBV	234	143	0.01%	0.001%
91	11.249	3163	3175	3199	rBV	721525	1126455	53.90%	7.665%
92	11.542	3262	3266	3274	rVB6	1724	2119	0.10%	0.014%
93	11.622	3279	3291	3317	rBV	811877	1295295	61.98%	8.814%
94	12.030	3415	3418	3419	rBV	315	154	0.01%	0.001%
95	12.127	3447	3448	3449	rBV	633	169	0.01%	0.001%
96	12.455	3547	3550	3551	rBV	559	318	0.02%	0.002%
97	12.747	3639	3641	3644	rBV3	439	313	0.01%	0.002%
98	12.841	3666	3670	3673	rBV	661	477	0.02%	0.003%
99	13.017	3719	3725	3728	rBV3	688	675	0.03%	0.005%
100	13.088	3745	3747	3751	rBV	303	266	0.01%	0.002%




Sum of corrected areas: 14696015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027015.D
Acq On : 27 Jul 2022 22:17
Operator : SY/MD
Sample : N3897-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

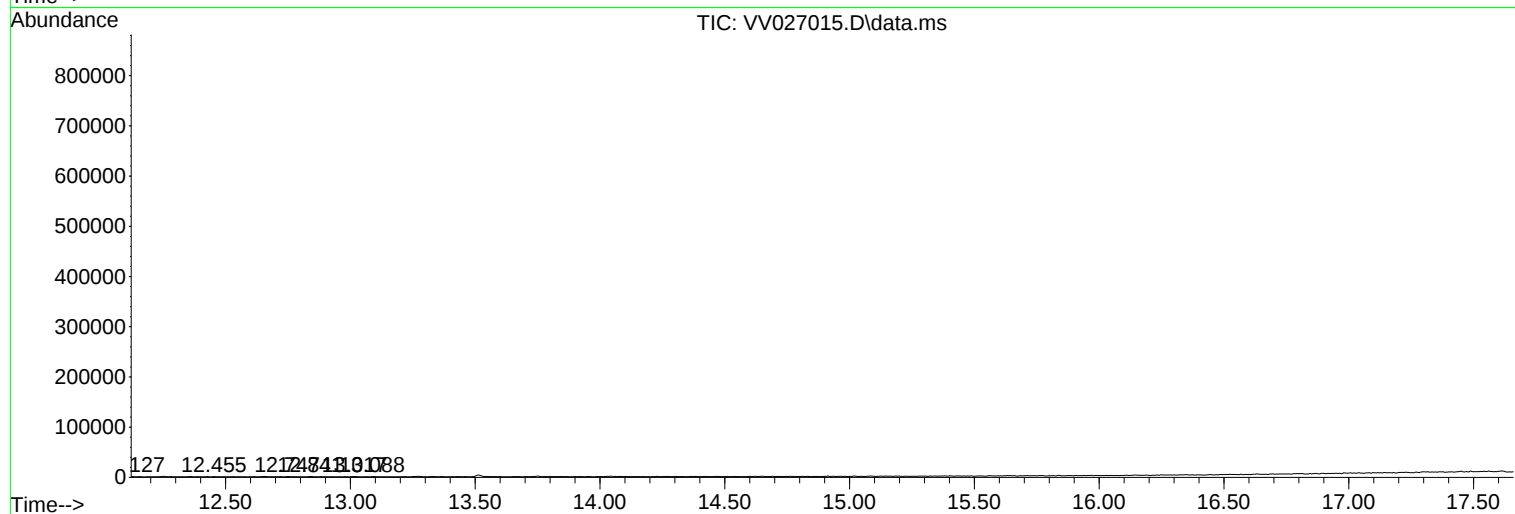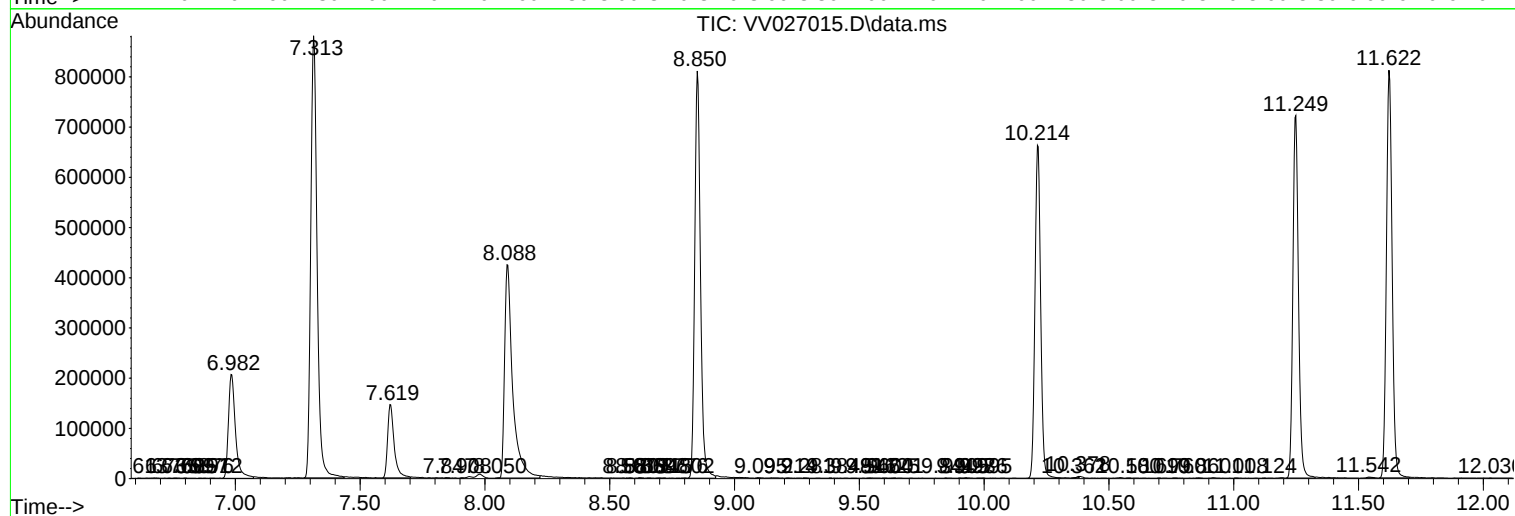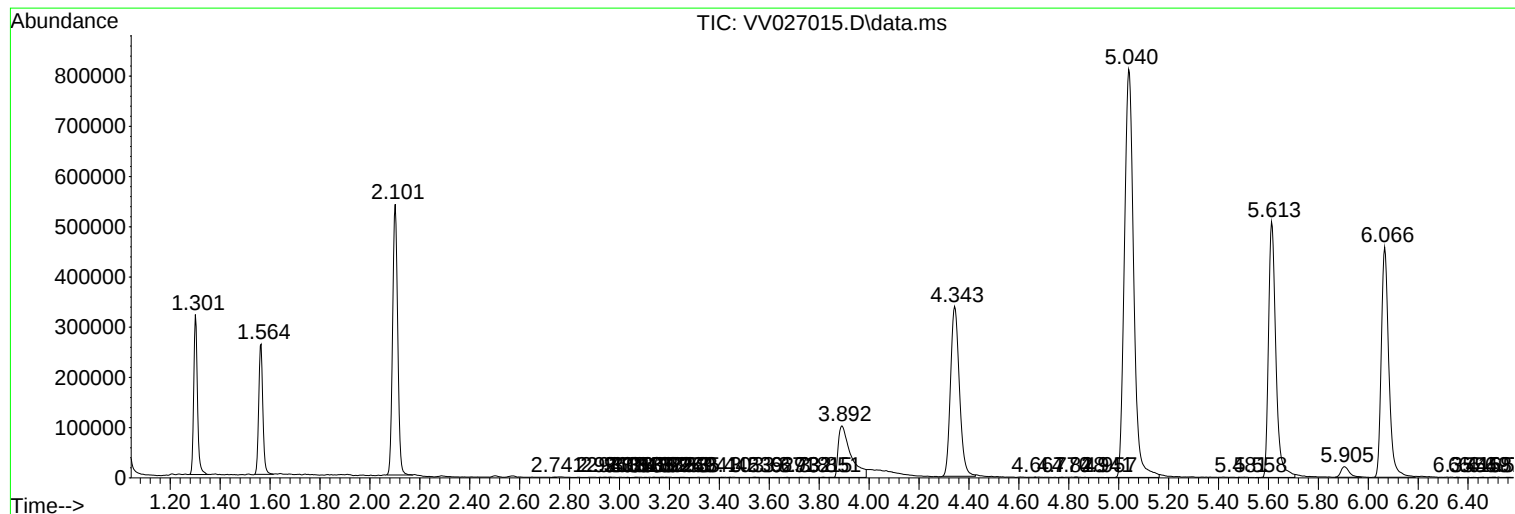

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027015.D
Acq On : 27 Jul 2022 22:17
Operator : SY/MD
Sample : N3897-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027015.D
Acq On : 27 Jul 2022 22:17
Operator : SY/MD
Sample : N3897-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc