

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027019.D
 Acq On : 27 Jul 2022 23:55
 Operator : SY/MD
 Sample : N3880-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rBV	319501	334529	15.56%	2.079%
2	1.565	156	163	178	rVB	266194	303939	14.14%	1.889%
3	2.102	320	330	346	rVB	555169	789057	36.71%	4.903%
4	2.503	446	455	466	rVB	10797	17788	0.83%	0.111%
5	2.616	481	490	504	rVB7	1969	4603	0.21%	0.029%
6	2.764	529	536	540	rBV4	1387	1574	0.07%	0.010%
7	3.073	629	632	637	rVB4	521	331	0.02%	0.002%
8	3.098	637	640	642	rBV2	467	308	0.01%	0.002%
9	3.114	642	645	649	rVB2	493	356	0.02%	0.002%
10	3.253	685	688	694	rVV3	386	401	0.02%	0.002%
11	3.442	742	747	751	rBV3	302	338	0.02%	0.002%
12	3.491	759	762	765	rVB2	436	299	0.01%	0.002%
13	3.683	819	822	829	rVB2	356	382	0.02%	0.002%
14	3.892	876	887	935	rBV2	113182	482618	22.45%	2.999%
15	4.343	1010	1027	1060	rBV	345156	857180	39.87%	5.327%
16	4.597	1100	1106	1111	rBV5	559	801	0.04%	0.005%
17	4.745	1148	1152	1156	rVB3	635	625	0.03%	0.004%
18	4.786	1160	1165	1168	rBV3	539	484	0.02%	0.003%
19	4.896	1195	1199	1203	rVB2	654	422	0.02%	0.003%
20	4.915	1203	1205	1211	rVB	458	287	0.01%	0.002%
21	5.044	1228	1245	1290	rBV2	832207	2149673	100.00%	13.358%
22	5.224	1298	1301	1304	rBV2	867	694	0.03%	0.004%
23	5.285	1317	1320	1325	rVB5	429	306	0.01%	0.002%
24	5.333	1332	1335	1338	rBV3	511	341	0.02%	0.002%
25	5.407	1353	1358	1363	rVB4	606	694	0.03%	0.004%
26	5.526	1389	1395	1398	rBV2	442	398	0.02%	0.002%
27	5.613	1410	1422	1461	rBV	523411	1082518	50.36%	6.727%
28	5.912	1501	1515	1535	rVB10	13883	35525	1.65%	0.221%
29	5.998	1539	1542	1549	rBV6	689	685	0.03%	0.004%
30	6.066	1549	1563	1597	rBV	466900	971564	45.20%	6.037%
31	6.330	1641	1645	1647	rBV3	568	432	0.02%	0.003%
32	6.416	1670	1672	1676	rVB2	491	346	0.02%	0.002%
33	6.442	1677	1680	1684	rVB3	617	424	0.02%	0.003%
34	6.471	1684	1689	1691	rBV3	510	364	0.02%	0.002%
35	6.503	1695	1699	1704	rBV4	610	702	0.03%	0.004%
36	6.600	1725	1729	1735	rVB3	442	487	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027019.D
 Acq On : 27 Jul 2022 23:55
 Operator : SY/MD
 Sample : N3880-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.638	1735	1741	1744	rBV2	420	479	0.02%	0.003%
38	6.693	1754	1758	1765	rVB3	812	1096	0.05%	0.007%
39	6.725	1765	1768	1771	rBV2	599	323	0.02%	0.002%
40	6.751	1771	1776	1780	rBV3	661	616	0.03%	0.004%
41	6.777	1780	1784	1787	rBV3	372	326	0.02%	0.002%
42	6.796	1787	1790	1795	rVB3	410	338	0.02%	0.002%
43	6.831	1795	1801	1803	rBV3	387	319	0.01%	0.002%
44	6.937	1829	1834	1837	rBV2	414	426	0.02%	0.003%
45	6.982	1837	1848	1879	rBV	204955	399841	18.60%	2.485%
46	7.198	1912	1915	1918	rBV3	731	557	0.03%	0.003%
47	7.314	1939	1951	1982	rBV	907446	1602644	74.55%	9.959%
48	7.619	2034	2046	2071	rBV	144495	267090	12.42%	1.660%
49	7.860	2118	2121	2126	rVV6	783	690	0.03%	0.004%
50	7.921	2137	2140	2141	rBV	656	298	0.01%	0.002%
51	7.973	2141	2156	2180	rBV	465842	792227	36.85%	4.923%
52	8.088	2182	2192	2237	rVV	463692	939532	43.71%	5.838%
53	8.596	2346	2350	2354	rVB2	404	306	0.01%	0.002%
54	8.635	2360	2362	2368	rVB4	504	370	0.02%	0.002%
55	8.709	2379	2385	2387	rBV3	523	413	0.02%	0.003%
56	8.850	2415	2429	2458	rBV	824110	1338495	62.27%	8.318%
57	9.018	2479	2481	2485	rVB3	550	290	0.01%	0.002%
58	9.143	2517	2520	2524	rVB3	555	354	0.02%	0.002%
59	9.545	2639	2645	2649	rBV4	560	658	0.03%	0.004%
60	9.645	2670	2676	2680	rBV3	392	434	0.02%	0.003%
61	9.670	2680	2684	2690	rVV3	398	449	0.02%	0.003%
62	9.706	2693	2695	2701	rVB2	474	321	0.01%	0.002%
63	9.799	2722	2724	2731	rVB4	472	442	0.02%	0.003%
64	9.863	2742	2744	2751	rVB	525	431	0.02%	0.003%
65	9.931	2758	2765	2767	rBV2	667	730	0.03%	0.005%
66	10.214	2840	2853	2880	rBV	691430	1088288	50.63%	6.763%
67	10.471	2930	2933	2936	rBV2	409	293	0.01%	0.002%
68	10.577	2963	2966	2969	rBV	611	412	0.02%	0.003%
69	10.593	2969	2971	2976	rVB4	463	416	0.02%	0.003%
70	10.664	2990	2993	2997	rBV2	388	345	0.02%	0.002%
71	10.886	3058	3062	3065	rVB2	450	302	0.01%	0.002%
72	11.021	3100	3104	3110	rVB	471	340	0.02%	0.002%
73	11.246	3163	3174	3196	rBV	769001	1197925	55.73%	7.444%
74	11.368	3210	3212	3216	rVV4	813	515	0.02%	0.003%
75	11.387	3216	3218	3223	rVB4	869	462	0.02%	0.003%
76	11.622	3278	3291	3316	rBV	883244	1371509	63.80%	8.523%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027019.D
 Acq On : 27 Jul 2022 23:55
 Operator : SY/MD
 Sample : N3880-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.796	3343	3345	3351	rVB4	586	312	0.01%	0.002%
78	11.985	3401	3404	3409	rBV3	425	380	0.02%	0.002%
79	12.381	3521	3527	3535	rVB4	2668	3433	0.16%	0.021%
80	12.503	3562	3565	3571	rVB3	639	645	0.03%	0.004%
81	12.548	3573	3579	3582	rBV2	411	514	0.02%	0.003%
82	12.654	3608	3612	3618	rVB3	1094	918	0.04%	0.006%
83	12.731	3632	3636	3640	rBV3	692	720	0.03%	0.004%
84	12.889	3682	3685	3688	rVB	734	428	0.02%	0.003%
85	12.960	3702	3707	3715	rVB7	1625	2512	0.12%	0.016%
86	13.159	3760	3769	3781	rBV8	8035	13051	0.61%	0.081%
87	13.265	3798	3802	3803	rBV2	844	514	0.02%	0.003%
88	13.349	3825	3828	3829	rBV2	594	367	0.02%	0.002%
89	13.394	3840	3842	3845	rVB2	677	314	0.01%	0.002%
90	13.477	3864	3868	3870	rBV4	641	500	0.02%	0.003%
91	13.513	3872	3879	3888	rVB4	4811	7156	0.33%	0.044%
92	13.757	3951	3955	3957	rBV3	542	405	0.02%	0.003%
93	13.796	3963	3967	3969	rBV3	500	375	0.02%	0.002%
94	13.857	3979	3986	3989	rBV3	721	976	0.05%	0.006%
95	13.915	3997	4004	4009	rBV5	667	913	0.04%	0.006%
96	14.214	4094	4097	4103	rVB3	472	404	0.02%	0.003%
97	14.246	4103	4107	4109	rBV3	371	348	0.02%	0.002%
98	14.644	4224	4231	4234	rBV4	1730	2428	0.11%	0.015%
99	14.818	4280	4285	4286	rBV2	1101	872	0.04%	0.005%
100	15.149	4383	4388	4391	rBV4	1182	1128	0.05%	0.007%

Sum of corrected areas: 16092390




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027019.D
Acq On : 27 Jul 2022 23:55
Operator : SY/MD
Sample : N3880-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

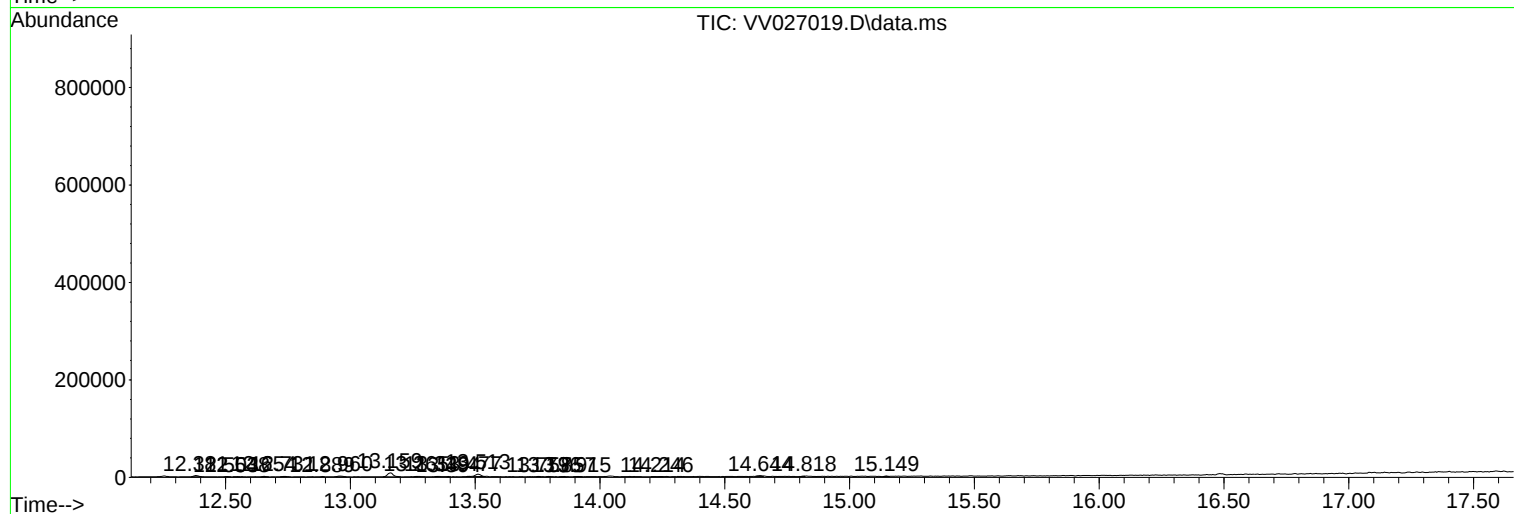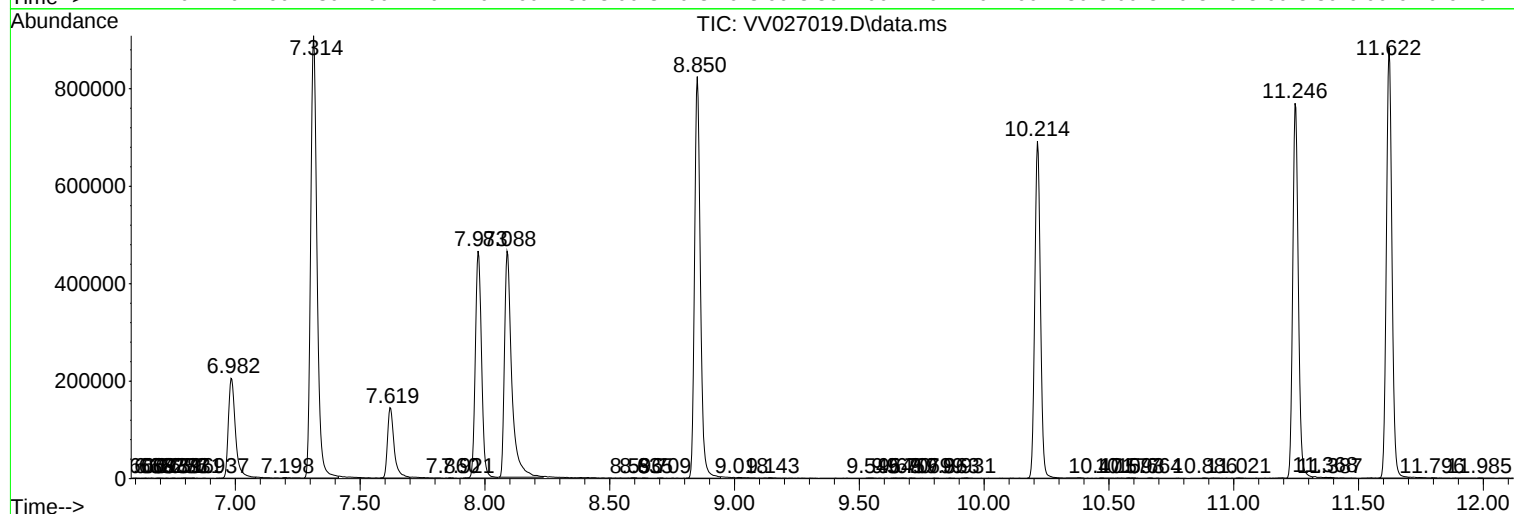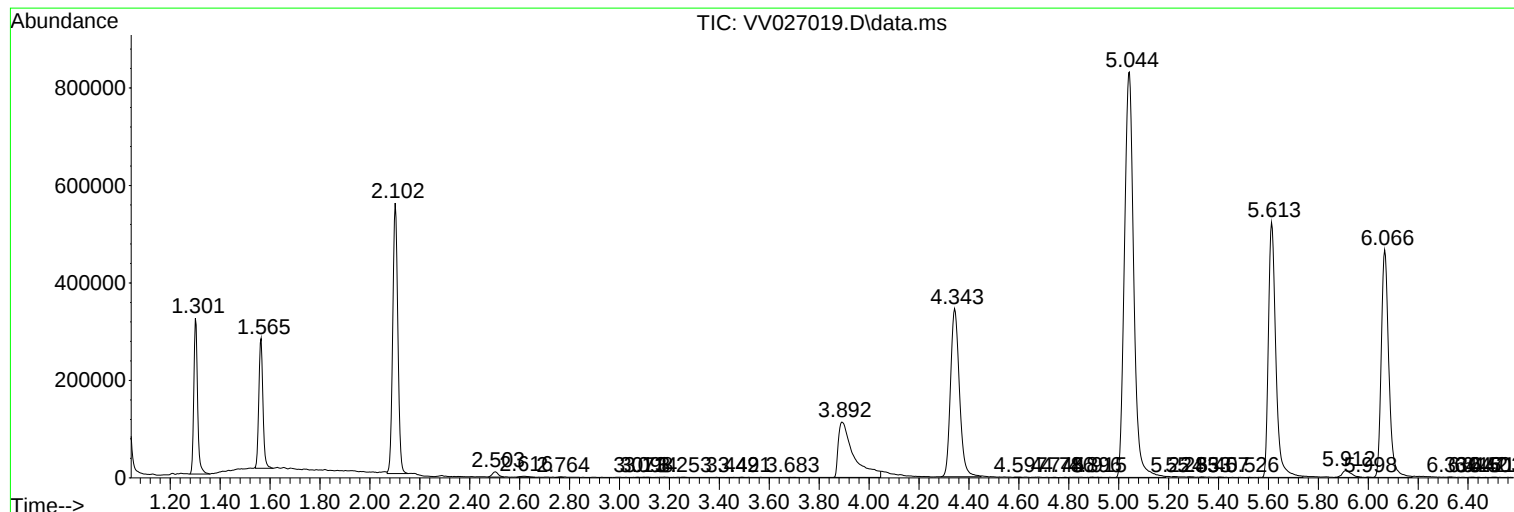

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027019.D
Acq On : 27 Jul 2022 23:55
Operator : SY/MD
Sample : N3880-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027019.D
Acq On : 27 Jul 2022 23:55
Operator : SY/MD
Sample : N3880-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------