

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027020.D
 Acq On : 28 Jul 2022 00:20
 Operator : SY/MD
 Sample : N3880-11DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	304951	313944	15.22%	1.977%
2	1.564	156	163	177	rVB	254142	288950	14.01%	1.819%
3	2.101	321	330	347	rVB	516026	730869	35.43%	4.601%
4	2.883	571	573	575	rVB2	305	115	0.01%	0.001%
5	2.982	602	604	607	rBV2	438	207	0.01%	0.001%
6	3.085	634	636	637	rBV	327	140	0.01%	0.001%
7	3.239	680	684	687	rVB2	358	262	0.01%	0.002%
8	3.265	688	692	693	rBV	222	152	0.01%	0.001%
9	3.326	707	711	714	rBV2	184	203	0.01%	0.001%
10	3.381	724	728	733	rBV2	247	265	0.01%	0.002%
11	3.458	749	752	754	rBV2	334	181	0.01%	0.001%
12	3.497	760	764	768	rVB3	268	205	0.01%	0.001%
13	3.584	788	791	793	rBV	173	134	0.01%	0.001%
14	3.625	801	804	807	rBV	550	265	0.01%	0.002%
15	3.690	822	824	828	rVB2	549	247	0.01%	0.002%
16	3.744	836	841	844	rBV2	226	228	0.01%	0.001%
17	3.844	869	872	875	rVB2	490	282	0.01%	0.002%
18	3.902	875	890	964	rBV5	138967	666685	32.32%	4.197%
19	4.342	1012	1027	1049	rBV	333741	823664	39.93%	5.186%
20	4.606	1106	1109	1111	rBV3	658	408	0.02%	0.003%
21	4.645	1119	1121	1122	rBV	465	131	0.01%	0.001%
22	4.741	1149	1151	1153	rVB	481	200	0.01%	0.001%
23	4.757	1153	1156	1158	rBV2	535	340	0.02%	0.002%
24	4.815	1170	1174	1175	rBV	386	201	0.01%	0.001%
25	4.831	1175	1179	1185	rVB3	619	661	0.03%	0.004%
26	4.940	1210	1213	1217	rVV2	393	330	0.02%	0.002%
27	4.979	1222	1225	1228	rBV3	320	213	0.01%	0.001%
28	5.040	1228	1244	1299	rBV2	793310	2062972	100.00%	12.988%
29	5.548	1398	1402	1403	rBV2	455	266	0.01%	0.002%
30	5.558	1403	1405	1408	rBV3	251	135	0.01%	0.001%
31	5.612	1409	1422	1460	rBV	485899	1016409	49.27%	6.399%
32	5.915	1502	1516	1535	rBV2	70573	156817	7.60%	0.987%
33	6.066	1548	1563	1592	rBV	450913	941644	45.65%	5.928%
34	6.336	1645	1647	1652	rVB4	496	332	0.02%	0.002%
35	6.384	1659	1662	1664	rBV2	518	384	0.02%	0.002%
36	6.429	1674	1676	1680	rVB2	390	212	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027020.D
 Acq On : 28 Jul 2022 00:20
 Operator : SY/MD
 Sample : N3880-11DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.452	1680	1683	1684	rBV2	227	138	0.01%	0.001%
38	6.506	1695	1700	1701	rBV2	427	262	0.01%	0.002%
39	6.574	1719	1721	1723	rBV	210	107	0.01%	0.001%
40	6.622	1733	1736	1738	rBV2	415	242	0.01%	0.002%
41	6.709	1760	1763	1764	rBV	491	312	0.02%	0.002%
42	6.802	1787	1792	1796	rBV3	371	448	0.02%	0.003%
43	6.828	1798	1800	1802	rVB2	295	118	0.01%	0.001%
44	6.850	1804	1807	1810	rBV2	313	211	0.01%	0.001%
45	6.985	1836	1849	1877	rBV	197244	378372	18.34%	2.382%
46	7.201	1913	1916	1918	rBV3	690	522	0.03%	0.003%
47	7.313	1939	1951	1974	rBV	840720	1477615	71.63%	9.303%
48	7.619	2037	2046	2078	rBV	139233	255599	12.39%	1.609%
49	7.831	2110	2112	2114	rBV2	457	215	0.01%	0.001%
50	7.972	2140	2156	2183	rBV	697673	1190971	57.73%	7.498%
51	8.091	2183	2193	2232	rVV	444077	923084	44.75%	5.811%
52	8.484	2313	2315	2317	rBV	532	267	0.01%	0.002%
53	8.680	2374	2376	2378	rBV2	424	254	0.01%	0.002%
54	8.718	2385	2388	2391	rVB3	330	180	0.01%	0.001%
55	8.763	2399	2402	2405	rBV2	401	302	0.01%	0.002%
56	8.805	2411	2415	2417	rBV2	490	440	0.02%	0.003%
57	8.850	2417	2429	2462	rVV	757358	1246517	60.42%	7.848%
58	9.181	2530	2532	2538	rVB3	482	330	0.02%	0.002%
59	9.210	2538	2541	2546	rVB3	495	429	0.02%	0.003%
60	9.242	2546	2551	2554	rBV4	566	575	0.03%	0.004%
61	9.307	2569	2571	2575	rBV3	237	146	0.01%	0.001%
62	9.352	2581	2585	2586	rBV	413	265	0.01%	0.002%
63	9.448	2612	2615	2617	rBV	426	251	0.01%	0.002%
64	9.477	2622	2624	2627	rBV2	223	106	0.01%	0.001%
65	9.548	2642	2646	2647	rBV	667	447	0.02%	0.003%
66	9.590	2657	2659	2664	rVB5	515	409	0.02%	0.003%
67	9.619	2664	2668	2671	rBV3	431	299	0.01%	0.002%
68	9.632	2671	2672	2675	rBV	237	117	0.01%	0.001%
69	9.705	2687	2695	2697	rBV3	383	486	0.02%	0.003%
70	9.744	2705	2707	2709	rBV3	243	125	0.01%	0.001%
71	9.786	2717	2720	2723	rBV3	310	253	0.01%	0.002%
72	9.824	2728	2732	2734	rBV	320	246	0.01%	0.002%
73	9.853	2737	2741	2743	rBV3	644	465	0.02%	0.003%
74	9.889	2749	2752	2754	rBV	311	150	0.01%	0.001%
75	9.943	2760	2769	2774	rBV2	635	778	0.04%	0.005%
76	10.004	2784	2788	2791	rBV3	386	284	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027020.D
 Acq On : 28 Jul 2022 00:20
 Operator : SY/MD
 Sample : N3880-11DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.024	2791	2794	2796	rVB2	372	219	0.01%	0.001%
78	10.053	2796	2803	2806	rVB3	327	363	0.02%	0.002%
79	10.072	2806	2809	2811	rBV	386	276	0.01%	0.002%
80	10.104	2816	2819	2822	rBV4	300	216	0.01%	0.001%
81	10.172	2836	2840	2841	rBV2	488	302	0.01%	0.002%
82	10.213	2841	2853	2878	rVV	670534	1065845	51.67%	6.710%
83	10.451	2925	2927	2930	rVB3	458	177	0.01%	0.001%
84	10.615	2974	2978	2982	rBV2	399	457	0.02%	0.003%
85	10.818	3038	3041	3042	rBV2	272	148	0.01%	0.001%
86	10.853	3048	3052	3057	rBV3	765	626	0.03%	0.004%
87	10.921	3067	3073	3075	rBV2	733	622	0.03%	0.004%
88	11.046	3108	3112	3114	rBV2	348	277	0.01%	0.002%
89	11.133	3136	3139	3143	rBV2	353	215	0.01%	0.001%
90	11.249	3163	3175	3203	rBV	689763	1072766	52.00%	6.754%
91	11.545	3263	3267	3268	rBV2	457	387	0.02%	0.002%
92	11.622	3279	3291	3316	rBV	797288	1246083	60.40%	7.845%
93	12.043	3420	3422	3423	rBV	368	181	0.01%	0.001%
94	12.336	3510	3513	3516	rBV3	347	287	0.01%	0.002%
95	12.625	3597	3603	3607	rBV2	634	705	0.03%	0.004%
96	12.895	3685	3687	3688	rBV2	336	120	0.01%	0.001%
97	12.937	3698	3700	3702	rBV2	502	196	0.01%	0.001%
98	13.046	3732	3734	3736	rVB	740	193	0.01%	0.001%
99	13.159	3765	3769	3773	rBV4	2015	1864	0.09%	0.012%
100	13.300	3811	3813	3816	rBV	426	281	0.01%	0.002%




Sum of corrected areas: 15883796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027020.D
Acq On : 28 Jul 2022 00:20
Operator : SY/MD
Sample : N3880-11DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

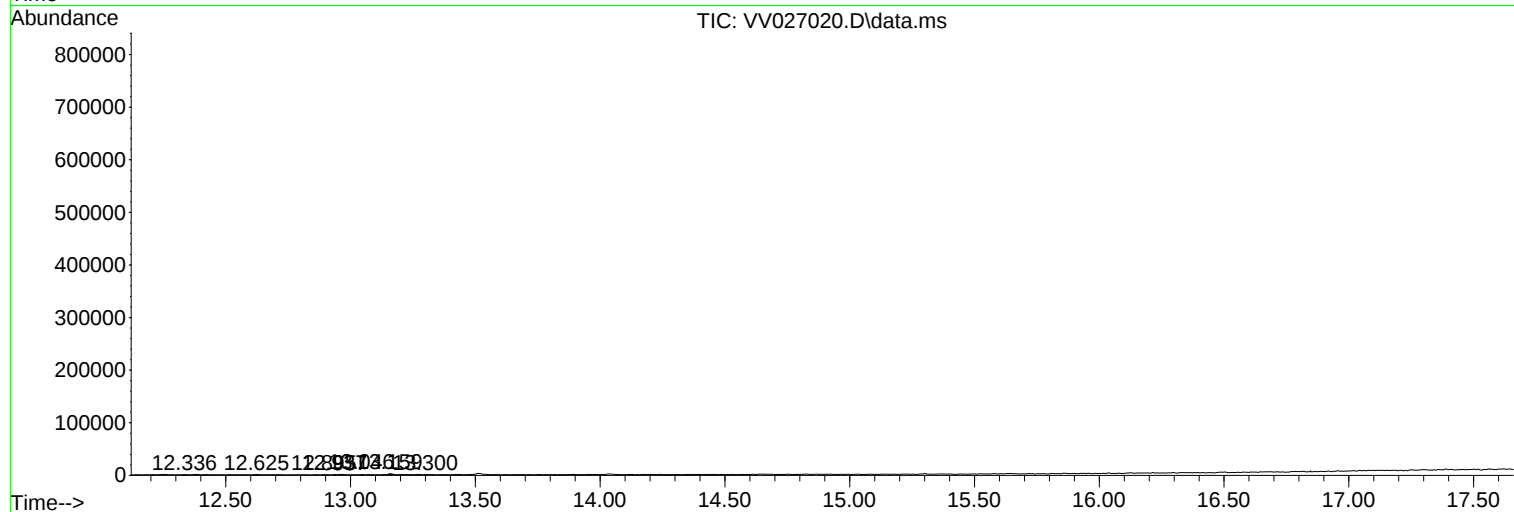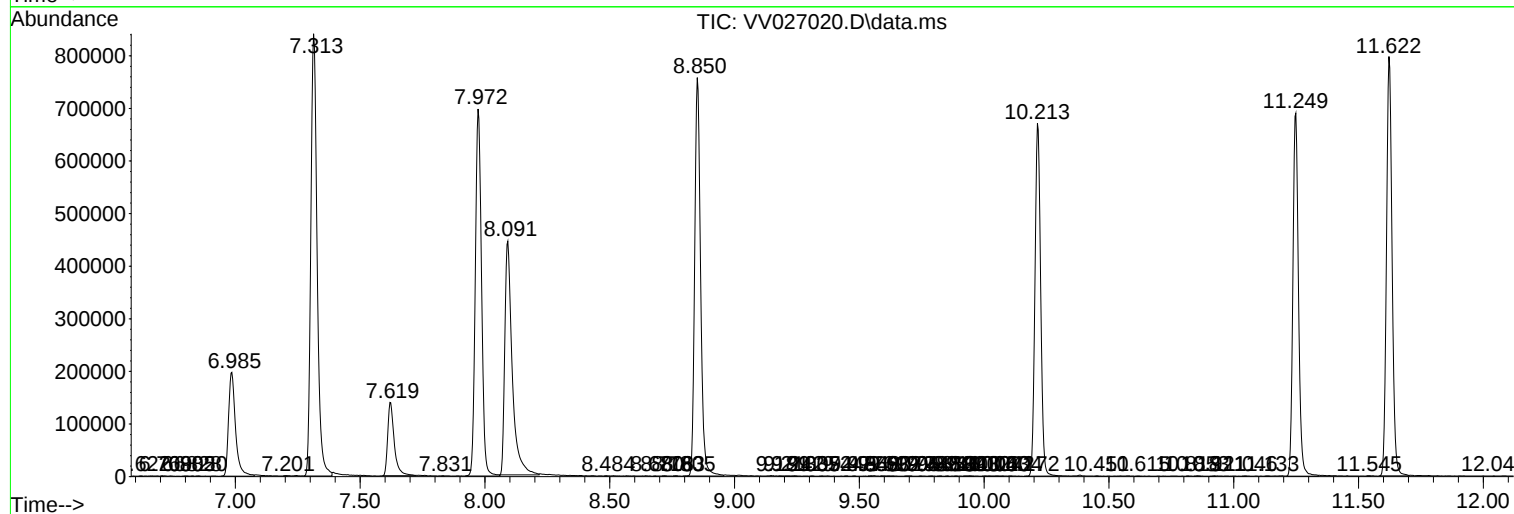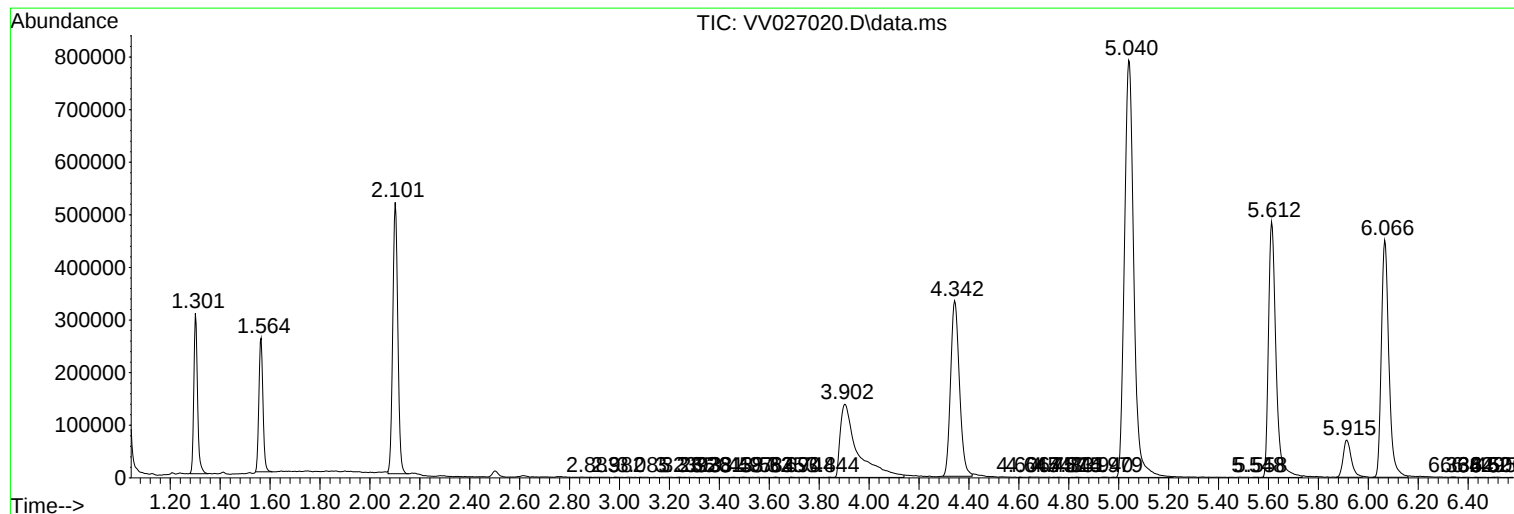

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027020.D
Acq On : 28 Jul 2022 00:20
Operator : SY/MD
Sample : N3880-11DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027020.D
Acq On : 28 Jul 2022 00:20
Operator : SY/MD
Sample : N3880-11DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc