

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027021.D
 Acq On : 28 Jul 2022 00:44
 Operator : SY/MD
 Sample : N3880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rVB	318044	326275	15.82%	2.091%
2	1.564	155	163	174	rBV	251834	294546	14.28%	1.887%
3	2.101	320	330	347	rVB	515178	732067	35.49%	4.691%
4	2.404	421	424	429	rVB5	977	734	0.04%	0.005%
5	2.503	445	455	469	rBV5	14101	25648	1.24%	0.164%
6	2.908	576	581	584	rBV2	453	394	0.02%	0.003%
7	2.969	592	600	604	rBV3	355	549	0.03%	0.004%
8	3.008	607	612	613	rBV2	356	321	0.02%	0.002%
9	3.031	613	619	635	rVB7	1454	2655	0.13%	0.017%
10	3.175	659	664	666	rBV3	449	377	0.02%	0.002%
11	3.304	699	704	706	rBV2	554	460	0.02%	0.003%
12	3.342	713	716	722	rBV2	407	438	0.02%	0.003%
13	3.510	764	768	771	rBV3	369	345	0.02%	0.002%
14	3.564	781	785	790	rVB2	408	355	0.02%	0.002%
15	3.596	790	795	801	rBV3	398	448	0.02%	0.003%
16	3.764	833	847	857	rVB6	3116	7077	0.34%	0.045%
17	3.899	874	889	926	rBV2	104062	486417	23.58%	3.117%
18	4.342	1010	1027	1050	rBV	329143	825543	40.02%	5.290%
19	4.664	1115	1127	1140	rBV7	3890	8873	0.43%	0.057%
20	4.744	1146	1152	1156	rVB5	468	443	0.02%	0.003%
21	4.812	1170	1173	1177	rVB4	651	572	0.03%	0.004%
22	4.834	1177	1180	1184	rBV2	803	770	0.04%	0.005%
23	4.860	1184	1188	1191	rBV2	404	290	0.01%	0.002%
24	4.879	1191	1194	1198	rVV3	478	340	0.02%	0.002%
25	5.040	1227	1244	1288	rBV2	787454	2063014	100.00%	13.219%
26	5.378	1344	1349	1350	rBV2	586	429	0.02%	0.003%
27	5.436	1364	1367	1370	rVB3	625	419	0.02%	0.003%
28	5.529	1394	1396	1401	rVB2	335	302	0.01%	0.002%
29	5.567	1401	1408	1410	rBV2	443	416	0.02%	0.003%
30	5.612	1410	1422	1456	rBV	463599	967345	46.89%	6.198%
31	5.915	1503	1516	1539	rVB7	28345	68337	3.31%	0.438%
32	6.066	1549	1563	1603	rBV	449068	950619	46.08%	6.091%
33	6.284	1629	1631	1634	rBV3	473	305	0.01%	0.002%
34	6.368	1654	1657	1660	rBV2	493	304	0.01%	0.002%
35	6.439	1674	1679	1681	rBV4	414	346	0.02%	0.002%
36	6.509	1697	1701	1704	rVB3	475	385	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027021.D
 Acq On : 28 Jul 2022 00:44
 Operator : SY/MD
 Sample : N3880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.538	1706	1710	1715	rVB4	321	300	0.01%	0.002%
38	6.821	1794	1798	1800	rBV2	390	289	0.01%	0.002%
39	6.850	1804	1807	1812	rVB2	580	414	0.02%	0.003%
40	6.985	1837	1849	1872	rBV	196268	372639	18.06%	2.388%
41	7.243	1926	1929	1933	rVV5	729	579	0.03%	0.004%
42	7.313	1938	1951	1984	rBV	831721	1482769	71.87%	9.501%
43	7.522	2014	2016	2019	rVB4	798	325	0.02%	0.002%
44	7.548	2022	2024	2028	rVB2	777	389	0.02%	0.002%
45	7.622	2036	2047	2079	rBV	135541	256177	12.42%	1.641%
46	7.863	2119	2122	2124	rBV4	543	401	0.02%	0.003%
47	7.972	2141	2156	2178	rVV	758785	1296527	62.85%	8.308%
48	8.091	2183	2193	2233	rVV	434687	922150	44.70%	5.909%
49	8.657	2364	2369	2372	rBV2	684	653	0.03%	0.004%
50	8.715	2381	2387	2389	rBV2	661	508	0.02%	0.003%
51	8.741	2391	2395	2398	rVB	426	322	0.02%	0.002%
52	8.767	2398	2403	2405	rBV3	339	299	0.01%	0.002%
53	8.850	2417	2429	2453	rBV	714930	1182049	57.30%	7.574%
54	9.146	2513	2521	2537	rBV3	8243	15396	0.75%	0.099%
55	9.220	2542	2544	2549	rBV3	326	336	0.02%	0.002%
56	9.519	2634	2637	2640	rBV	462	335	0.02%	0.002%
57	9.783	2716	2719	2723	rVB	512	386	0.02%	0.002%
58	9.815	2723	2729	2731	rBV	538	477	0.02%	0.003%
59	9.921	2758	2762	2763	rBV	925	463	0.02%	0.003%
60	9.988	2780	2783	2788	rBV2	358	353	0.02%	0.002%
61	10.214	2840	2853	2875	rBV	675351	1067171	51.73%	6.838%
62	10.377	2901	2904	2912	rVB6	1088	1233	0.06%	0.008%
63	10.423	2916	2918	2924	rVB2	343	353	0.02%	0.002%
64	10.468	2924	2932	2935	rBV2	338	321	0.02%	0.002%
65	10.493	2937	2940	2944	rVB2	458	321	0.02%	0.002%
66	10.545	2945	2956	2965	rBV3	2932	4834	0.23%	0.031%
67	10.580	2965	2967	2973	rVB2	787	668	0.03%	0.004%
68	10.815	3036	3040	3043	rBV2	348	295	0.01%	0.002%
69	10.921	3066	3073	3081	rVB3	2731	4032	0.20%	0.026%
70	11.037	3103	3109	3114	rVB3	401	443	0.02%	0.003%
71	11.069	3114	3119	3123	rBV2	425	515	0.02%	0.003%
72	11.191	3154	3157	3161	rBV3	494	337	0.02%	0.002%
73	11.249	3163	3175	3199	rBV	623821	978370	47.42%	6.269%
74	11.622	3279	3291	3309	rBV	770589	1229583	59.60%	7.879%
75	11.731	3322	3325	3329	rBV3	716	599	0.03%	0.004%
76	11.921	3380	3384	3390	rBV3	620	648	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027021.D
 Acq On : 28 Jul 2022 00:44
 Operator : SY/MD
 Sample : N3880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.947	3390	3392	3396	rBV2	406	294	0.01%	0.002%
78	12.255	3485	3488	3496	rVB3	852	809	0.04%	0.005%
79	12.291	3496	3499	3502	rBV2	426	351	0.02%	0.002%
80	12.410	3534	3536	3541	rVV3	492	312	0.02%	0.002%
81	12.995	3716	3718	3722	rVB3	569	312	0.02%	0.002%
82	13.014	3722	3724	3729	rBV2	361	306	0.01%	0.002%
83	13.082	3742	3745	3748	rBV2	483	336	0.02%	0.002%
84	13.165	3769	3771	3779	rVB4	694	655	0.03%	0.004%
85	13.271	3800	3804	3806	rBV2	477	325	0.02%	0.002%
86	13.332	3817	3823	3825	rBV2	451	462	0.02%	0.003%
87	13.352	3825	3829	3833	rVB4	316	394	0.02%	0.003%
88	13.516	3876	3880	3887	rVB3	1471	1439	0.07%	0.009%
89	13.747	3949	3952	3958	rVB4	745	692	0.03%	0.004%
90	13.885	3991	3995	3999	rBV2	650	609	0.03%	0.004%
91	13.966	4018	4020	4024	rBV3	541	488	0.02%	0.003%
92	14.040	4040	4043	4051	rVB4	1315	1348	0.07%	0.009%
93	14.252	4106	4109	4111	rBV2	577	330	0.02%	0.002%
94	14.287	4116	4120	4124	rBV2	501	581	0.03%	0.004%
95	14.573	4206	4209	4212	rVB2	577	367	0.02%	0.002%
96	14.602	4212	4218	4223	rVB4	794	933	0.05%	0.006%
97	14.647	4223	4232	4233	rBV4	1064	1374	0.07%	0.009%
98	15.162	4389	4392	4398	rBV2	703	607	0.03%	0.004%
99	15.268	4422	4425	4427	rBV2	628	476	0.02%	0.003%
100	15.342	4446	4448	4450	rBV2	803	451	0.02%	0.003%


Sum of corrected areas: 15606668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027021.D
Acq On : 28 Jul 2022 00:44
Operator : SY/MD
Sample : N3880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

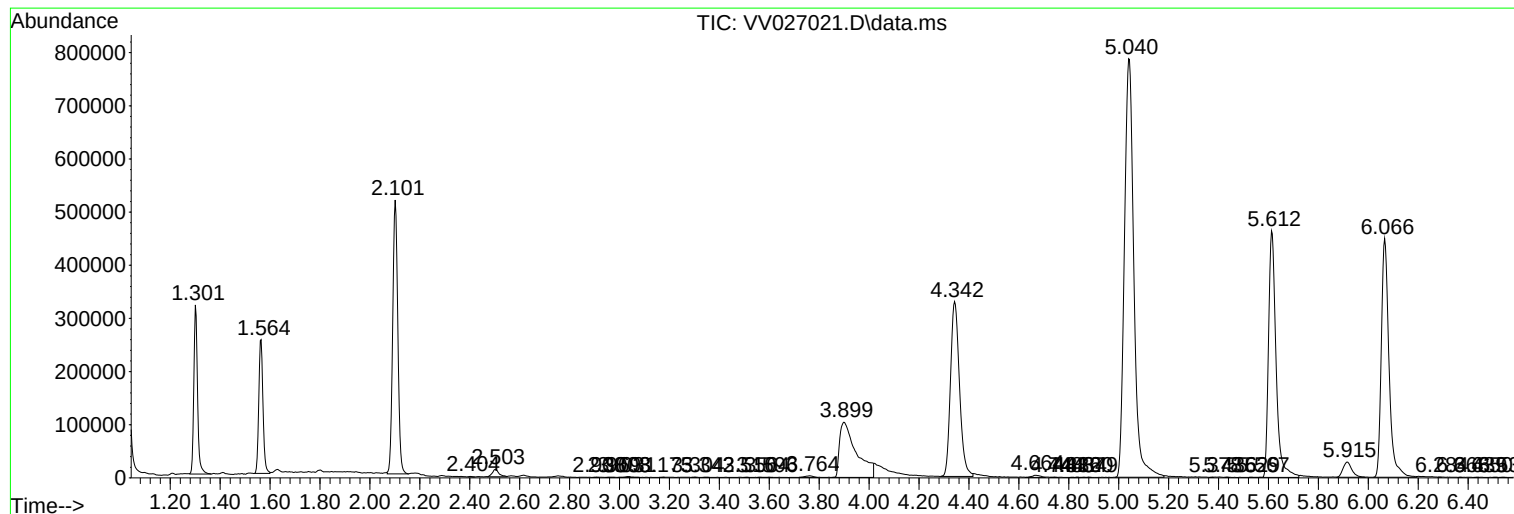

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027021.D
Acq On : 28 Jul 2022 00:44
Operator : SY/MD
Sample : N3880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027021.D
Acq On : 28 Jul 2022 00:44
Operator : SY/MD
Sample : N3880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc