

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV0727022.D
 Acq On : 28 Jul 2022 01:09
 Operator : SY/MD
 Sample : N3880-13DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV0727022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	102	rVB	305918	321569	15.76%	2.083%
2	1.564	155	163	180	rBV	253209	292416	14.33%	1.894%
3	2.101	320	330	348	rVB	527915	751937	36.85%	4.870%
4	2.503	446	455	468	rVB2	12143	20414	1.00%	0.132%
5	2.613	477	489	498	rBV4	3529	7249	0.36%	0.047%
6	2.728	522	525	528	rVB2	486	325	0.02%	0.002%
7	2.754	529	533	537	rBV3	862	843	0.04%	0.005%
8	2.789	542	544	548	rBV3	503	264	0.01%	0.002%
9	2.957	593	596	598	rVV3	434	250	0.01%	0.002%
10	3.050	621	625	628	rBV2	355	352	0.02%	0.002%
11	3.150	652	656	658	rBV	346	296	0.01%	0.002%
12	3.400	731	734	738	rVB3	387	303	0.01%	0.002%
13	3.423	738	741	745	rBV	343	295	0.01%	0.002%
14	3.561	780	784	790	rVV3	263	255	0.01%	0.002%
15	3.680	818	821	828	rVB3	231	313	0.02%	0.002%
16	3.731	833	837	841	rVB3	333	309	0.02%	0.002%
17	3.770	841	849	852	rBV	293	367	0.02%	0.002%
18	3.895	874	888	922	rBV2	110790	449850	22.04%	2.914%
19	4.342	1011	1027	1059	rBV	331848	822666	40.31%	5.329%
20	4.584	1099	1102	1106	rVB4	418	265	0.01%	0.002%
21	4.629	1111	1116	1120	rBV4	334	389	0.02%	0.003%
22	4.699	1131	1138	1142	rVB5	586	696	0.03%	0.005%
23	4.731	1142	1148	1150	rVB2	555	543	0.03%	0.004%
24	4.892	1194	1198	1202	rBV3	586	530	0.03%	0.003%
25	4.918	1202	1206	1207	rBV	462	301	0.01%	0.002%
26	4.963	1217	1220	1222	rVB2	366	255	0.01%	0.002%
27	5.040	1227	1244	1296	rBV2	780468	2040791	100.00%	13.218%
28	5.265	1311	1314	1319	rVB4	812	632	0.03%	0.004%
29	5.339	1333	1337	1341	rVB3	811	655	0.03%	0.004%
30	5.612	1409	1422	1462	rBV	482394	1010656	49.52%	6.546%
31	5.911	1504	1515	1540	rVB7	14090	36815	1.80%	0.238%
32	6.001	1540	1543	1547	rBV4	685	534	0.03%	0.003%
33	6.066	1549	1563	1601	rBV	450283	930634	45.60%	6.028%
34	6.278	1627	1629	1632	rVB3	620	302	0.01%	0.002%
35	6.339	1646	1648	1651	rBV3	558	302	0.01%	0.002%
36	6.362	1651	1655	1656	rBV3	333	249	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072722\
 Data File : VW072702.D
 Acq On : 28 Jul 2022 01:09
 Operator : SY/MD
 Sample : N3880-13DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.513	1696	1702	1704	rBV2	629	600	0.03%	0.004%
38	6.558	1714	1716	1721	rVB	602	401	0.02%	0.003%
39	6.606	1727	1731	1734	rBV3	326	312	0.02%	0.002%
40	6.657	1741	1747	1750	rBV4	685	736	0.04%	0.005%
41	6.744	1770	1774	1779	rBV4	581	524	0.03%	0.003%
42	6.902	1820	1823	1827	rVB	472	341	0.02%	0.002%
43	6.985	1838	1849	1877	rBV	193649	372258	18.24%	2.411%
44	7.204	1912	1917	1923	rBV5	819	1074	0.05%	0.007%
45	7.313	1937	1951	1986	rBV	847443	1503238	73.66%	9.737%
46	7.484	2002	2004	2005	rBV2	746	246	0.01%	0.002%
47	7.622	2034	2047	2078	rBV	134644	255232	12.51%	1.653%
48	7.773	2091	2094	2098	rBV3	502	413	0.02%	0.003%
49	7.972	2141	2156	2182	rBV	616758	1043845	51.15%	6.761%
50	8.091	2182	2193	2229	rBV	421102	908095	44.50%	5.882%
51	8.554	2333	2337	2339	rBV2	569	331	0.02%	0.002%
52	8.664	2367	2371	2375	rVB2	419	381	0.02%	0.002%
53	8.744	2392	2396	2402	rBV3	467	456	0.02%	0.003%
54	8.850	2416	2429	2455	rBV	759656	1250363	61.27%	8.099%
55	9.162	2522	2526	2531	rVB3	755	727	0.04%	0.005%
56	9.207	2538	2540	2543	rVB	610	334	0.02%	0.002%
57	9.230	2543	2547	2551	rBV3	544	445	0.02%	0.003%
58	9.304	2567	2570	2574	rVB3	431	322	0.02%	0.002%
59	9.326	2574	2577	2581	rBV2	327	286	0.01%	0.002%
60	9.352	2581	2585	2590	rBV2	208	251	0.01%	0.002%
61	9.384	2590	2595	2597	rBV2	483	434	0.02%	0.003%
62	9.464	2618	2620	2623	rBV2	431	260	0.01%	0.002%
63	9.545	2642	2645	2648	rVV2	420	292	0.01%	0.002%
64	9.680	2684	2687	2690	rBV	296	283	0.01%	0.002%
65	9.706	2691	2695	2700	rVB2	503	443	0.02%	0.003%
66	9.799	2719	2724	2728	rBV3	322	375	0.02%	0.002%
67	9.931	2761	2765	2767	rBV3	420	337	0.02%	0.002%
68	10.005	2784	2788	2793	rVB	376	343	0.02%	0.002%
69	10.033	2793	2797	2802	rBV	356	291	0.01%	0.002%
70	10.062	2802	2806	2810	rBV3	286	305	0.01%	0.002%
71	10.111	2818	2821	2826	rVB	374	283	0.01%	0.002%
72	10.143	2829	2831	2840	rVB3	355	390	0.02%	0.003%
73	10.214	2840	2853	2876	rBV	671236	1052000	51.55%	6.814%
74	10.451	2917	2927	2928	rBV3	314	455	0.02%	0.003%
75	10.657	2987	2991	2993	rBV2	462	255	0.01%	0.002%
76	10.914	3066	3071	3073	rBV2	579	471	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV0727022.D
 Acq On : 28 Jul 2022 01:09
 Operator : SY/MD
 Sample : N3880-13DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.979	3088	3091	3096	rVB2	455	411	0.02%	0.003%
78	11.249	3163	3175	3205	rBV	676293	1082050	53.02%	7.009%
79	11.455	3234	3239	3242	rBV3	547	537	0.03%	0.003%
80	11.622	3278	3291	3313	rBV	792615	1251147	61.31%	8.104%
81	12.252	3482	3487	3498	rVB3	1077	1664	0.08%	0.011%
82	12.419	3536	3539	3542	rBV2	356	314	0.02%	0.002%
83	12.635	3599	3606	3608	rBV3	422	481	0.02%	0.003%
84	12.657	3610	3613	3618	rVB3	656	608	0.03%	0.004%
85	12.821	3660	3664	3667	rBB	457	344	0.02%	0.002%
86	12.892	3683	3686	3690	rBV2	524	428	0.02%	0.003%
87	12.959	3702	3707	3710	rBV3	654	638	0.03%	0.004%
88	13.111	3752	3754	3760	rVB3	374	286	0.01%	0.002%
89	13.467	3860	3865	3868	rBV2	591	686	0.03%	0.004%
90	13.503	3871	3876	3877	rVV3	749	626	0.03%	0.004%
91	13.516	3877	3880	3885	rVB4	1157	1069	0.05%	0.007%
92	13.712	3935	3941	3945	rBV3	734	914	0.04%	0.006%
93	13.747	3950	3952	3955	rVV4	451	302	0.01%	0.002%
94	14.024	4035	4038	4039	rBV2	501	281	0.01%	0.002%
95	14.281	4116	4118	4122	rBV2	390	266	0.01%	0.002%
96	14.696	4245	4247	4253	rBV2	494	431	0.02%	0.003%
97	14.811	4280	4283	4285	rBV2	482	361	0.02%	0.002%
98	14.853	4292	4296	4299	rBV3	629	473	0.02%	0.003%
99	15.062	4359	4361	4365	rVB3	538	270	0.01%	0.002%
100	15.631	4534	4538	4541	rBV5	1316	1111	0.05%	0.007%




Sum of corrected areas: 15438948

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV072722.D
Acq On : 28 Jul 2022 01:09
Operator : SY/MD
Sample : N3880-13DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

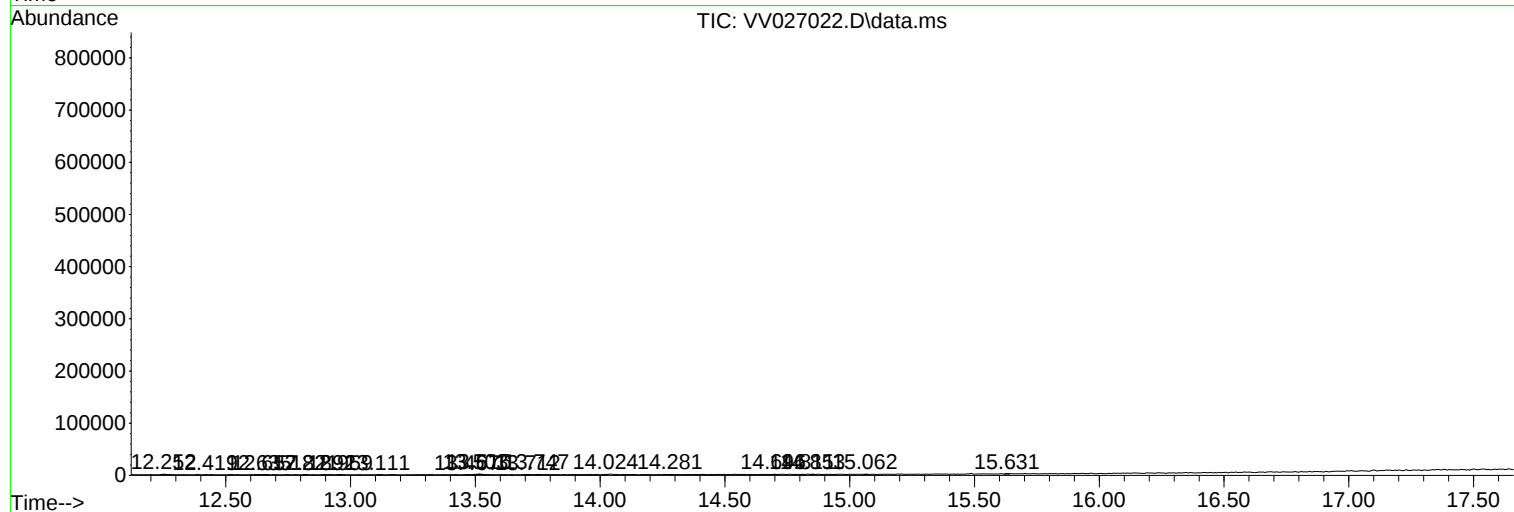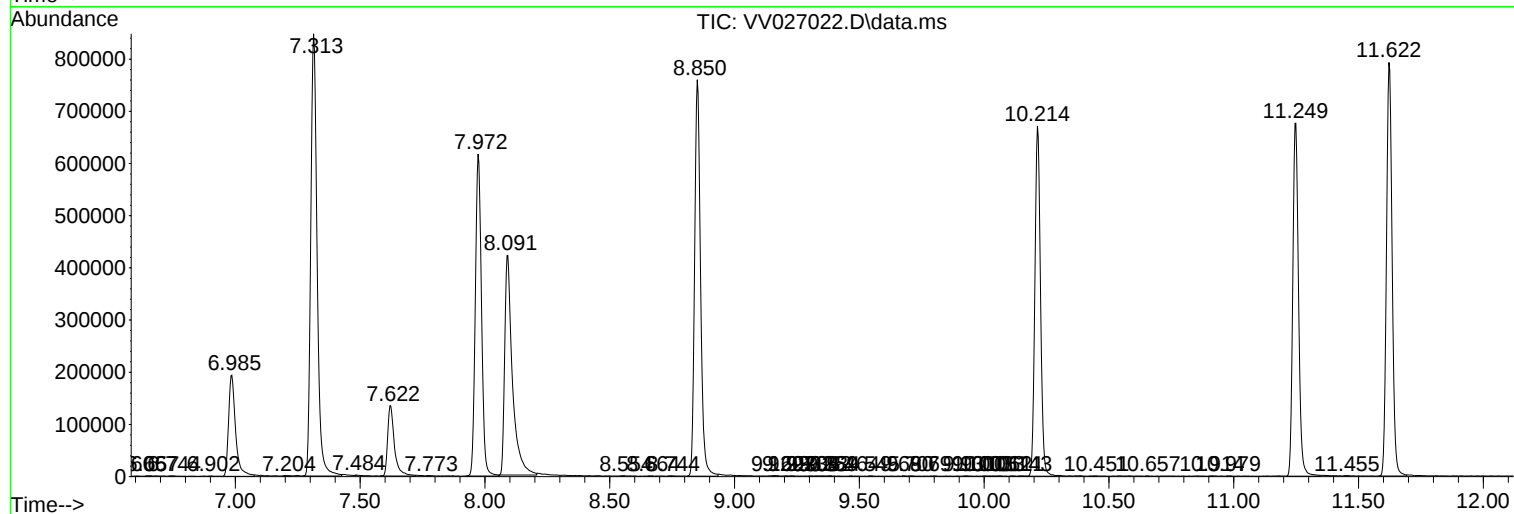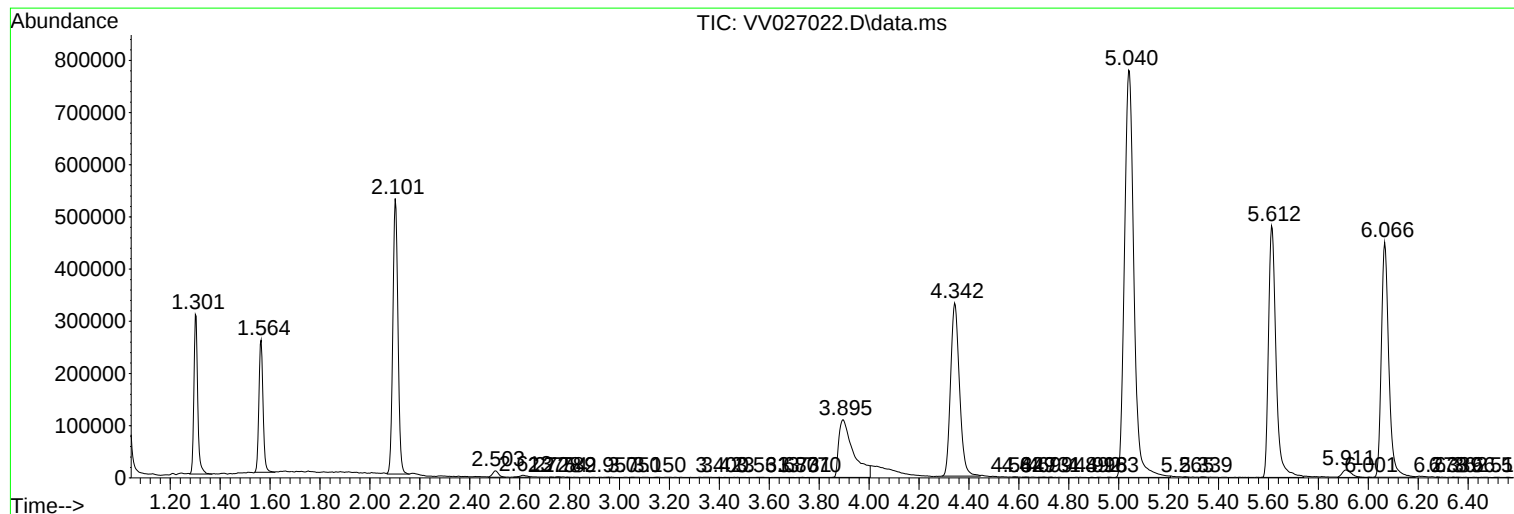

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027022.D
Acq On : 28 Jul 2022 01:09
Operator : SY/MD
Sample : N3880-13DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027022.D
Acq On : 28 Jul 2022 01:09
Operator : SY/MD
Sample : N3880-13DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc