

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027023.D
 Acq On : 28 Jul 2022 01:33
 Operator : SY/MD
 Sample : N3897-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	97	rVB	317066	324917	15.52%	2.188%
2	1.381	102	106	117	rVB2	7819	9859	0.47%	0.066%
3	1.565	155	163	175	rBV	254129	296749	14.17%	1.998%
4	2.102	320	330	344	rVB	537579	757729	36.19%	5.102%
5	2.182	346	355	375	rVV2	38302	101982	4.87%	0.687%
6	3.548	775	780	784	rBV2	320	371	0.02%	0.002%
7	3.690	810	824	832	rBV5	3739	9817	0.47%	0.066%
8	3.896	872	888	909	rBV	89405	313973	15.00%	2.114%
9	4.343	1011	1027	1069	rBV	341599	854433	40.81%	5.753%
10	4.966	1216	1221	1224	rVB	513	324	0.02%	0.002%
11	5.040	1228	1244	1298	rBV2	811997	2093625	100.00%	14.098%
12	5.256	1309	1311	1317	rVB4	628	488	0.02%	0.003%
13	5.378	1346	1349	1352	rVB	531	347	0.02%	0.002%
14	5.526	1391	1395	1398	rBV5	665	658	0.03%	0.004%
15	5.613	1409	1422	1455	rBV	504274	1046197	49.97%	7.045%
16	5.905	1501	1513	1531	rVB2	13556	29898	1.43%	0.201%
17	6.066	1548	1563	1594	rBV	460176	948458	45.30%	6.387%
18	6.314	1636	1640	1641	rBV4	683	535	0.03%	0.004%
19	6.346	1647	1650	1651	rBV2	1014	491	0.02%	0.003%
20	6.484	1691	1693	1697	rVB4	820	513	0.02%	0.003%
21	6.532	1697	1708	1709	rBV4	2696	3287	0.16%	0.022%
22	6.580	1713	1723	1739	rVB3	7581	18500	0.88%	0.125%
23	6.674	1748	1752	1755	rBV3	749	594	0.03%	0.004%
24	6.735	1768	1771	1774	rVV2	429	331	0.02%	0.002%
25	6.986	1838	1849	1878	rBV	195336	376817	18.00%	2.537%
26	7.236	1924	1927	1930	rBV3	588	545	0.03%	0.004%
27	7.314	1939	1951	1988	rBV	858523	1555592	74.30%	10.475%
28	7.468	1997	1999	2001	rBV3	742	358	0.02%	0.002%
29	7.619	2036	2046	2073	rVV	141095	257763	12.31%	1.736%
30	7.870	2122	2124	2128	rVB2	613	349	0.02%	0.002%
31	7.937	2134	2145	2151	rBV5	5774	10016	0.48%	0.067%
32	7.979	2152	2158	2171	rVB5	7551	13712	0.65%	0.092%
33	8.043	2171	2178	2182	rBV5	1144	1548	0.07%	0.010%
34	8.092	2182	2193	2231	rBV	413189	925019	44.18%	6.229%
35	8.384	2272	2284	2304	rBV2	11816	38442	1.84%	0.259%
36	8.596	2349	2350	2358	rVB3	655	611	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027023.D
 Acq On : 28 Jul 2022 01:33
 Operator : SY/MD
 Sample : N3897-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	8.632	2358	2361	2363	rBV2	555	307	0.01%	0.002%
38	8.670	2369	2373	2379	rBV2	393	400	0.02%	0.003%
39	8.789	2408	2410	2415	rVB3	654	431	0.02%	0.003%
40	8.850	2416	2429	2452	rBV	798943	1300134	62.10%	8.755%
41	9.076	2494	2499	2504	rVB5	781	816	0.04%	0.005%
42	9.117	2509	2512	2514	rBV4	576	339	0.02%	0.002%
43	9.153	2519	2523	2529	rBV4	845	1066	0.05%	0.007%
44	9.259	2553	2556	2562	rVB4	778	809	0.04%	0.005%
45	9.403	2598	2601	2604	rVB	523	345	0.02%	0.002%
46	9.487	2623	2627	2630	rBV3	400	377	0.02%	0.003%
47	9.545	2642	2645	2648	rBV2	663	500	0.02%	0.003%
48	9.580	2654	2656	2659	rBV2	530	343	0.02%	0.002%
49	9.625	2665	2670	2673	rVV3	768	757	0.04%	0.005%
50	9.641	2673	2675	2680	rVB3	506	362	0.02%	0.002%
51	9.731	2698	2703	2706	rBV2	543	513	0.02%	0.003%
52	10.021	2784	2793	2796	rVV3	879	1077	0.05%	0.007%
53	10.127	2822	2826	2830	rBV2	432	337	0.02%	0.002%
54	10.214	2840	2853	2882	rBV	673349	1071128	51.16%	7.213%
55	10.384	2894	2906	2919	rVB2	5818	9919	0.47%	0.067%
56	10.545	2952	2956	2961	rBV4	661	753	0.04%	0.005%
57	10.577	2961	2966	2973	rBV5	1041	1284	0.06%	0.009%
58	10.738	3013	3016	3020	rVB2	442	352	0.02%	0.002%
59	10.760	3020	3023	3029	rBV2	300	329	0.02%	0.002%
60	10.792	3029	3033	3037	rBV2	434	448	0.02%	0.003%
61	10.854	3049	3052	3058	rVV4	793	691	0.03%	0.005%
62	10.921	3065	3073	3077	rBV3	963	1073	0.05%	0.007%
63	11.040	3106	3110	3115	rBV3	429	484	0.02%	0.003%
64	11.088	3120	3125	3127	rBV2	471	414	0.02%	0.003%
65	11.188	3150	3156	3157	rBV3	737	492	0.02%	0.003%
66	11.249	3163	3175	3197	rBV	731971	1123500	53.66%	7.565%
67	11.535	3255	3264	3279	rBV3	8208	14443	0.69%	0.097%
68	11.622	3279	3291	3315	rBV	837721	1305176	62.34%	8.788%
69	11.834	3353	3357	3360	rBV2	442	372	0.02%	0.003%
70	11.850	3360	3362	3366	rVB2	505	345	0.02%	0.002%
71	12.214	3467	3475	3478	rBV2	442	505	0.02%	0.003%
72	12.246	3478	3485	3486	rBV3	1263	1034	0.05%	0.007%
73	12.333	3509	3512	3515	rBV2	617	426	0.02%	0.003%
74	12.371	3521	3524	3525	rBV	640	362	0.02%	0.002%
75	12.657	3605	3613	3617	rVB4	771	1097	0.05%	0.007%
76	12.783	3648	3652	3657	rBV3	361	441	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV0727023.D
 Acq On : 28 Jul 2022 01:33
 Operator : SY/MD
 Sample : N3897-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.825	3660	3665	3669	rVB2	498	540	0.03%	0.004%
78	12.850	3669	3673	3675	rBV2	532	335	0.02%	0.002%
79	12.982	3711	3714	3716	rBV3	515	352	0.02%	0.002%
80	13.082	3742	3745	3751	rVB	379	343	0.02%	0.002%
81	13.149	3761	3766	3770	rBV5	524	495	0.02%	0.003%
82	13.271	3801	3804	3808	rVV5	693	449	0.02%	0.003%
83	13.516	3874	3880	3886	rBV6	1480	1711	0.08%	0.012%
84	13.699	3934	3937	3942	rVB2	559	438	0.02%	0.003%
85	13.728	3942	3946	3948	rBV3	360	355	0.02%	0.002%
86	13.757	3951	3955	3958	rBV4	528	476	0.02%	0.003%
87	13.828	3975	3977	3982	rVB4	455	417	0.02%	0.003%
88	13.931	4007	4009	4013	rBB3	451	310	0.01%	0.002%
89	13.969	4018	4021	4026	rBV3	364	370	0.02%	0.002%
90	14.185	4084	4088	4090	rBV2	662	483	0.02%	0.003%
91	14.284	4115	4119	4121	rBV3	614	519	0.02%	0.003%
92	14.371	4144	4146	4150	rVB3	555	349	0.02%	0.002%
93	14.519	4190	4192	4197	rVB4	417	319	0.02%	0.002%
94	14.606	4217	4219	4223	rVB2	733	406	0.02%	0.003%
95	14.702	4247	4249	4255	rVB3	447	304	0.01%	0.002%
96	14.815	4280	4284	4287	rBV3	540	497	0.02%	0.003%
97	14.960	4324	4329	4330	rBV3	482	420	0.02%	0.003%
98	15.101	4371	4373	4376	rBV3	515	329	0.02%	0.002%
99	15.329	4441	4444	4445	rBV3	672	437	0.02%	0.003%
100	15.722	4561	4566	4569	rBV5	1275	1483	0.07%	0.010%




Sum of corrected areas: 14850966

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

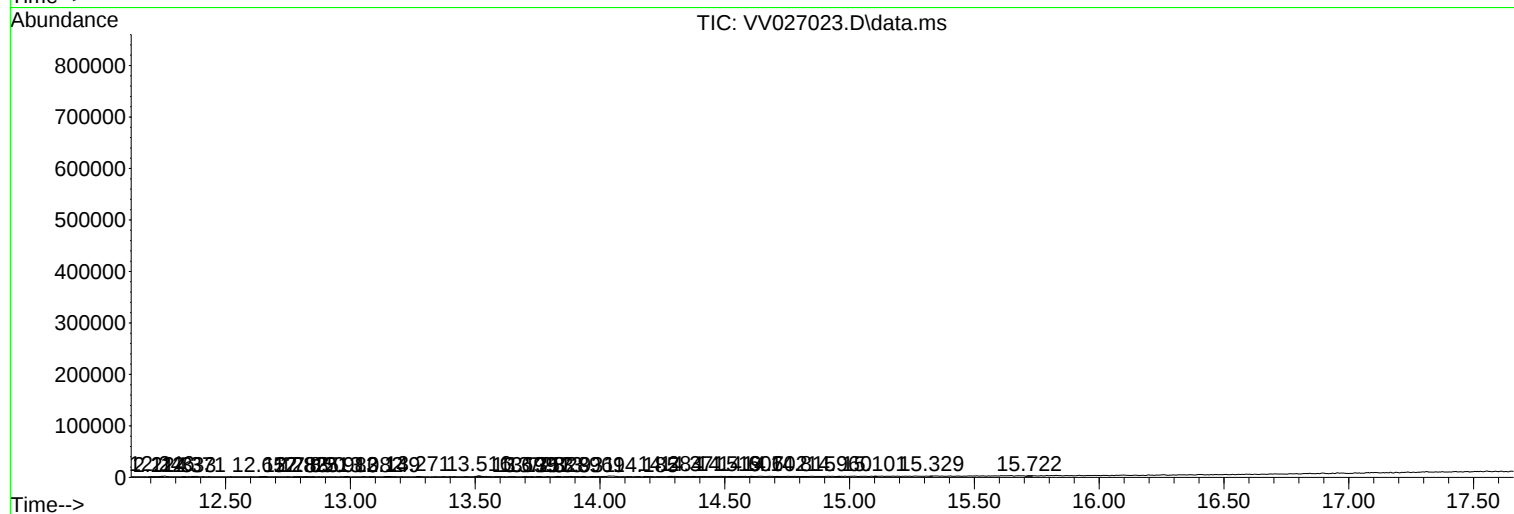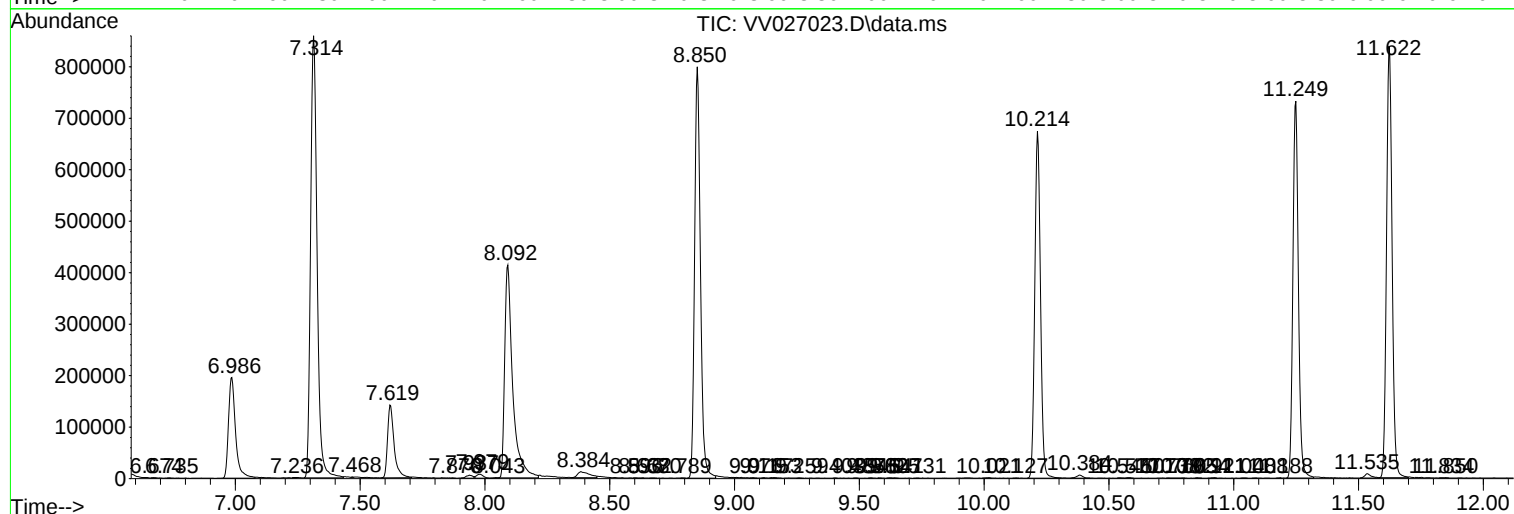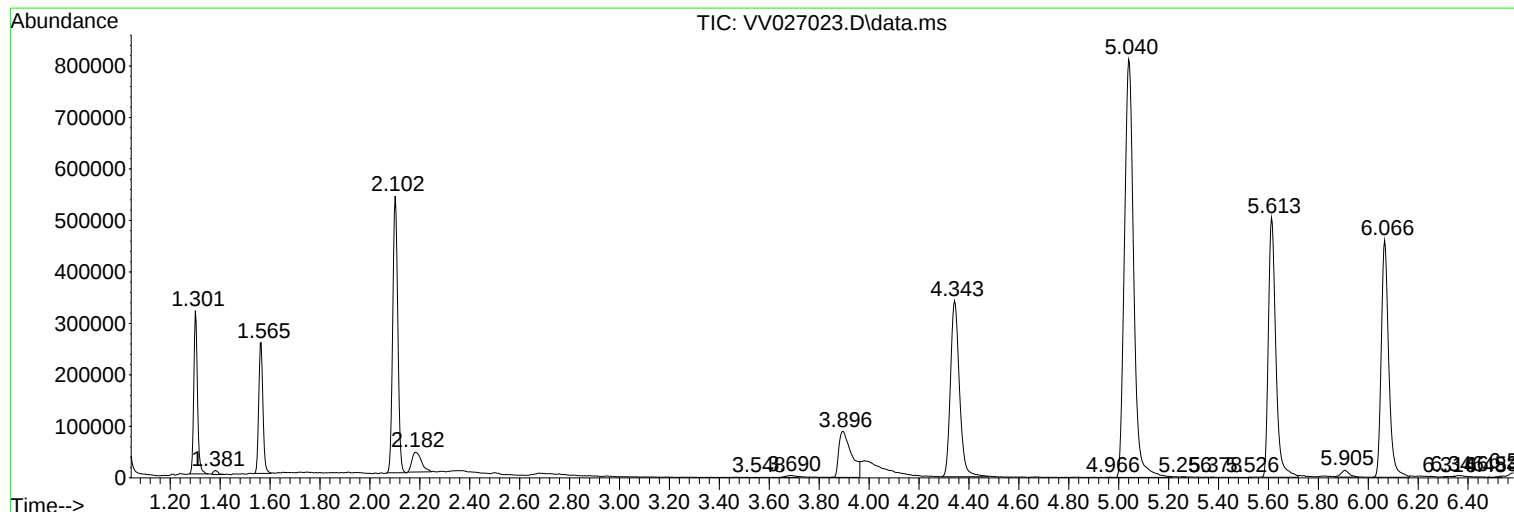

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027023.D
Acq On : 28 Jul 2022 01:33
Operator : SY/MD
Sample : N3897-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc