

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027024.D
 Acq On : 28 Jul 2022 01:58
 Operator : SY/MD
 Sample : N3897-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	314636	327430	15.56%	2.215%
2	1.564	155	163	178	rBV	258821	300493	14.28%	2.033%
3	2.101	321	330	344	rBV	537937	755526	35.91%	5.111%
4	3.130	647	650	653	rVB3	455	307	0.01%	0.002%
5	3.150	653	656	658	rBV	343	269	0.01%	0.002%
6	3.236	678	683	687	rBV3	307	365	0.02%	0.002%
7	3.359	718	721	723	rBV2	385	269	0.01%	0.002%
8	3.410	733	737	738	rBV2	360	201	0.01%	0.001%
9	3.445	746	748	751	rBV	386	219	0.01%	0.001%
10	3.635	802	807	810	rVB2	240	243	0.01%	0.002%
11	3.664	810	816	819	rBV3	221	212	0.01%	0.001%
12	3.693	820	825	827	rBV2	240	235	0.01%	0.002%
13	3.780	847	852	853	rBV	211	157	0.01%	0.001%
14	3.809	857	861	863	rBV2	267	137	0.01%	0.001%
15	3.831	865	868	872	rVB2	383	280	0.01%	0.002%
16	3.854	872	875	878	rBV2	431	365	0.02%	0.002%
17	3.899	878	889	958	rBV	83743	459486	21.84%	3.108%
18	4.342	1012	1027	1065	rBV	341315	858745	40.82%	5.809%
19	4.606	1107	1109	1112	rVB2	695	320	0.02%	0.002%
20	4.751	1152	1154	1159	rBV4	423	357	0.02%	0.002%
21	4.786	1163	1165	1173	rVB4	498	577	0.03%	0.004%
22	4.825	1173	1177	1181	rBV4	610	651	0.03%	0.004%
23	4.873	1190	1192	1197	rBV3	382	325	0.02%	0.002%
24	4.947	1213	1215	1218	rVB2	488	220	0.01%	0.001%
25	4.985	1222	1227	1228	rBV2	332	285	0.01%	0.002%
26	5.040	1228	1244	1290	rBV2	809476	2103691	100.00%	14.230%
27	5.339	1335	1337	1341	rBV2	422	275	0.01%	0.002%
28	5.384	1349	1351	1353	rBV2	322	157	0.01%	0.001%
29	5.484	1378	1382	1383	rBV2	424	241	0.01%	0.002%
30	5.535	1395	1398	1403	rBV	533	396	0.02%	0.003%
31	5.561	1403	1406	1409	rBV4	366	284	0.01%	0.002%
32	5.612	1410	1422	1458	rBV	493072	1021798	48.57%	6.912%
33	5.902	1507	1512	1529	rVB4	12505	24471	1.16%	0.166%
34	5.992	1536	1540	1543	rBV6	408	417	0.02%	0.003%
35	6.066	1549	1563	1595	rBV2	457479	956049	45.45%	6.467%
36	6.346	1646	1650	1655	rVB4	468	431	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027024.D
 Acq On : 28 Jul 2022 01:58
 Operator : SY/MD
 Sample : N3897-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.391	1661	1664	1667	rVB2	588	391	0.02%	0.003%
38	6.416	1668	1672	1675	rVB3	477	238	0.01%	0.002%
39	6.439	1676	1679	1685	rBV3	442	475	0.02%	0.003%
40	6.500	1696	1698	1701	rBV2	397	268	0.01%	0.002%
41	6.529	1705	1707	1710	rBV3	328	201	0.01%	0.001%
42	6.561	1715	1717	1720	rBV3	456	326	0.02%	0.002%
43	6.625	1734	1737	1739	rBV2	388	243	0.01%	0.002%
44	6.741	1770	1773	1777	rVB2	299	275	0.01%	0.002%
45	6.773	1781	1783	1784	rBV	218	94	0.00%	0.001%
46	6.783	1784	1786	1787	rBV	230	98	0.00%	0.001%
47	6.812	1792	1795	1798	rVB2	442	268	0.01%	0.002%
48	6.837	1801	1803	1804	rBV	268	102	0.00%	0.001%
49	6.876	1813	1815	1817	rVB2	287	107	0.01%	0.001%
50	6.895	1817	1821	1825	rVB	266	241	0.01%	0.002%
51	6.921	1825	1829	1832	rBV	414	321	0.02%	0.002%
52	6.940	1832	1835	1838	rBV2	449	396	0.02%	0.003%
53	6.985	1838	1849	1872	rBV	200289	380816	18.10%	2.576%
54	7.313	1939	1951	1976	rBV	875675	1556068	73.97%	10.526%
55	7.619	2037	2046	2070	rBV	138351	252852	12.02%	1.710%
56	7.860	2117	2121	2123	rBV4	729	585	0.03%	0.004%
57	8.034	2170	2175	2177	rBV3	464	383	0.02%	0.003%
58	8.050	2177	2180	2182	rBV2	545	303	0.01%	0.002%
59	8.091	2182	2193	2235	rBV	425141	930792	44.25%	6.296%
60	8.587	2345	2347	2349	rBV3	256	135	0.01%	0.001%
61	8.850	2417	2429	2459	rBV	772441	1285174	61.09%	8.693%
62	9.197	2533	2537	2540	rBV2	510	321	0.02%	0.002%
63	9.214	2540	2542	2546	rVB	380	269	0.01%	0.002%
64	9.259	2554	2556	2559	rBV	355	213	0.01%	0.001%
65	9.310	2566	2572	2574	rBV3	356	293	0.01%	0.002%
66	9.326	2574	2577	2579	rVV3	423	209	0.01%	0.001%
67	9.452	2613	2616	2618	rVB	372	197	0.01%	0.001%
68	9.471	2618	2622	2624	rBV2	370	374	0.02%	0.003%
69	9.513	2632	2635	2637	rBV2	228	130	0.01%	0.001%
70	9.554	2643	2648	2653	rVB2	600	751	0.04%	0.005%
71	9.583	2653	2657	2662	rBV3	307	344	0.02%	0.002%
72	9.606	2662	2664	2665	rBV3	183	59	0.00%	0.000%
73	9.670	2682	2684	2686	rBV	204	92	0.00%	0.001%
74	9.731	2700	2703	2707	rVB	276	202	0.01%	0.001%
75	9.754	2707	2710	2713	rBV2	207	118	0.01%	0.001%
76	9.805	2724	2726	2728	rVB	209	65	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV0727024.D
 Acq On : 28 Jul 2022 01:58
 Operator : SY/MD
 Sample : N3897-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.815	2728	2729	2730	rBV	274	80	0.00%	0.001%
78	9.905	2755	2757	2759	rBV	148	70	0.00%	0.000%
79	10.014	2782	2791	2796	rBV4	1933	2708	0.13%	0.018%
80	10.127	2823	2826	2830	rVB3	316	219	0.01%	0.001%
81	10.146	2830	2832	2834	rBV	238	160	0.01%	0.001%
82	10.214	2841	2853	2870	rBV	685670	1071262	50.92%	7.246%
83	10.381	2899	2905	2917	rVB4	4338	6758	0.32%	0.046%
84	10.426	2917	2919	2921	rBV	331	154	0.01%	0.001%
85	10.686	2998	3000	3003	rBV2	271	157	0.01%	0.001%
86	10.738	3012	3016	3018	rBV2	327	243	0.01%	0.002%
87	10.902	3061	3067	3070	rBV3	508	661	0.03%	0.004%
88	10.998	3095	3097	3099	rBV	245	95	0.00%	0.001%
89	11.014	3099	3102	3106	rBV2	333	273	0.01%	0.002%
90	11.085	3121	3124	3125	rBV	185	113	0.01%	0.001%
91	11.146	3140	3143	3145	rBV	234	188	0.01%	0.001%
92	11.181	3149	3154	3157	rBV4	745	708	0.03%	0.005%
93	11.249	3164	3175	3203	rBV	697561	1102053	52.39%	7.455%
94	11.535	3255	3264	3279	rBV3	20795	40057	1.90%	0.271%
95	11.622	3280	3291	3318	rVB	845043	1321572	62.82%	8.939%
96	12.181	3462	3465	3468	rBV	440	310	0.01%	0.002%
97	12.445	3543	3547	3552	rBV2	443	611	0.03%	0.004%
98	12.609	3596	3598	3602	rBV2	385	291	0.01%	0.002%
99	12.754	3641	3643	3645	rVB	389	81	0.00%	0.001%
100	12.959	3699	3707	3714	rBV3	2555	4146	0.20%	0.028%




Sum of corrected areas: 14783643

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027024.D
Acq On : 28 Jul 2022 01:58
Operator : SY/MD
Sample : N3897-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

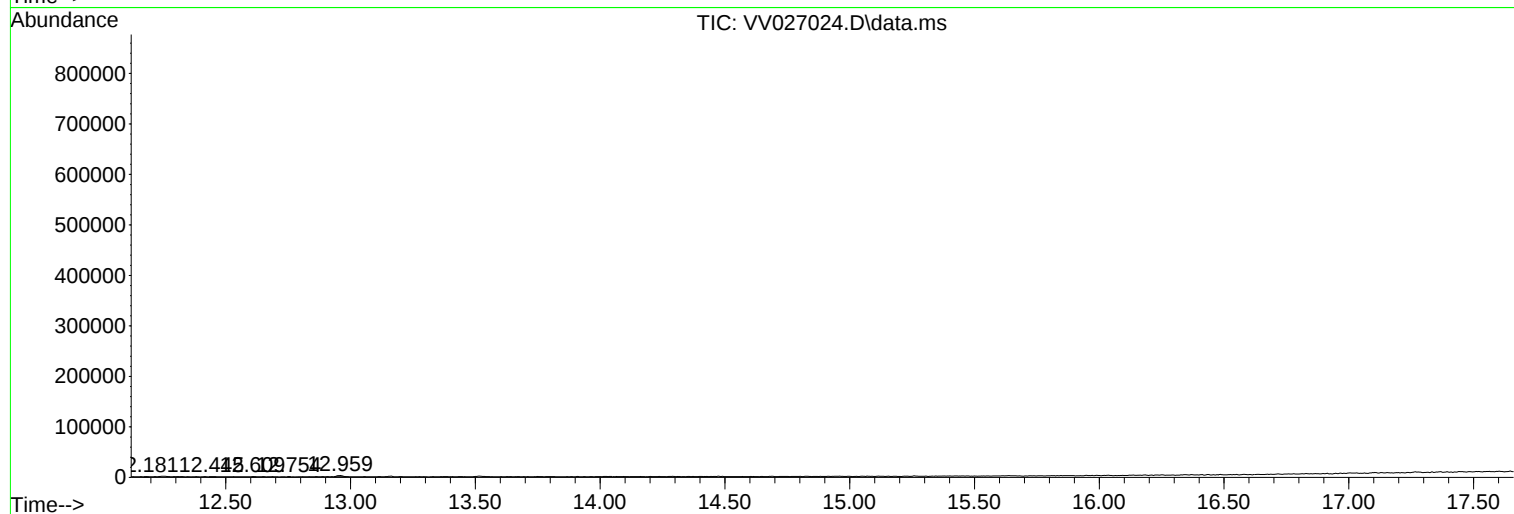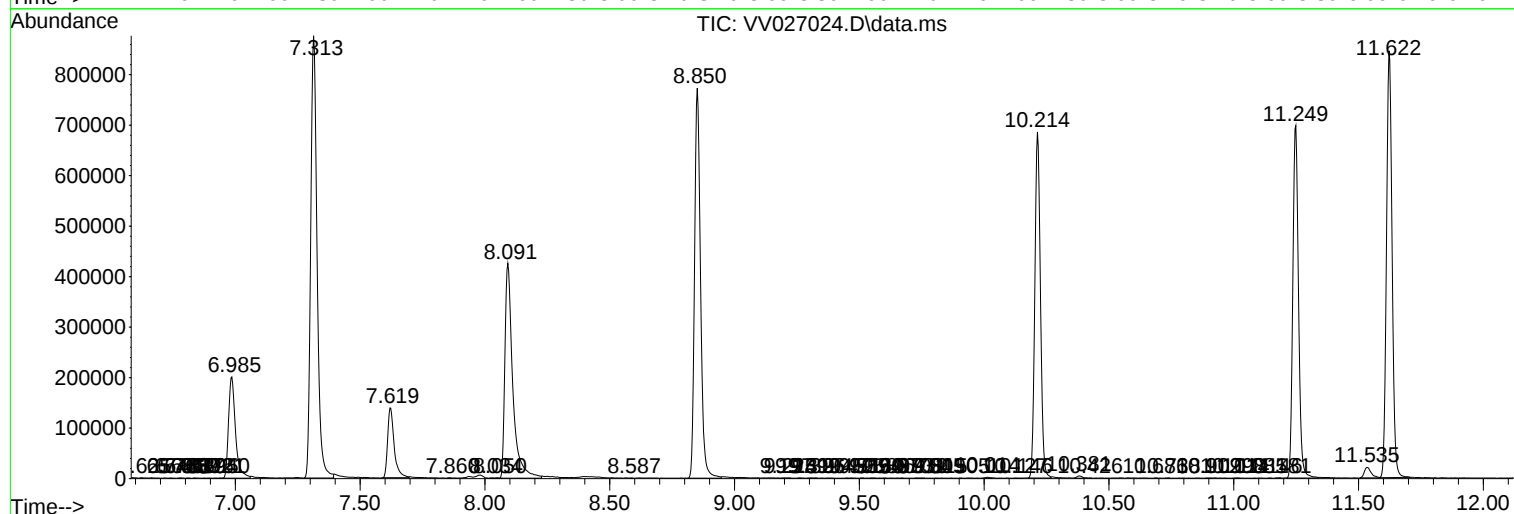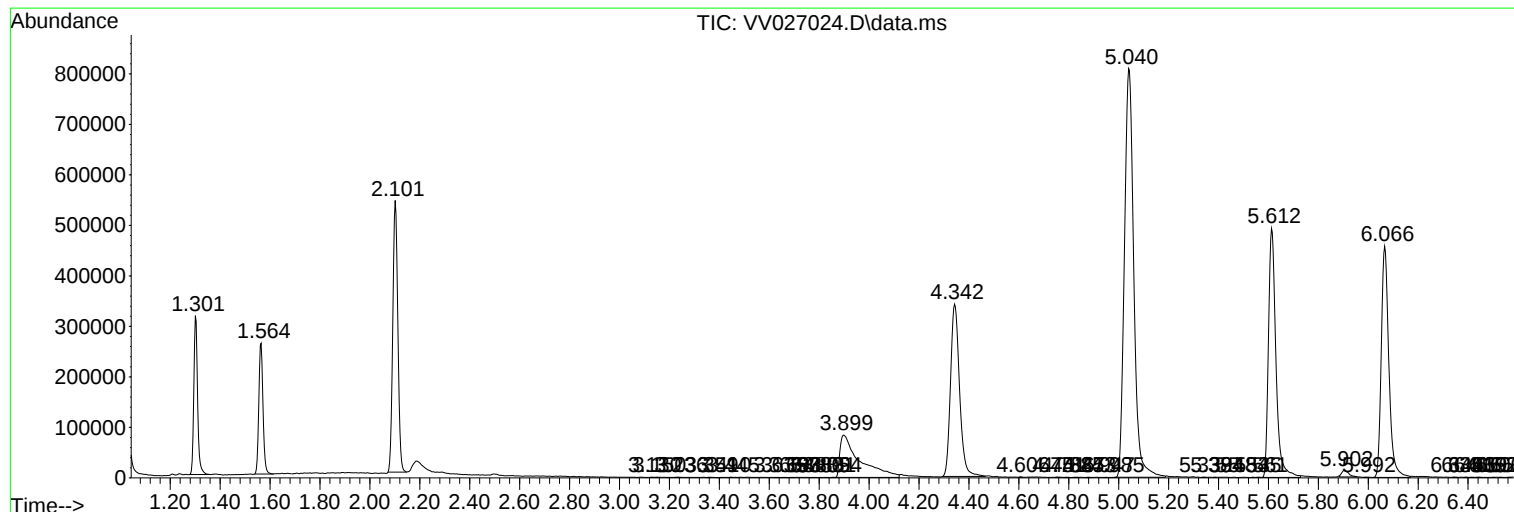

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027024.D
Acq On : 28 Jul 2022 01:58
Operator : SY/MD
Sample : N3897-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027024.D
Acq On : 28 Jul 2022 01:58
Operator : SY/MD
Sample : N3897-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc