

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV0727027.D
 Acq On : 28 Jul 2022 03:11
 Operator : SY/MD
 Sample : N3897-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV0727027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	305835	313182	15.40%	2.224%
2	1.564	155	163	175	rBV	249823	290895	14.31%	2.066%
3	2.101	321	330	344	rVB	520942	735276	36.17%	5.222%
4	3.162	658	660	663	rBV2	322	149	0.01%	0.001%
5	3.182	663	666	667	rBV	458	257	0.01%	0.002%
6	3.249	684	687	689	rBV2	351	164	0.01%	0.001%
7	3.310	704	706	709	rBV3	421	277	0.01%	0.002%
8	3.342	714	716	720	rVB2	485	286	0.01%	0.002%
9	3.365	720	723	729	rVB2	305	254	0.01%	0.002%
10	3.403	729	735	738	rVB3	327	313	0.02%	0.002%
11	3.426	738	742	745	rBV2	322	233	0.01%	0.002%
12	3.493	760	763	769	rVB	305	291	0.01%	0.002%
13	3.522	769	772	776	rBV2	204	227	0.01%	0.002%
14	3.558	781	783	785	rBV2	160	96	0.00%	0.001%
15	3.680	819	821	824	rVB	294	114	0.01%	0.001%
16	3.709	826	830	831	rBV2	328	187	0.01%	0.001%
17	3.744	839	841	845	rVB2	210	107	0.01%	0.001%
18	3.770	845	849	853	rBV3	227	253	0.01%	0.002%
19	3.799	853	858	862	rVB2	361	365	0.02%	0.003%
20	3.825	864	866	868	rBV	165	78	0.00%	0.001%
21	3.895	877	888	909	rBV	84048	278641	13.71%	1.979%
22	4.342	1012	1027	1054	rBV	332018	819165	40.29%	5.818%
23	4.603	1106	1108	1112	rBV3	473	284	0.01%	0.002%
24	4.754	1153	1155	1157	rBV2	374	179	0.01%	0.001%
25	4.812	1171	1173	1178	rVB4	663	376	0.02%	0.003%
26	4.960	1217	1219	1221	rVB	280	103	0.01%	0.001%
27	4.982	1221	1226	1228	rBV2	198	209	0.01%	0.001%
28	5.040	1228	1244	1283	rBV2	783274	2033032	100.00%	14.439%
29	5.542	1398	1400	1401	rBV	250	116	0.01%	0.001%
30	5.551	1401	1403	1405	rBV	412	227	0.01%	0.002%
31	5.612	1410	1422	1462	rBV	472065	989260	48.66%	7.026%
32	5.995	1538	1541	1542	rBV2	370	184	0.01%	0.001%
33	6.017	1545	1548	1549	rBV	390	209	0.01%	0.001%
34	6.066	1549	1563	1598	rBV	439959	920659	45.29%	6.539%
35	6.387	1661	1663	1665	rVB2	230	69	0.00%	0.000%
36	6.400	1665	1667	1671	rBV2	184	64	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027027.D
 Acq On : 28 Jul 2022 03:11
 Operator : SY/MD
 Sample : N3897-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.419	1671	1673	1674	rBV	425	163	0.01%	0.001%
38	6.506	1697	1700	1701	rBV	120	50	0.00%	0.000%
39	6.577	1720	1722	1730	rVB4	956	984	0.05%	0.007%
40	6.635	1739	1740	1741	rBV4	222	67	0.00%	0.000%
41	6.648	1741	1744	1748	rVV4	757	549	0.03%	0.004%
42	6.744	1770	1774	1776	rBV	418	245	0.01%	0.002%
43	6.776	1781	1784	1785	rBV	211	111	0.01%	0.001%
44	6.841	1800	1804	1807	rBV2	507	413	0.02%	0.003%
45	6.892	1816	1820	1821	rBV2	170	129	0.01%	0.001%
46	6.921	1826	1829	1831	rVB	207	107	0.01%	0.001%
47	6.937	1831	1834	1836	rBV	271	179	0.01%	0.001%
48	6.985	1837	1849	1880	rBV	189450	365535	17.98%	2.596%
49	7.243	1926	1929	1931	rBV4	885	433	0.02%	0.003%
50	7.313	1939	1951	1980	rBV	846111	1497294	73.65%	10.634%
51	7.622	2037	2047	2081	rBV2	134128	249943	12.29%	1.775%
52	8.040	2174	2177	2179	rBV2	236	174	0.01%	0.001%
53	8.091	2182	2193	2230	rBV	395325	906618	44.59%	6.439%
54	8.686	2373	2378	2381	rBV2	572	529	0.03%	0.004%
55	8.767	2398	2403	2408	rBV2	590	623	0.03%	0.004%
56	8.805	2411	2415	2417	rBV2	321	191	0.01%	0.001%
57	8.850	2417	2429	2456	rBV	760632	1255115	61.74%	8.914%
58	9.406	2594	2602	2605	rBV3	428	671	0.03%	0.005%
59	9.435	2608	2611	2617	rVV2	371	356	0.02%	0.003%
60	9.474	2621	2623	2626	rBV	290	150	0.01%	0.001%
61	9.535	2639	2642	2644	rBV2	227	193	0.01%	0.001%
62	9.583	2654	2657	2662	rVB4	488	325	0.02%	0.002%
63	9.660	2679	2681	2688	rBV2	278	296	0.01%	0.002%
64	9.738	2700	2705	2708	rBV2	508	319	0.02%	0.002%
65	9.789	2718	2721	2724	rBV2	383	243	0.01%	0.002%
66	9.824	2730	2732	2736	rBV	341	237	0.01%	0.002%
67	9.860	2741	2743	2744	rBV2	184	79	0.00%	0.001%
68	9.914	2757	2760	2761	rBV2	470	272	0.01%	0.002%
69	9.998	2781	2786	2787	rBV	844	627	0.03%	0.004%
70	10.114	2820	2822	2826	rVB2	291	146	0.01%	0.001%
71	10.133	2826	2828	2831	rBV	187	80	0.00%	0.001%
72	10.213	2841	2853	2881	rBV	667003	1052879	51.79%	7.478%
73	10.384	2898	2906	2915	rVB2	4747	6954	0.34%	0.049%
74	10.506	2940	2944	2945	rBV2	316	209	0.01%	0.001%
75	10.580	2962	2967	2969	rVB3	617	520	0.03%	0.004%
76	10.828	3040	3044	3047	rBV2	369	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027027.D
 Acq On : 28 Jul 2022 03:11
 Operator : SY/MD
 Sample : N3897-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.924	3069	3074	3078	rBV2	558	659	0.03%	0.005%
78	11.139	3138	3141	3144	rBV2	319	224	0.01%	0.002%
79	11.168	3149	3150	3152	rBV	191	103	0.01%	0.001%
80	11.184	3153	3155	3157	rBV	399	252	0.01%	0.002%
81	11.249	3164	3175	3200	rBV	681620	1062658	52.27%	7.547%
82	11.535	3257	3264	3279	rBV4	7510	13096	0.64%	0.093%
83	11.622	3279	3291	3319	rBV	800311	1271985	62.57%	9.034%
84	12.374	3523	3525	3528	rVB3	489	239	0.01%	0.002%
85	12.525	3571	3572	3573	rBV	583	122	0.01%	0.001%
86	12.792	3653	3655	3657	rBV2	209	90	0.00%	0.001%
87	12.805	3657	3659	3661	rBV2	506	264	0.01%	0.002%
88	13.782	3960	3963	3965	rBV	505	392	0.02%	0.003%




Sum of corrected areas: 14080200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027027.D
Acq On : 28 Jul 2022 03:11
Operator : SY/MD
Sample : N3897-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

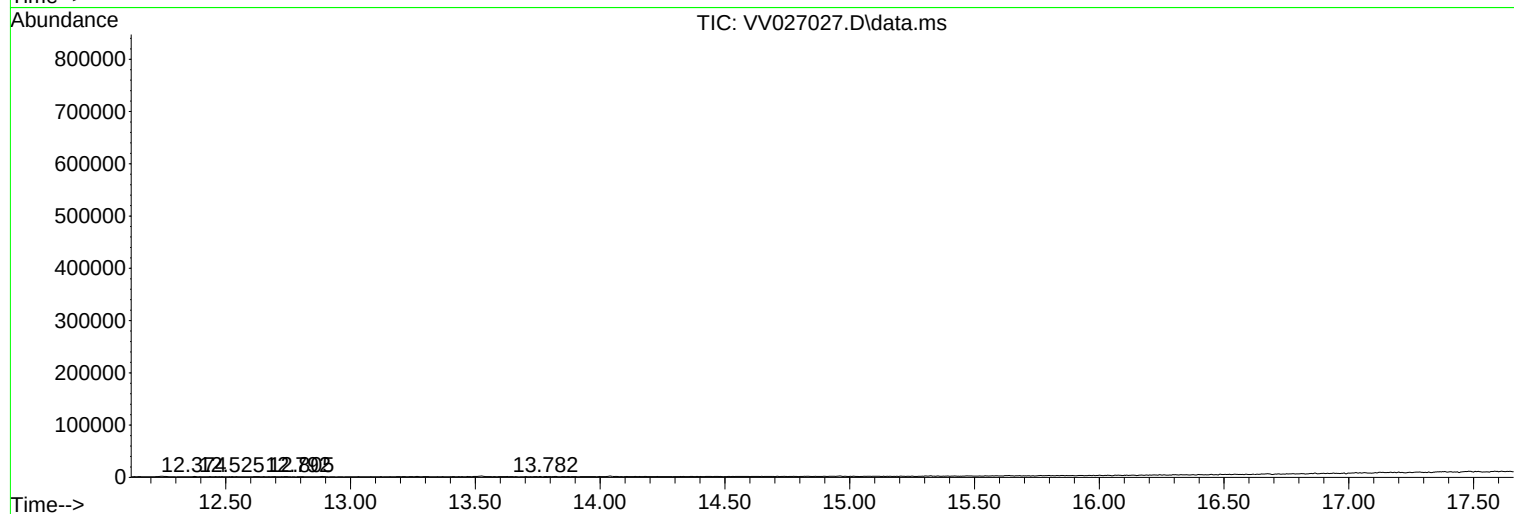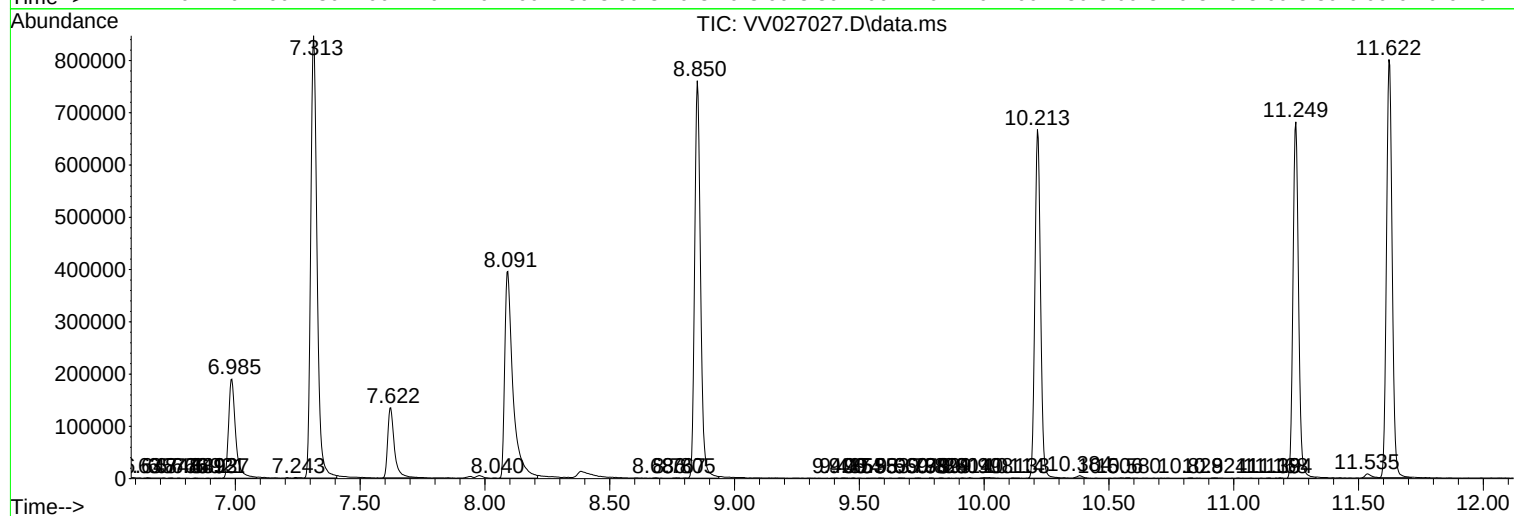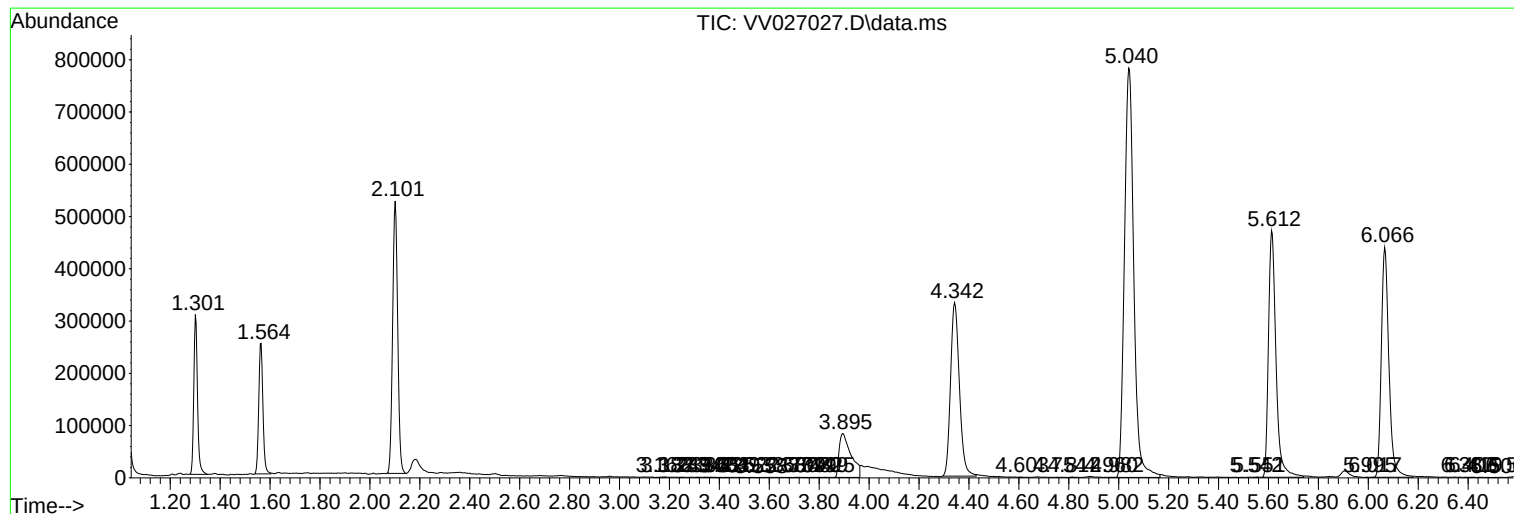

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027027.D
Acq On : 28 Jul 2022 03:11
Operator : SY/MD
Sample : N3897-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027027.D
Acq On : 28 Jul 2022 03:11
Operator : SY/MD
Sample : N3897-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc