

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027030.D
 Acq On : 28 Jul 2022 04:25
 Operator : SY/MD
 Sample : N3897-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	98	rVB	308569	317649	15.35%	2.196%
2	1.565	155	163	177	rVB	251075	287756	13.90%	1.990%
3	2.102	320	330	347	rVB	529883	755201	36.49%	5.221%
4	2.503	447	455	467	rVB5	2486	4818	0.23%	0.033%
5	2.767	527	537	543	rBV6	2629	4047	0.20%	0.028%
6	2.973	597	601	603	rBV2	419	336	0.02%	0.002%
7	3.282	693	697	700	rBV3	602	525	0.03%	0.004%
8	3.600	794	796	799	rVV	568	431	0.02%	0.003%
9	3.667	813	817	819	rVV2	431	437	0.02%	0.003%
10	3.680	819	821	824	rVV3	580	372	0.02%	0.003%
11	3.700	824	827	833	rVB2	465	470	0.02%	0.003%
12	3.847	867	873	877	rVB2	314	347	0.02%	0.002%
13	3.892	877	887	915	rBV2	85867	306059	14.79%	2.116%
14	4.343	1011	1027	1068	rVB	339497	843105	40.74%	5.829%
15	4.642	1116	1120	1122	rBV2	364	339	0.02%	0.002%
16	4.703	1136	1139	1145	rVB4	818	602	0.03%	0.004%
17	4.732	1145	1148	1151	rBV2	347	298	0.01%	0.002%
18	4.764	1155	1158	1161	rBV3	399	316	0.02%	0.002%
19	4.809	1169	1172	1173	rBV2	723	438	0.02%	0.003%
20	5.040	1227	1244	1296	rBV2	792918	2069474	100.00%	14.308%
21	5.384	1345	1351	1355	rVB4	420	571	0.03%	0.004%
22	5.410	1355	1359	1362	rVB2	653	448	0.02%	0.003%
23	5.497	1382	1386	1391	rBV4	519	579	0.03%	0.004%
24	5.568	1400	1408	1410	rVB3	587	612	0.03%	0.004%
25	5.613	1410	1422	1456	rBV	492438	1014396	49.02%	7.014%
26	5.908	1501	1514	1530	rBV5	8864	20152	0.97%	0.139%
27	6.066	1549	1563	1595	rBV	446835	938222	45.34%	6.487%
28	6.362	1650	1655	1658	rBV2	419	395	0.02%	0.003%
29	6.426	1670	1675	1677	rBV3	574	382	0.02%	0.003%
30	6.513	1692	1702	1704	rBV4	1925	2216	0.11%	0.015%
31	6.622	1729	1736	1739	rBV3	397	422	0.02%	0.003%
32	6.661	1743	1748	1753	rBV3	459	569	0.03%	0.004%
33	6.706	1759	1762	1766	rVV2	609	412	0.02%	0.003%
34	6.777	1782	1784	1789	rVB2	433	311	0.02%	0.002%
35	6.986	1834	1849	1887	rBV	195441	379422	18.33%	2.623%
36	7.185	1905	1911	1912	rBV2	352	351	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027030.D
 Acq On : 28 Jul 2022 04:25
 Operator : SY/MD
 Sample : N3897-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	7.211	1912	1919	1921	rBV3	739	840	0.04%	0.006%
38	7.314	1938	1951	1985	rBV	863748	1523188	73.60%	10.531%
39	7.526	2015	2017	2020	rVB3	698	372	0.02%	0.003%
40	7.619	2034	2046	2069	rBV	135694	248919	12.03%	1.721%
41	7.805	2102	2104	2109	rBV4	389	348	0.02%	0.002%
42	7.892	2129	2131	2137	rVB3	566	441	0.02%	0.003%
43	7.937	2137	2145	2150	rBV3	3750	6302	0.30%	0.044%
44	7.979	2152	2158	2169	rVB6	9598	16339	0.79%	0.113%
45	8.024	2169	2172	2175	rBV	455	316	0.02%	0.002%
46	8.092	2180	2193	2233	rBV	402382	919999	44.46%	6.361%
47	8.368	2277	2279	2281	rBV3	544	326	0.02%	0.002%
48	8.416	2291	2294	2296	rVB2	618	344	0.02%	0.002%
49	8.436	2296	2300	2301	rBV3	455	306	0.01%	0.002%
50	8.568	2339	2341	2347	rVB4	325	296	0.01%	0.002%
51	8.651	2362	2367	2371	rBV3	370	415	0.02%	0.003%
52	8.850	2417	2429	2463	rBV	767046	1260395	60.90%	8.714%
53	9.034	2482	2486	2492	rVB4	951	988	0.05%	0.007%
54	9.066	2492	2496	2500	rBV3	671	546	0.03%	0.004%
55	9.294	2565	2567	2573	rVB4	418	364	0.02%	0.003%
56	9.378	2588	2593	2596	rVB2	335	343	0.02%	0.002%
57	9.555	2642	2648	2655	rBV4	817	1113	0.05%	0.008%
58	9.863	2741	2744	2749	rVB2	331	317	0.02%	0.002%
59	10.047	2795	2801	2805	rVB2	359	362	0.02%	0.003%
60	10.095	2809	2816	2823	rBV3	485	633	0.03%	0.004%
61	10.214	2841	2853	2877	rVV	673546	1071458	51.77%	7.408%
62	10.384	2897	2906	2913	rVB2	4479	6642	0.32%	0.046%
63	10.519	2943	2948	2951	rBV3	454	515	0.02%	0.004%
64	10.551	2951	2958	2962	rBV3	444	637	0.03%	0.004%
65	10.587	2967	2969	2974	rVB3	431	319	0.02%	0.002%
66	10.657	2988	2991	2996	rBV2	381	311	0.02%	0.002%
67	10.764	3016	3024	3028	rVB3	408	574	0.03%	0.004%
68	10.883	3057	3061	3066	rVB2	396	404	0.02%	0.003%
69	10.918	3066	3072	3073	rBV	663	557	0.03%	0.004%
70	11.156	3142	3146	3150	rBV3	363	386	0.02%	0.003%
71	11.246	3162	3174	3201	rBV	691163	1084480	52.40%	7.498%
72	11.487	3247	3249	3254	rVB3	499	314	0.02%	0.002%
73	11.532	3254	3263	3277	rBV2	17991	34180	1.65%	0.236%
74	11.622	3280	3291	3312	rVV	830172	1294633	62.56%	8.951%
75	11.892	3373	3375	3381	rVB3	430	369	0.02%	0.003%
76	12.027	3414	3417	3423	rVB4	360	318	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027030.D
 Acq On : 28 Jul 2022 04:25
 Operator : SY/MD
 Sample : N3897-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.214	3470	3475	3479	rBV2	432	491	0.02%	0.003%
78	12.362	3517	3521	3526	rBV3	419	352	0.02%	0.002%
79	12.439	3541	3545	3551	rBV2	275	355	0.02%	0.002%
80	12.648	3607	3610	3612	rBV2	493	324	0.02%	0.002%
81	12.661	3612	3614	3617	rVB	545	305	0.01%	0.002%
82	12.709	3624	3629	3635	rBV3	289	499	0.02%	0.003%
83	12.825	3661	3665	3668	rBV2	398	467	0.02%	0.003%
84	13.198	3773	3781	3785	rBV3	830	1058	0.05%	0.007%
85	13.291	3807	3810	3814	rBV2	583	428	0.02%	0.003%
86	13.506	3868	3877	3889	rBV	6134	10066	0.49%	0.070%
87	13.612	3905	3910	3912	rBV4	445	440	0.02%	0.003%
88	13.625	3912	3914	3918	rVB2	608	347	0.02%	0.002%
89	13.683	3929	3932	3934	rBV	512	356	0.02%	0.002%
90	13.757	3953	3955	3959	rVB3	480	316	0.02%	0.002%
91	13.792	3963	3966	3970	rBV2	528	433	0.02%	0.003%
92	13.815	3970	3973	3979	rVV3	683	480	0.02%	0.003%
93	13.850	3981	3984	3989	rVV2	610	422	0.02%	0.003%
94	14.127	4064	4070	4072	rBV3	432	483	0.02%	0.003%
95	14.641	4222	4230	4240	rVB4	3768	6139	0.30%	0.042%
96	14.725	4253	4256	4259	rBV3	585	417	0.02%	0.003%
97	14.818	4278	4285	4294	rBV5	2155	3680	0.18%	0.025%
98	15.371	4454	4457	4462	rVB5	1570	1705	0.08%	0.012%
99	15.612	4530	4532	4535	rBV4	908	599	0.03%	0.004%
100	15.924	4626	4629	4635	rBV6	1045	871	0.04%	0.006%




Sum of corrected areas: 14463422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027030.D
Acq On : 28 Jul 2022 04:25
Operator : SY/MD
Sample : N3897-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

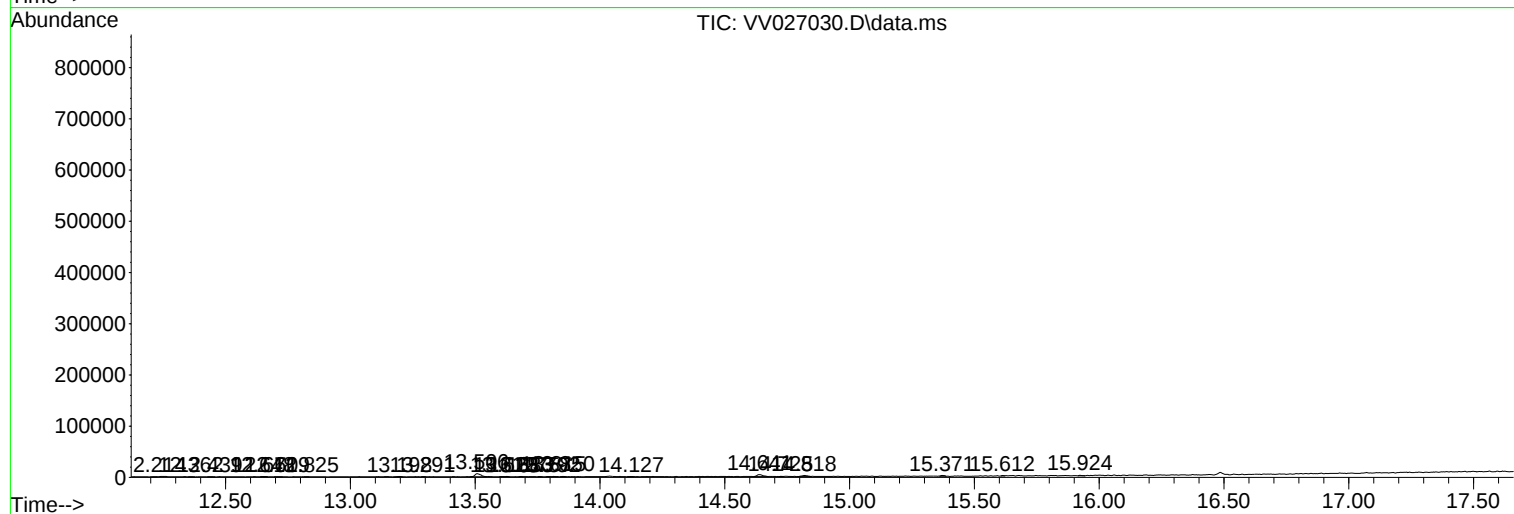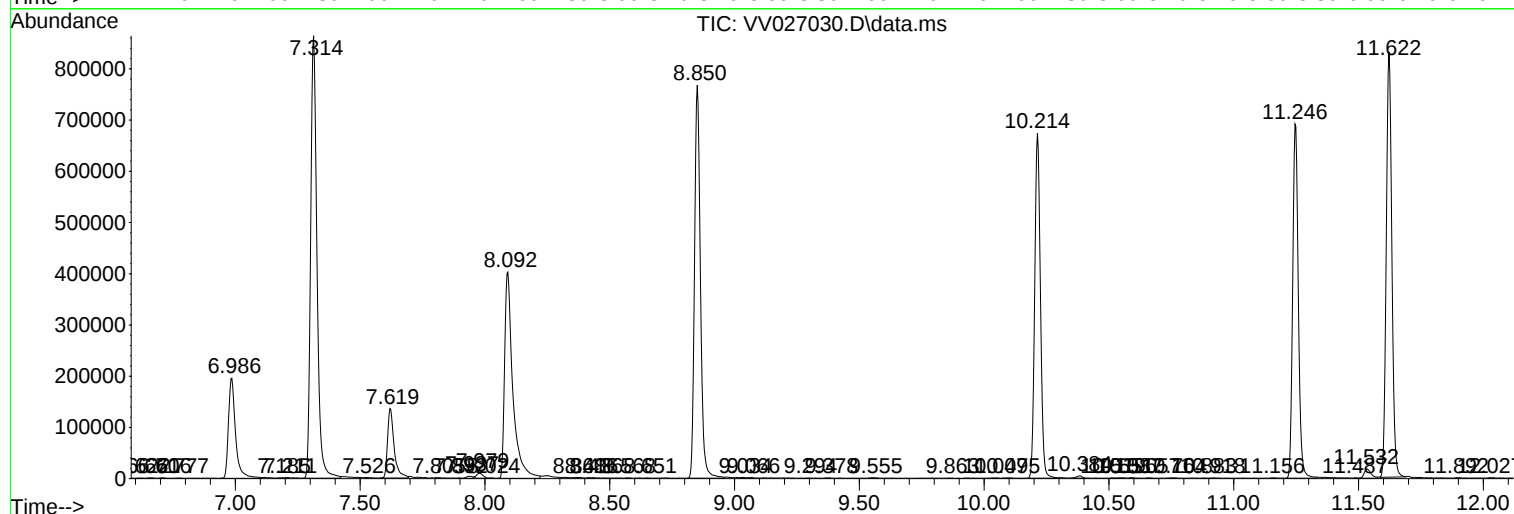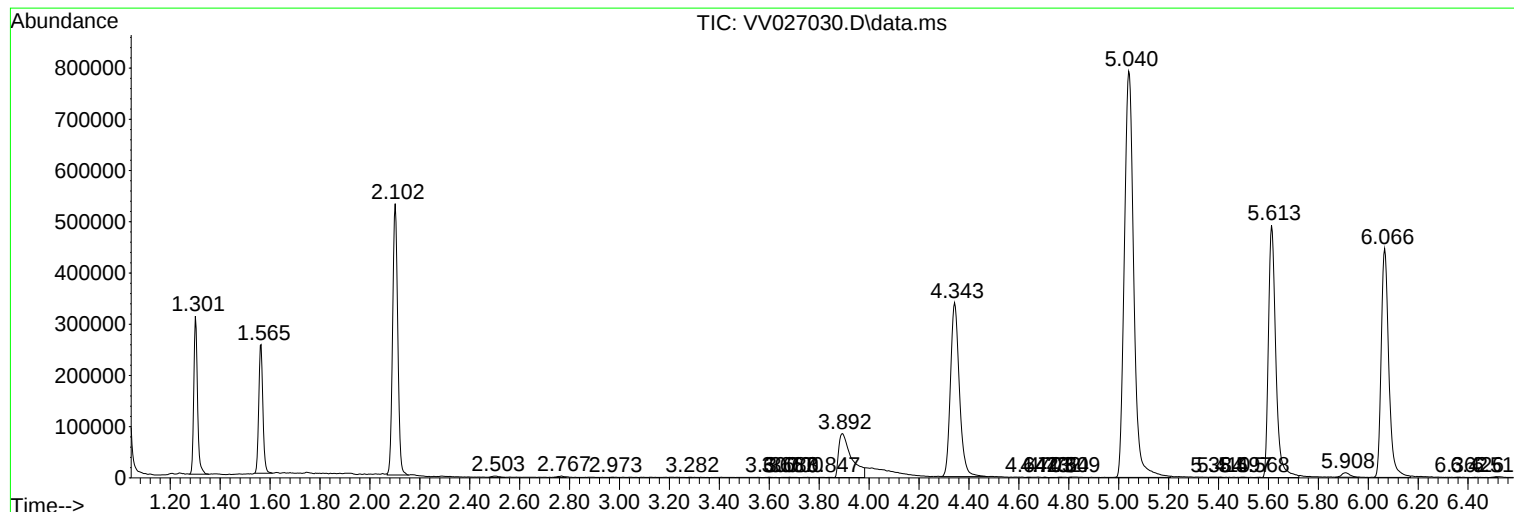

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027030.D
Acq On : 28 Jul 2022 04:25
Operator : SY/MD
Sample : N3897-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027030.D
Acq On : 28 Jul 2022 04:25
Operator : SY/MD
Sample : N3897-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc