

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027033.D
 Acq On : 28 Jul 2022 05:38
 Operator : SY/MD
 Sample : N3899-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	98	rVB	295202	309197	15.25%	2.218%
2	1.565	156	163	177	rVB	252119	289133	14.26%	2.074%
3	2.101	320	330	347	rVB	521231	739778	36.49%	5.308%
4	2.571	473	476	480	rBV2	604	444	0.02%	0.003%
5	2.806	546	549	554	rBV2	366	279	0.01%	0.002%
6	2.828	554	556	562	rBV3	308	249	0.01%	0.002%
7	3.047	621	624	626	rVB2	240	129	0.01%	0.001%
8	3.063	626	629	630	rBV	364	222	0.01%	0.002%
9	3.166	659	661	664	rVV	343	160	0.01%	0.001%
10	3.211	673	675	677	rBV2	234	106	0.01%	0.001%
11	3.256	685	689	694	rBV3	437	380	0.02%	0.003%
12	3.346	714	717	720	rBV2	281	225	0.01%	0.002%
13	3.420	737	740	743	rBV2	161	132	0.01%	0.001%
14	3.494	759	763	766	rBV2	243	217	0.01%	0.002%
15	3.548	776	780	784	rBV2	172	187	0.01%	0.001%
16	3.590	787	793	795	rBV2	359	296	0.01%	0.002%
17	3.651	808	812	818	rBV3	338	434	0.02%	0.003%
18	3.690	819	824	828	rBV2	366	415	0.02%	0.003%
19	3.767	844	848	850	rBV2	294	216	0.01%	0.002%
20	3.828	865	867	870	rBV	218	134	0.01%	0.001%
21	3.892	876	887	917	rBV	80644	291049	14.36%	2.088%
22	4.343	1013	1027	1055	rBV2	324816	801409	39.53%	5.750%
23	4.693	1132	1136	1139	rBV3	573	509	0.03%	0.004%
24	4.741	1148	1151	1152	rBV2	281	162	0.01%	0.001%
25	4.777	1159	1162	1164	rVB2	424	200	0.01%	0.001%
26	4.789	1164	1166	1167	rBV	222	111	0.01%	0.001%
27	4.863	1186	1189	1192	rBV3	401	250	0.01%	0.002%
28	4.880	1192	1194	1195	rVV	219	69	0.00%	0.000%
29	4.908	1200	1203	1204	rBV	298	177	0.01%	0.001%
30	5.043	1228	1245	1294	rBV2	773069	2027107	100.00%	14.544%
31	5.317	1327	1330	1336	rBV5	544	633	0.03%	0.005%
32	5.359	1340	1343	1348	rBV3	339	358	0.02%	0.003%
33	5.481	1377	1381	1382	rBV	363	293	0.01%	0.002%
34	5.507	1387	1389	1393	rVV4	331	266	0.01%	0.002%
35	5.564	1406	1407	1410	rVB	316	116	0.01%	0.001%
36	5.613	1410	1422	1454	rBV	471331	971945	47.95%	6.973%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027033.D
 Acq On : 28 Jul 2022 05:38
 Operator : SY/MD
 Sample : N3899-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	5.912	1505	1515	1533	rVB3	9559	19818	0.98%	0.142%
38	6.015	1544	1547	1549	rBV	540	261	0.01%	0.002%
39	6.066	1549	1563	1598	rBV	438878	919196	45.35%	6.595%
40	6.494	1691	1696	1699	rBV2	507	520	0.03%	0.004%
41	6.555	1711	1715	1716	rBV	393	265	0.01%	0.002%
42	6.629	1736	1738	1741	rBV2	363	209	0.01%	0.001%
43	6.648	1742	1744	1745	rVB2	282	76	0.00%	0.001%
44	6.680	1752	1754	1756	rBV2	268	194	0.01%	0.001%
45	6.822	1794	1798	1802	rVB	552	419	0.02%	0.003%
46	6.847	1802	1806	1809	rBV2	357	363	0.02%	0.003%
47	6.883	1813	1817	1819	rVB3	272	192	0.01%	0.001%
48	6.905	1821	1824	1826	rBV2	135	95	0.00%	0.001%
49	6.931	1829	1832	1837	rVB2	320	198	0.01%	0.001%
50	6.982	1837	1848	1883	rBV	183696	356312	17.58%	2.556%
51	7.233	1924	1926	1927	rBV2	369	194	0.01%	0.001%
52	7.314	1939	1951	1981	rBV	834578	1492126	73.61%	10.706%
53	7.619	2036	2046	2069	rBV	129947	240889	11.88%	1.728%
54	7.809	2103	2105	2108	rBV3	581	355	0.02%	0.003%
55	7.937	2139	2145	2151	rBV	3934	6051	0.30%	0.043%
56	8.031	2172	2174	2177	rVB2	241	107	0.01%	0.001%
57	8.050	2177	2180	2182	rBV2	317	218	0.01%	0.002%
58	8.092	2182	2193	2234	rBV	373231	878506	43.34%	6.303%
59	8.658	2367	2369	2373	rBV2	459	245	0.01%	0.002%
60	8.690	2378	2379	2383	rVB2	251	129	0.01%	0.001%
61	8.722	2384	2389	2391	rBV2	379	346	0.02%	0.002%
62	8.850	2416	2429	2457	rBV	744023	1222177	60.29%	8.769%
63	9.214	2540	2542	2547	rVB2	400	247	0.01%	0.002%
64	9.272	2557	2560	2562	rVB	295	153	0.01%	0.001%
65	9.310	2569	2572	2577	rVB3	493	414	0.02%	0.003%
66	9.490	2625	2628	2632	rBV2	232	258	0.01%	0.002%
67	9.551	2644	2647	2649	rBV2	615	418	0.02%	0.003%
68	9.593	2656	2660	2663	rVB2	375	258	0.01%	0.002%
69	9.609	2663	2665	2669	rBV2	175	112	0.01%	0.001%
70	9.693	2687	2691	2692	rBV	194	148	0.01%	0.001%
71	9.725	2697	2701	2703	rBV2	353	229	0.01%	0.002%
72	9.809	2724	2727	2728	rBV2	339	171	0.01%	0.001%
73	9.857	2738	2742	2746	rBV	476	354	0.02%	0.003%
74	9.883	2746	2750	2751	rBV	263	145	0.01%	0.001%
75	9.992	2782	2784	2789	rBV	164	138	0.01%	0.001%
76	10.037	2792	2798	2800	rBV	469	409	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027033.D
 Acq On : 28 Jul 2022 05:38
 Operator : SY/MD
 Sample : N3899-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.092	2814	2815	2816	rBV	307	72	0.00%	0.001%
78	10.214	2841	2853	2878	rBV	666192	1043115	51.46%	7.484%
79	10.481	2931	2936	2937	rBV	287	277	0.01%	0.002%
80	10.513	2942	2946	2951	rBV2	601	499	0.02%	0.004%
81	10.538	2951	2954	2956	rBV2	511	334	0.02%	0.002%
82	10.577	2964	2966	2969	rBV2	415	247	0.01%	0.002%
83	10.635	2979	2984	2988	rBV2	484	427	0.02%	0.003%
84	10.661	2988	2992	2995	rVB2	377	233	0.01%	0.002%
85	10.735	3012	3015	3017	rBV3	402	240	0.01%	0.002%
86	10.805	3034	3037	3039	rVB2	203	109	0.01%	0.001%
87	10.821	3039	3042	3047	rBV	385	373	0.02%	0.003%
88	10.854	3050	3052	3056	rVB2	630	377	0.02%	0.003%
89	11.082	3119	3123	3126	rBV2	345	281	0.01%	0.002%
90	11.130	3136	3138	3141	rVB	336	175	0.01%	0.001%
91	11.149	3141	3144	3147	rVB3	258	179	0.01%	0.001%
92	11.169	3147	3150	3153	rBV2	498	312	0.02%	0.002%
93	11.198	3153	3159	3162	rBV3	338	378	0.02%	0.003%
94	11.246	3163	3174	3200	rBV	665866	1048218	51.71%	7.521%
95	11.538	3256	3265	3267	rBV5	4820	5849	0.29%	0.042%
96	11.622	3279	3291	3321	rBV	795055	1254513	61.89%	9.001%
97	12.130	3447	3449	3451	rBV2	371	175	0.01%	0.001%
98	12.320	3505	3508	3509	rBV	274	182	0.01%	0.001%
99	13.072	3739	3742	3745	rVB2	549	297	0.01%	0.002%
100	13.516	3875	3880	3882	rBV2	1001	1053	0.05%	0.008%




Sum of corrected areas: 13937817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027033.D
Acq On : 28 Jul 2022 05:38
Operator : SY/MD
Sample : N3899-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

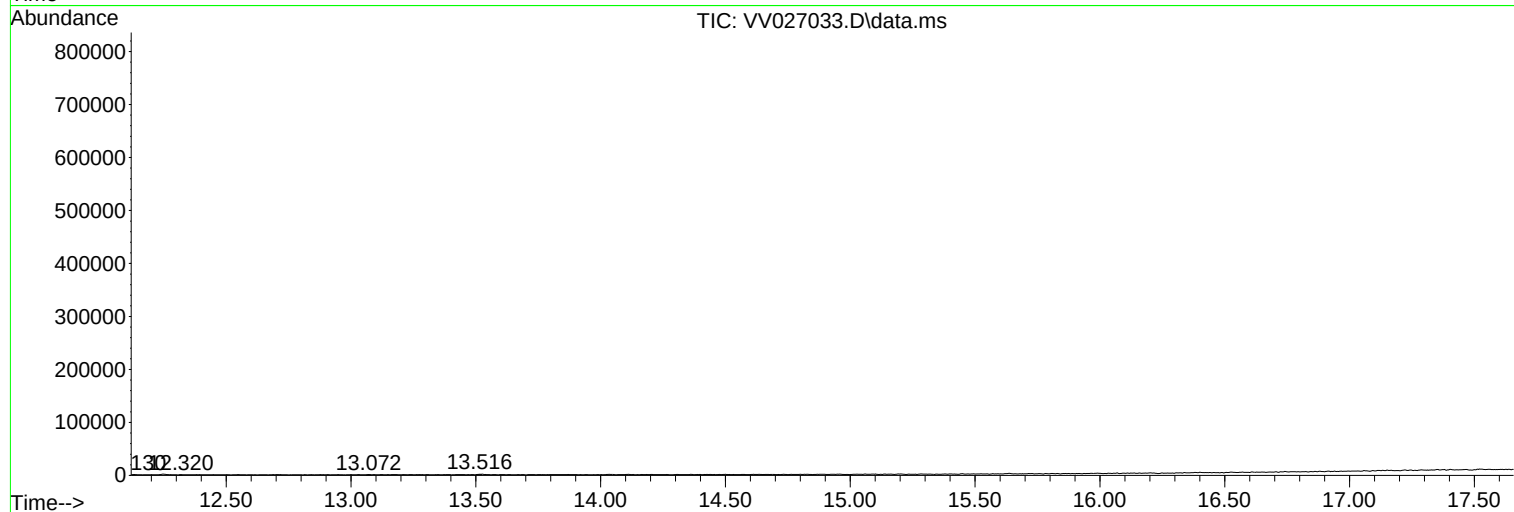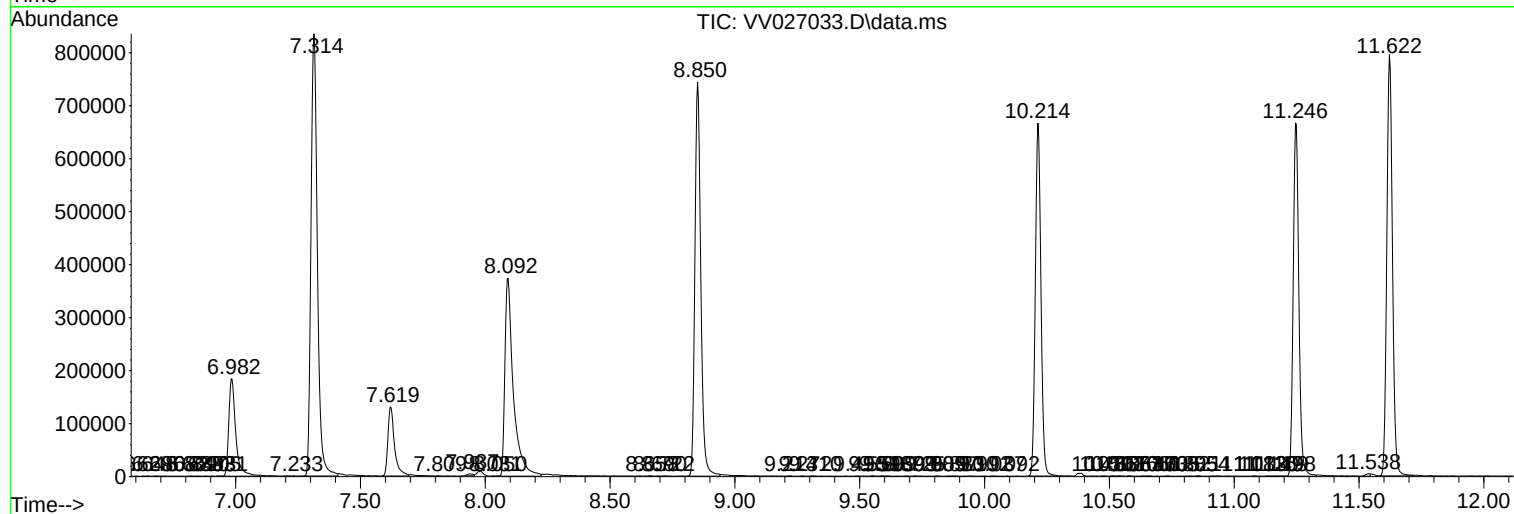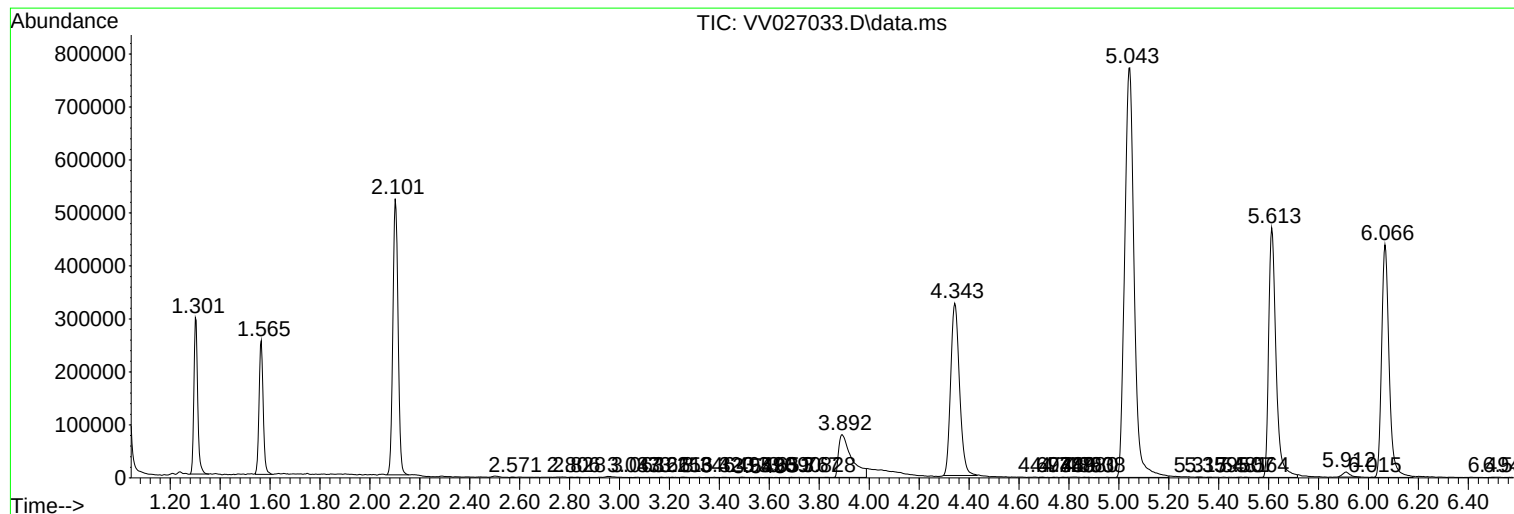

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027033.D
Acq On : 28 Jul 2022 05:38
Operator : SY/MD
Sample : N3899-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027033.D
Acq On : 28 Jul 2022 05:38
Operator : SY/MD
Sample : N3899-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc