

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027034.D
 Acq On : 28 Jul 2022 06:03
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV027034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	291142	307036	15.27%	2.210%
2	1.564	156	163	179	rVB	257556	289706	14.41%	2.085%
3	2.101	321	330	347	rVB	508241	718281	35.72%	5.169%
4	2.500	448	454	464	rVB5	3149	5305	0.26%	0.038%
5	2.915	578	583	589	rVB2	464	508	0.03%	0.004%
6	2.950	589	594	596	rBV3	745	718	0.04%	0.005%
7	2.989	604	606	607	rBV3	316	170	0.01%	0.001%
8	3.043	618	623	629	rBV4	480	412	0.02%	0.003%
9	3.153	653	657	661	rVB	375	299	0.01%	0.002%
10	3.179	661	665	668	rBV2	694	576	0.03%	0.004%
11	3.227	678	680	682	rBV	182	95	0.00%	0.001%
12	3.278	693	696	701	rBV2	222	205	0.01%	0.001%
13	3.301	701	703	707	rBV2	223	182	0.01%	0.001%
14	3.330	708	712	715	rVV2	456	314	0.02%	0.002%
15	3.371	721	725	728	rBV2	334	328	0.02%	0.002%
16	3.455	748	751	752	rVB3	227	91	0.00%	0.001%
17	3.503	763	766	769	rBV2	209	112	0.01%	0.001%
18	3.552	779	781	785	rVB2	564	300	0.01%	0.002%
19	3.580	785	790	793	rBV2	285	278	0.01%	0.002%
20	3.767	845	848	850	rBV	377	239	0.01%	0.002%
21	3.799	856	858	864	rVB2	386	228	0.01%	0.002%
22	3.831	864	868	873	rBV2	529	488	0.02%	0.004%
23	3.896	878	888	914	rBV	81649	304494	15.14%	2.191%
24	4.342	1013	1027	1066	rVB2	324391	807681	40.17%	5.813%
25	4.670	1127	1129	1130	rBV	338	91	0.00%	0.001%
26	4.812	1169	1173	1175	rBV2	762	646	0.03%	0.005%
27	4.883	1193	1195	1196	rVB	411	126	0.01%	0.001%
28	4.902	1199	1201	1209	rBV4	292	326	0.02%	0.002%
29	4.937	1209	1212	1214	rBV2	484	313	0.02%	0.002%
30	5.040	1226	1244	1281	rBV2	781679	2010606	100.00%	14.470%
31	5.484	1380	1382	1385	rVB4	341	172	0.01%	0.001%
32	5.497	1385	1386	1389	rVB2	397	158	0.01%	0.001%
33	5.613	1410	1422	1458	rBV	464062	974742	48.48%	7.015%
34	5.847	1492	1495	1501	rVB5	700	523	0.03%	0.004%
35	5.908	1504	1514	1528	rVV4	9691	20965	1.04%	0.151%
36	6.066	1547	1563	1595	rBV	439038	919476	45.73%	6.617%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027034.D
 Acq On : 28 Jul 2022 06:03
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.387	1660	1663	1667	rBV4	459	322	0.02%	0.002%
38	6.477	1688	1691	1693	rBV	282	148	0.01%	0.001%
39	6.603	1725	1730	1731	rBV	186	128	0.01%	0.001%
40	6.616	1731	1734	1735	rVV	362	186	0.01%	0.001%
41	6.635	1739	1740	1741	rBV	130	32	0.00%	0.000%
42	6.651	1741	1745	1748	rBV3	535	357	0.02%	0.003%
43	6.667	1748	1750	1752	rBV	276	130	0.01%	0.001%
44	6.757	1776	1778	1781	rBV2	303	193	0.01%	0.001%
45	6.802	1790	1792	1794	rBV3	220	110	0.01%	0.001%
46	6.841	1803	1804	1807	rBV	239	112	0.01%	0.001%
47	6.873	1810	1814	1815	rBV	206	80	0.00%	0.001%
48	6.918	1825	1828	1832	rBV2	241	190	0.01%	0.001%
49	6.940	1832	1835	1837	rVB	85	41	0.00%	0.000%
50	6.982	1837	1848	1876	rBV	180927	348366	17.33%	2.507%
51	7.313	1938	1951	1990	rBV	830647	1479190	73.57%	10.646%
52	7.619	2036	2046	2074	rBV	127823	239392	11.91%	1.723%
53	7.902	2132	2134	2136	rVB	526	234	0.01%	0.002%
54	7.921	2136	2140	2141	rBV3	950	629	0.03%	0.005%
55	8.018	2169	2170	2175	rBV2	343	203	0.01%	0.001%
56	8.092	2182	2193	2238	rBV	402638	904360	44.98%	6.509%
57	8.686	2373	2378	2380	rBV3	392	408	0.02%	0.003%
58	8.741	2392	2395	2398	rBV3	263	191	0.01%	0.001%
59	8.850	2418	2429	2457	rBV	732225	1224091	60.88%	8.810%
60	9.091	2502	2504	2508	rVB2	858	478	0.02%	0.003%
61	9.153	2516	2523	2528	rBV5	850	1058	0.05%	0.008%
62	9.185	2532	2533	2540	rBV4	311	335	0.02%	0.002%
63	9.281	2561	2563	2566	rBV2	226	110	0.01%	0.001%
64	9.297	2566	2568	2570	rBV	267	115	0.01%	0.001%
65	9.342	2578	2582	2583	rBV2	267	176	0.01%	0.001%
66	9.403	2598	2601	2603	rBV2	227	164	0.01%	0.001%
67	9.413	2603	2604	2605	rVV2	217	56	0.00%	0.000%
68	9.445	2611	2614	2616	rBV	192	135	0.01%	0.001%
69	9.490	2625	2628	2631	rBV	342	234	0.01%	0.002%
70	9.532	2638	2641	2644	rBV2	315	226	0.01%	0.002%
71	9.583	2654	2657	2658	rBV	307	159	0.01%	0.001%
72	9.702	2692	2694	2697	rBV3	206	125	0.01%	0.001%
73	9.744	2704	2707	2710	rVB	446	223	0.01%	0.002%
74	9.773	2713	2716	2718	rBV	261	146	0.01%	0.001%
75	9.841	2734	2737	2738	rBV	317	199	0.01%	0.001%
76	9.882	2747	2750	2753	rBV2	247	185	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
 Data File : VV027034.D
 Acq On : 28 Jul 2022 06:03
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	9.940	2757	2768	2774	rBV3	600	932	0.05%	0.007%
78	9.966	2774	2776	2779	rBV	182	104	0.01%	0.001%
79	10.017	2790	2792	2796	rBV2	143	64	0.00%	0.000%
80	10.040	2796	2799	2800	rBV2	379	196	0.01%	0.001%
81	10.214	2841	2853	2872	rBV	659239	1041759	51.81%	7.498%
82	10.426	2917	2919	2922	rVB	357	196	0.01%	0.001%
83	10.503	2941	2943	2949	rBV	262	175	0.01%	0.001%
84	10.567	2960	2963	2964	rBV	373	169	0.01%	0.001%
85	10.580	2964	2967	2971	rVB2	903	693	0.03%	0.005%
86	10.635	2980	2984	2988	rVB2	444	380	0.02%	0.003%
87	10.661	2988	2992	2994	rBV2	210	142	0.01%	0.001%
88	10.686	2997	3000	3003	rBV3	383	244	0.01%	0.002%
89	10.831	3042	3045	3047	rBV	265	204	0.01%	0.001%
90	11.088	3122	3125	3129	rVB2	376	261	0.01%	0.002%
91	11.107	3129	3131	3136	rBV2	244	123	0.01%	0.001%
92	11.165	3147	3149	3152	rBV2	423	150	0.01%	0.001%
93	11.246	3163	3174	3204	rBV	657537	1039549	51.70%	7.482%
94	11.509	3253	3256	3260	rBB3	520	433	0.02%	0.003%
95	11.548	3260	3268	3270	rBV3	1543	1984	0.10%	0.014%
96	11.622	3279	3291	3317	rBV	787392	1236932	61.52%	8.902%
97	11.985	3402	3404	3408	rVB2	403	197	0.01%	0.001%
98	12.805	3656	3659	3661	rBV2	393	249	0.01%	0.002%
99	13.898	3997	3999	4001	rBV2	431	204	0.01%	0.001%




Sum of corrected areas: 13894747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027034.D
Acq On : 28 Jul 2022 06:03
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

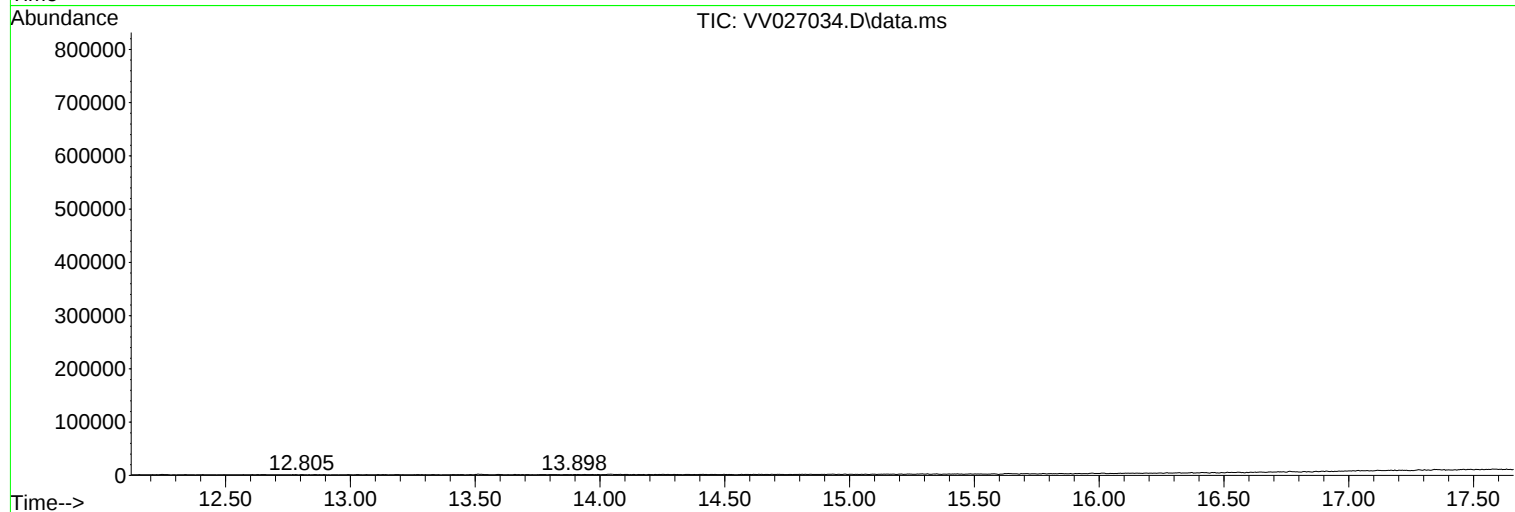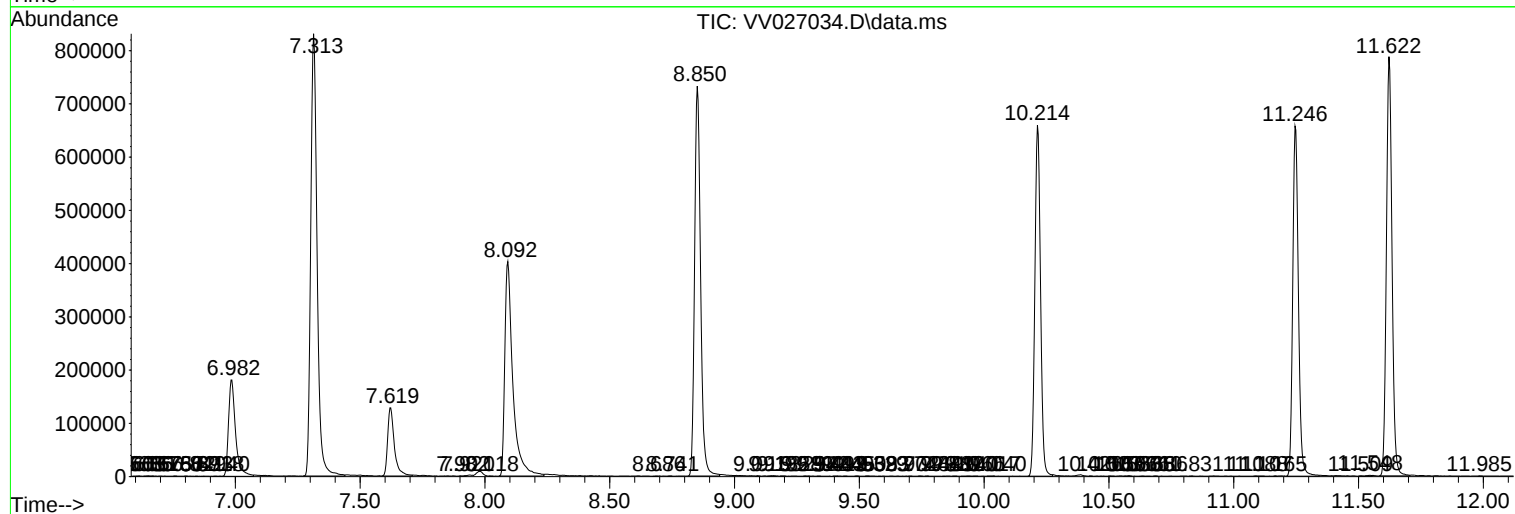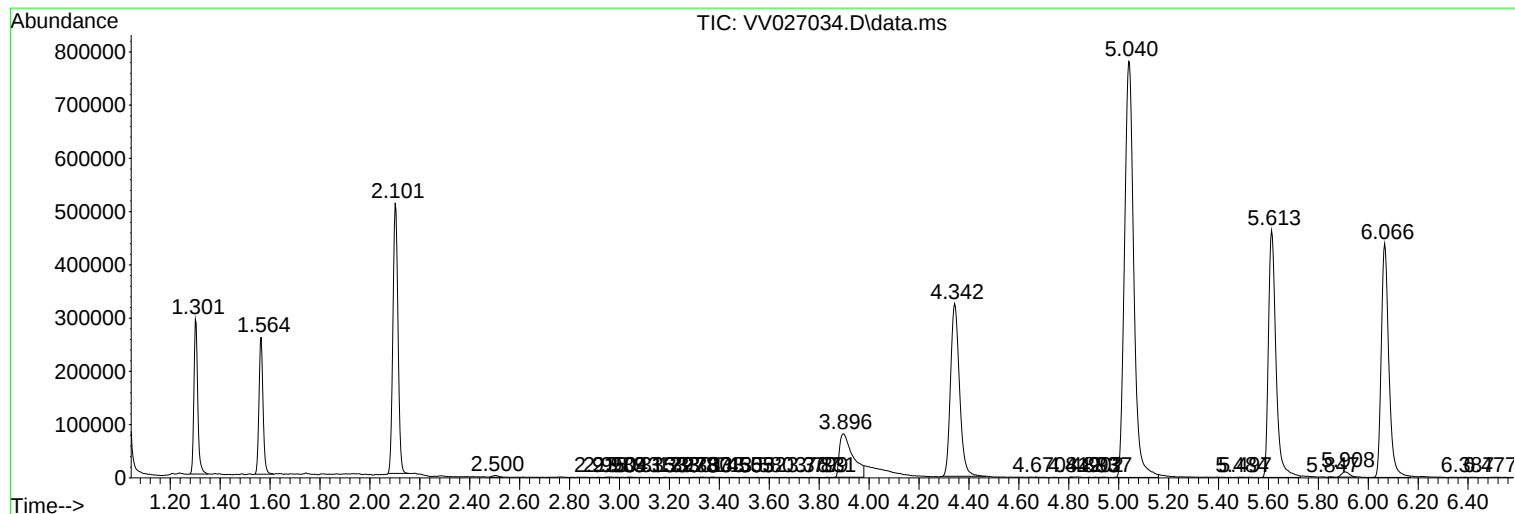

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027034.D
Acq On : 28 Jul 2022 06:03
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV027034.D
Acq On : 28 Jul 2022 06:03
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc