
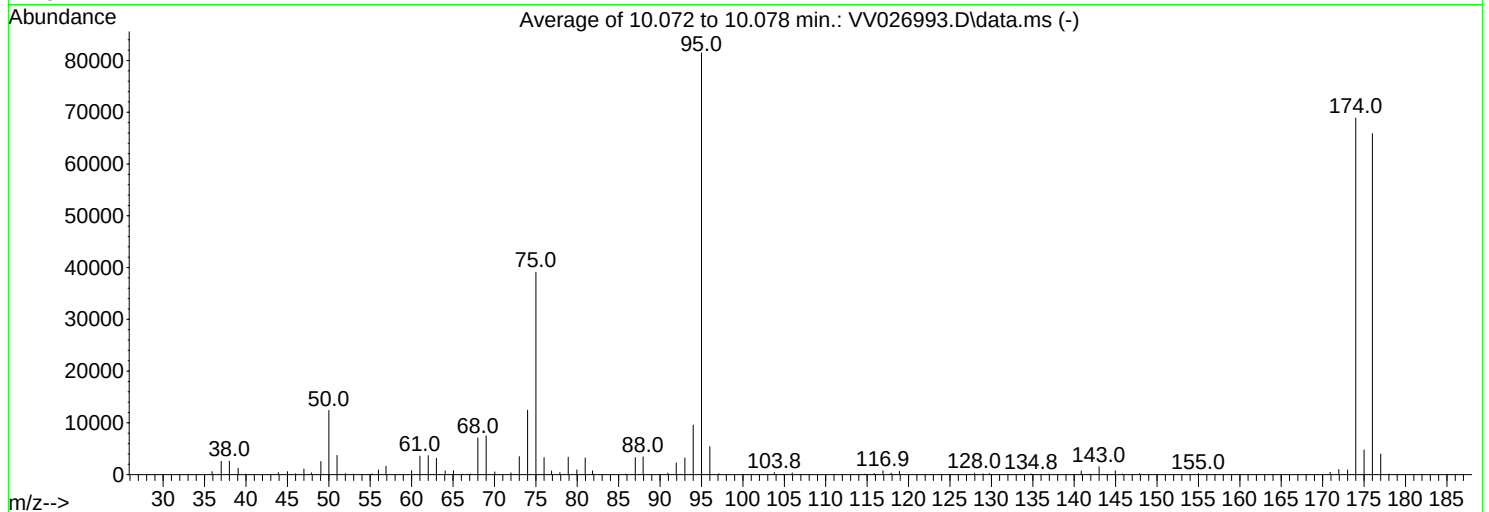


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072722\
Data File : VV026993.D
Acq On : 27 Jul 2022 09:24
Operator : SY/MD
Sample : BFB300
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB300

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis
Last Update : Thu Jul 28 02:51:09 2022

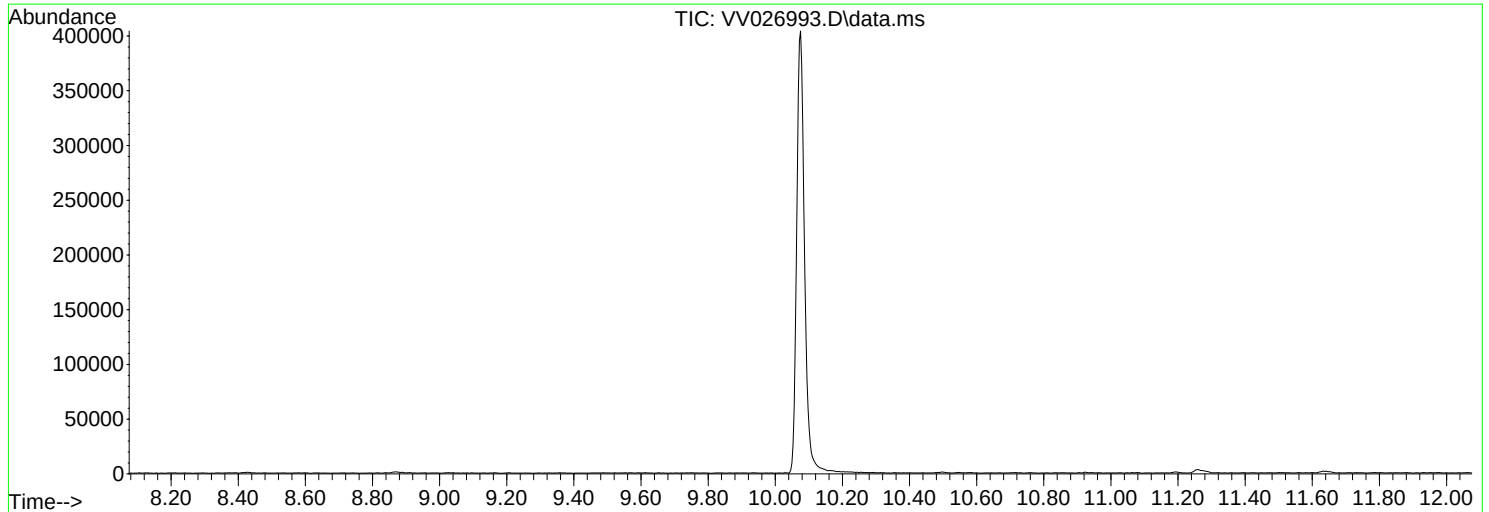

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12401	PASS
75	95	30	80	48.0	39096	PASS
95	95	100	100	100.0	81475	PASS
96	95	5	9	6.6	5410	PASS
173	174	0.00	2	1.3	898	PASS
174	95	50	120	84.5	68859	PASS
175	174	5	9	6.9	4759	PASS
176	174	95	105	95.7	65875	PASS
177	176	5	10	6.1	3987	PASS

m/z	Abundance
39.90	247.0
43.90	554.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
35.90	635.0
37.00	2605.0
38.00	2707.0
39.10	1287.0
39.90	400.0
43.90	973.0
44.90	577.0
46.00	174.0
47.00	1098.0
47.90	392.0
49.10	2552.0
50.00	12929.0
51.00	3699.0
52.00	223.0
53.00	138.0
54.70	149.0
55.20	135.0
56.00	904.0
56.90	1642.0
60.00	813.0
61.00	3802.0
62.00	3697.0
63.00	3070.0
64.00	789.0
65.10	746.0
66.10	146.0
66.80	163.0
68.00	7315.0
69.00	7512.0
70.10	486.0
72.00	289.0
73.00	3543.0
74.00	12978.0
75.00	39928.0
76.00	3398.0
76.90	716.0
77.90	432.0
78.90	3445.0
80.00	893.0
81.00	3139.0
81.90	701.0
87.00	3461.0
87.90	3411.0
90.90	276.0
92.00	2286.0
93.00	3274.0
94.00	9768.0
95.00	82216.0
96.00	5421.0
97.10	232.0
103.80	403.0
104.90	116.0
106.00	323.0
114.80	122.0
115.90	263.0
116.90	730.0
117.90	342.0
118.90	720.0
123.80	107.0
127.90	311.0
129.00	156.0
129.80	242.0
134.80	132.0
136.90	109.0
140.80	670.0
141.90	115.0
143.00	1614.0
145.00	720.0
145.90	138.0
148.00	228.0
154.90	264.0
171.00	407.0
172.00	1035.0
173.00	834.0
174.00	69768.0
175.00	4741.0
176.00	65256.0
177.00	4207.0
178.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
35.90	605.0
37.00	2643.0
38.00	2694.0
39.10	1262.0
39.90	379.0
43.90	1017.0
45.00	625.0
46.00	188.0
47.00	1149.0
47.90	374.0
49.10	2617.0
50.00	12801.0
51.00	3805.0
52.00	253.0
53.00	135.0
55.20	168.0
56.00	901.0
56.90	1726.0
60.00	822.0
61.00	3727.0
62.00	3809.0
63.00	3255.0
64.00	728.0
65.00	782.0
66.10	125.0
66.80	163.0
67.10	171.0
68.00	7262.0
69.00	7717.0
70.00	540.0
72.00	333.0
73.00	3665.0
74.00	12872.0
75.00	40384.0
76.00	3377.0
76.90	748.0
77.90	417.0
78.90	3493.0
79.90	961.0
80.90	3278.0
81.80	768.0
85.80	139.0
87.00	3340.0
88.00	3567.0
90.90	323.0
91.90	2323.0
93.00	3280.0
94.00	10019.0
95.00	84224.0
96.00	5544.0
97.10	182.0
103.80	422.0
104.90	113.0
106.00	367.0
114.80	126.0
115.80	267.0
116.90	765.0
117.90	337.0
118.90	679.0
127.90	274.0
129.00	157.0
129.70	211.0
134.80	161.0
136.90	120.0
140.90	753.0
141.90	135.0
143.00	1523.0
144.90	739.0
145.90	124.0
147.90	241.0
155.00	253.0
157.10	103.0
170.90	496.0
171.90	1006.0
173.00	924.0
174.00	71368.0
175.00	4913.0
176.00	68144.0
177.00	4038.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
35.90	510.0
37.00	2414.0
38.00	2444.0
39.00	1126.0
39.90	338.0
43.90	906.0
45.10	606.0
46.00	172.0
47.00	1026.0
47.90	307.0
49.00	2450.0
50.00	11472.0
51.00	3606.0
52.00	202.0
52.90	127.0
55.20	154.0
56.00	878.0
56.90	1595.0
60.00	726.0
61.00	3241.0
62.00	3501.0
63.00	3142.0
64.10	592.0
65.00	789.0
67.10	194.0
68.00	6756.0
69.00	7290.0
70.00	544.0
72.00	364.0
73.00	3316.0
74.00	11537.0
75.00	36976.0
76.00	3039.0
76.90	649.0
77.90	344.0
78.90	3182.0
79.90	922.0
80.90	3204.0
81.80	806.0
85.90	198.0
87.00	3106.0
88.00	3328.0
91.00	328.0
92.00	2176.0
93.00	3087.0
94.00	8976.0
95.00	77984.0
96.00	5264.0
97.10	129.0
103.80	381.0
105.90	338.0
114.70	110.0
115.80	260.0
116.90	738.0
117.90	289.0
118.90	592.0
128.00	250.0
129.00	146.0
129.80	200.0
134.80	154.0
137.00	128.0
140.90	749.0
141.90	137.0
143.00	1383.0
144.90	730.0
145.80	102.0
147.80	223.0
155.10	209.0
157.00	118.0
158.90	131.0
170.80	502.0
172.00	944.0
173.00	935.0
174.00	65440.0
175.00	4623.0
176.00	64224.0
177.00	3715.0
178.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300