

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072820\
 Data File : VV017697.D
 Acq On : 28 Jul 2020 11:52
 Operator : SY/MD
 Sample : L3446-01DL 5X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C47DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	60343	61788	13.12%	1.403%
2	1.579	145	152	165	rBV	48196	57363	12.18%	1.303%
3	2.122	312	321	337	rBV2	113072	174692	37.09%	3.968%
4	2.521	435	445	457	rBV4	10379	19048	4.04%	0.433%
5	3.929	871	883	885	rBV	43872	69639	14.78%	1.582%
6	4.373	1006	1021	1042	rBV	91930	224813	47.73%	5.106%
7	5.071	1221	1238	1256	rBV3	187581	454776	96.54%	10.329%
8	5.643	1402	1416	1441	rBV	188274	385670	81.87%	8.759%
9	5.939	1495	1508	1525	rBV	205055	404673	85.91%	9.191%
10	6.097	1544	1557	1578	rVB2	102118	211392	44.88%	4.801%
11	7.010	1830	1841	1856	rBV	55964	99476	21.12%	2.259%
12	7.338	1929	1943	1963	rBV	220460	389727	82.73%	8.851%
13	7.646	2028	2039	2052	rBV2	32211	57833	12.28%	1.313%
14	7.997	2134	2148	2164	rBV3	35727	65189	13.84%	1.481%
15	8.113	2173	2184	2211	rBV3	154932	316311	67.15%	7.184%
16	8.875	2409	2421	2437	rBV	283619	471057	100.00%	10.699%
17	10.238	2834	2845	2859	rBV	67936	110657	23.49%	2.513%
18	10.402	2884	2896	2904	rBV10	4023	7149	1.52%	0.162%
19	11.270	3153	3166	3180	rBV	279818	449004	95.32%	10.198%
20	11.646	3272	3283	3297	rBV	233765	372722	79.12%	8.465%


Sum of corrected areas: 4402979

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072820\
Data File : VV017697.D
Acq On : 28 Jul 2020 11:52
Operator : SY/MD
Sample : L3446-01DL 5X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C47DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

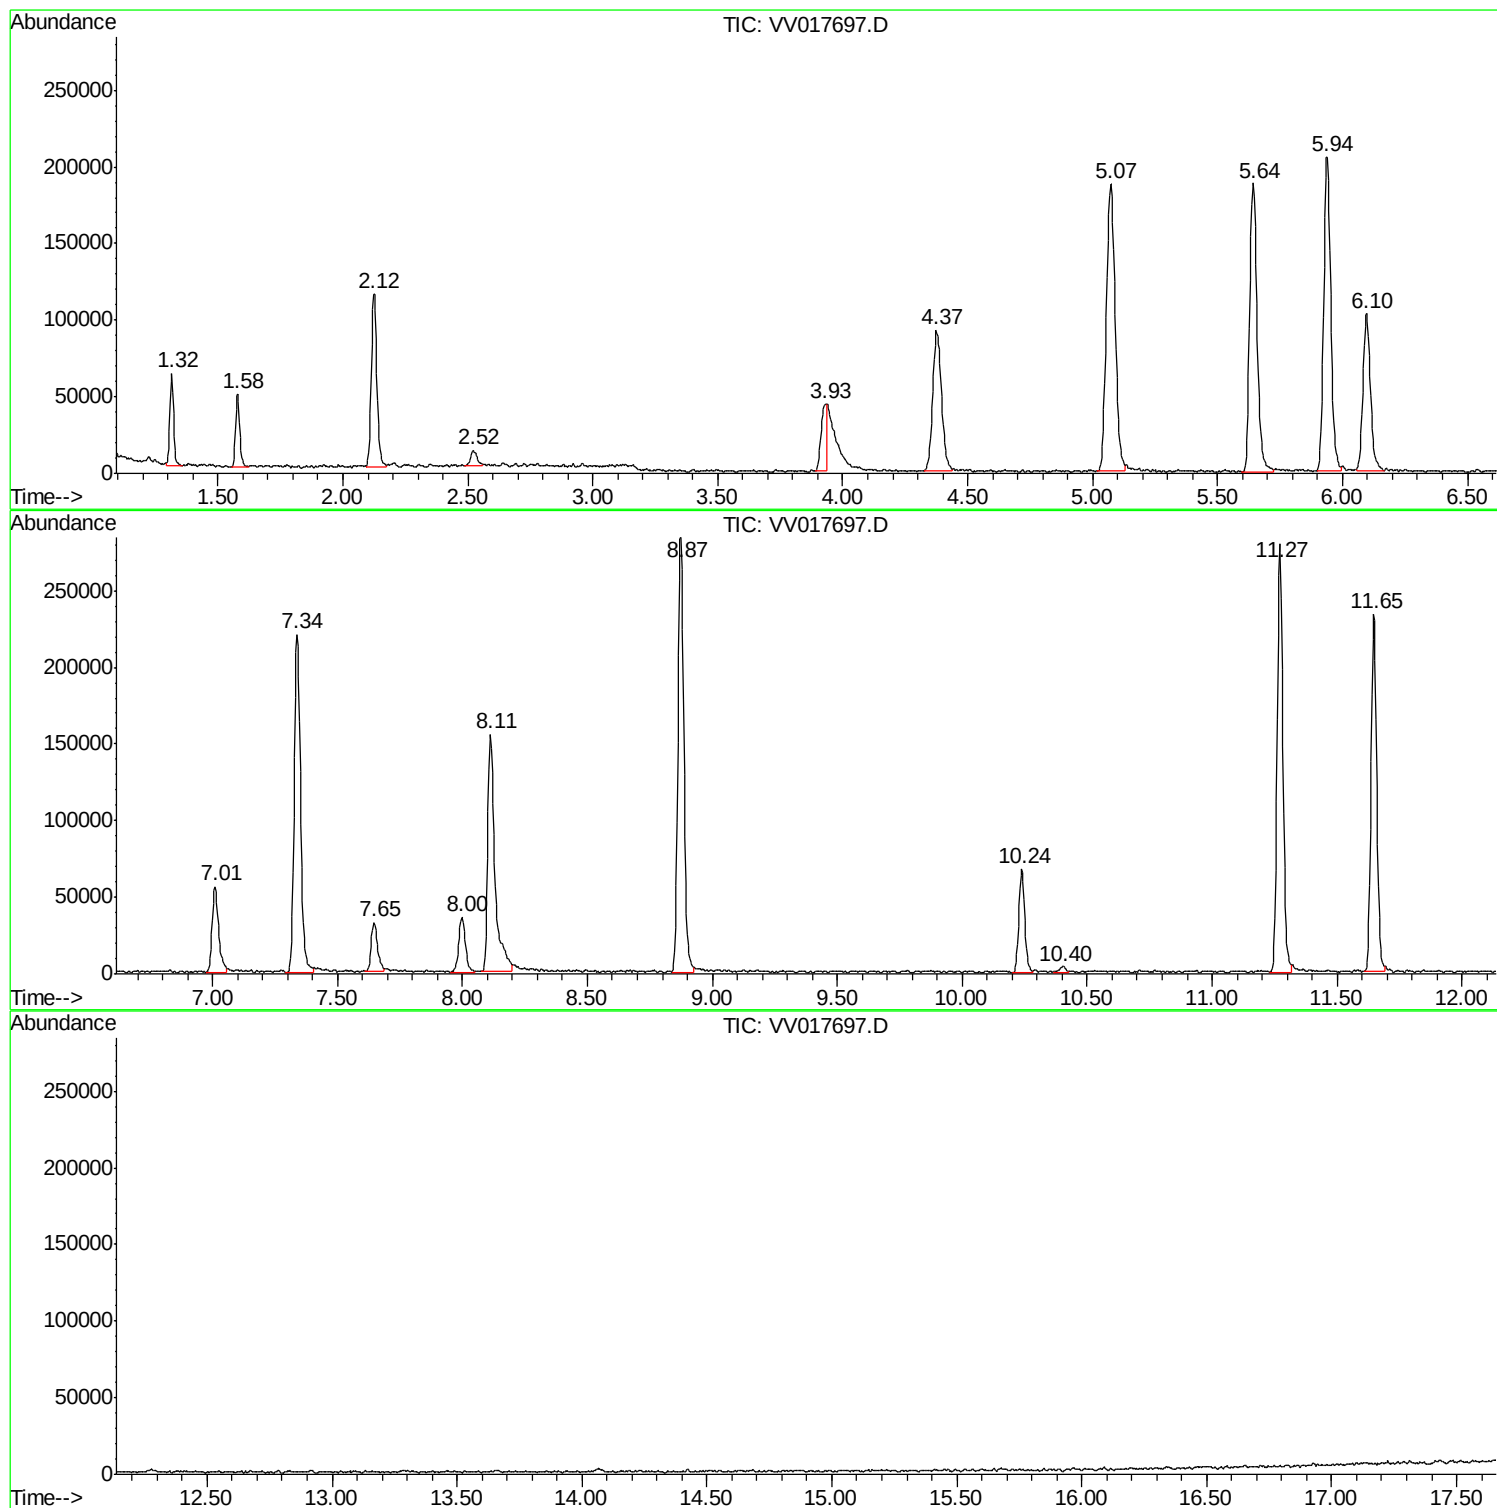

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072820\
Data File : VV017697.D
Acq On : 28 Jul 2020 11:52
Operator : SY/MD
Sample : L3446-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C47DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072820\
Data File : VV017697.D
Acq On : 28 Jul 2020 11:52
Operator : SY/MD
Sample : L3446-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C47DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc