


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072820\
 Data File : VV017692.D
 Acq On : 28 Jul 2020 08:55
 Operator : SY/MD
 Sample : BFB54
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 29 18:07:18 2020

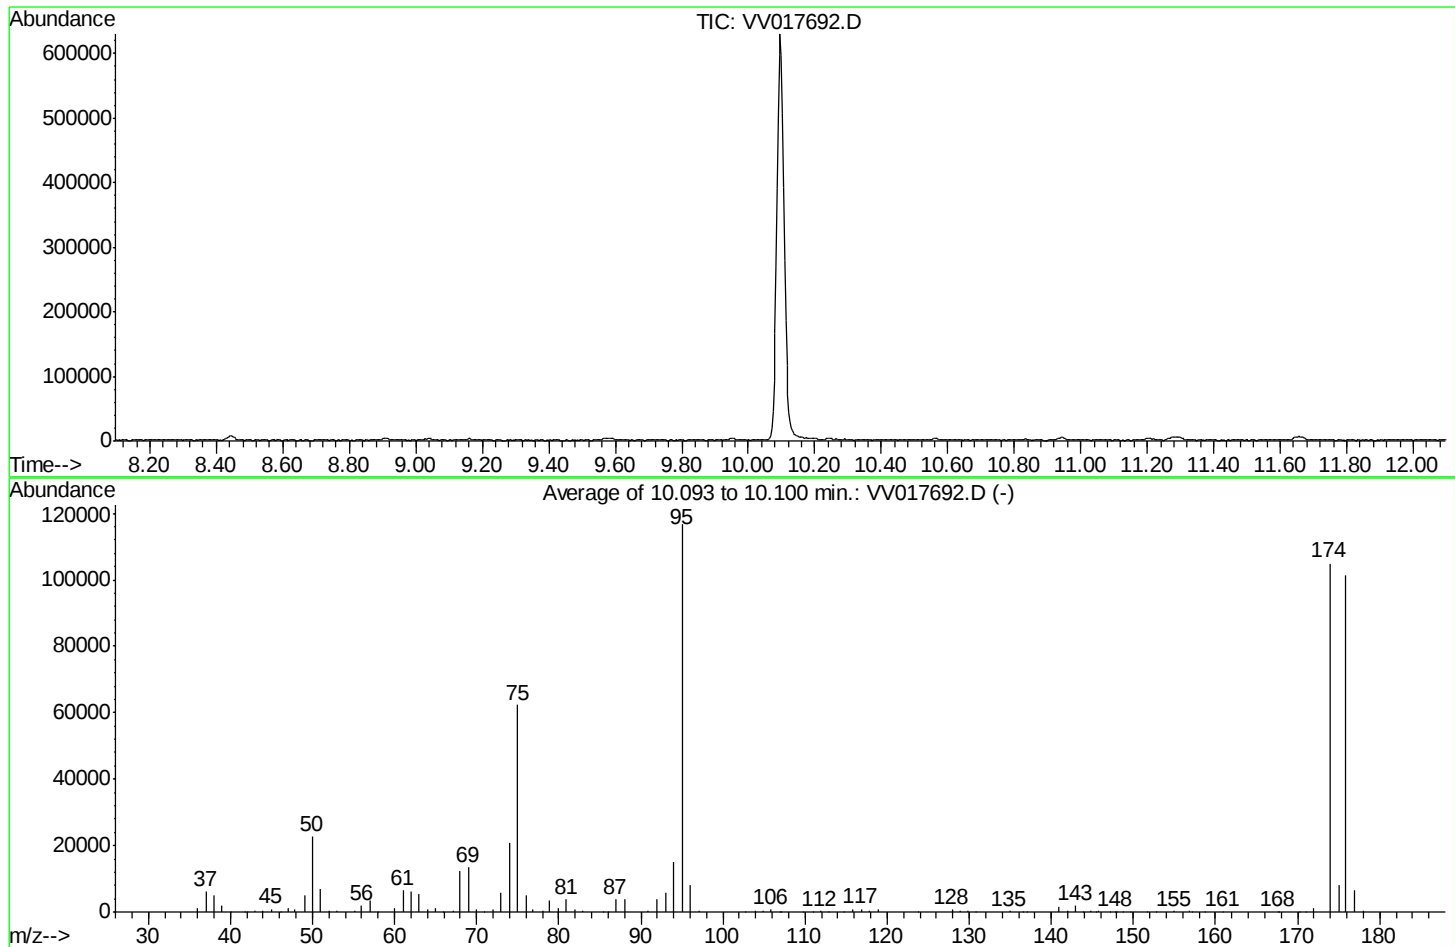

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	22669	PASS
75	95	30	80	53.4	62368	PASS
95	95	100	100	100.0	116701	PASS
96	95	5	9	6.9	8090	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.8	104821	PASS
175	174	5	9	7.6	7941	PASS
176	174	95	101	96.7	101333	PASS
177	176	5	9	6.4	6462	PASS

Scan 2788 (10.055 min): VV017692.D
BFB54

m/z	Abundance
36.00	146.0
36.30	138.0
38.90	101.0
39.60	107.0
40.10	190.0
41.30	106.0
44.00	339.0
45.00	184.0
56.70	112.0
60.50	120.0
63.30	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	1141.0
37.00	6175.0
38.00	5425.0
39.00	1972.0
40.00	303.0
41.70	106.0
43.00	207.0
44.00	839.0
45.10	1145.0
46.10	160.0
47.10	1011.0
47.90	711.0
49.00	5159.0
50.00	22832.0
51.00	6909.0
52.00	455.0
53.00	261.0
55.10	296.0
56.00	1930.0
57.00	3495.0
57.90	191.0
60.00	1215.0
61.00	6126.0
62.00	6324.0
63.00	5300.0
64.00	613.0
65.00	1091.0
67.10	415.0
68.00	12767.0
69.00	13094.0
70.00	737.0
70.90	144.0
72.10	723.0
73.00	5877.0
74.00	20416.0
75.00	61520.0
76.00	5002.0
76.90	615.0
78.10	365.0
78.90	3654.0
79.90	1134.0
80.90	3896.0
81.90	846.0
82.90	229.0
85.40	167.0
86.00	148.0
87.00	3762.0
88.00	3656.0
90.80	495.0
92.00	3814.0
93.00	5638.0
94.00	14636.0
95.00	115480.0
96.00	8369.0
97.10	272.0
104.00	466.0
105.00	213.0
105.90	606.0
106.80	130.0
107.10	121.0
110.80	163.0
111.80	193.0
112.90	128.0
114.80	128.0
115.90	505.0
116.90	914.0
117.80	523.0
118.90	853.0
123.80	115.0
127.90	600.0
128.80	327.0
129.90	454.0
130.60	215.0
135.00	266.0
136.60	180.0
137.00	169.0
140.90	1388.0
142.00	217.0
143.00	1928.0
143.90	168.0
144.80	579.0
145.50	312.0
147.10	160.0
147.80	304.0
148.70	126.0
149.70	109.0
151.70	105.0
155.00	393.0
156.90	251.0
158.70	196.0
160.90	136.0
172.00	1388.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

173.90	101440.0
175.00	7445.0
175.90	98264.0
177.00	6175.0
178.00	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	1251.0
37.00	6349.0
38.00	5375.0
39.10	2101.0
40.00	314.0
43.00	259.0
44.00	908.0
45.00	1184.0
46.10	137.0
47.00	993.0
47.90	646.0
49.00	5391.0
50.00	23408.0
51.00	6893.0
52.00	486.0
52.90	261.0
55.20	354.0
56.00	1803.0
57.00	3772.0
57.90	169.0
60.00	1274.0
61.00	6719.0
62.00	6335.0
63.00	5571.0
64.00	613.0
65.00	1100.0
67.10	509.0
68.00	13018.0
69.00	14062.0
70.00	899.0
70.90	157.0
72.10	805.0
73.00	5926.0
74.00	21784.0
75.00	64592.0
76.00	5151.0
76.90	634.0
78.10	510.0
78.90	3741.0
79.90	1193.0
80.90	3928.0
81.90	999.0
82.90	216.0
85.50	208.0
86.10	155.0
86.90	3885.0
88.00	3851.0
90.80	555.0
92.00	4129.0
93.00	6095.0
94.00	15735.0
95.00	120648.0
96.00	8485.0
97.10	239.0
102.60	120.0
103.90	453.0
105.00	217.0
105.90	613.0
106.90	152.0
109.80	118.0
110.90	149.0
111.80	244.0
112.80	125.0
114.80	136.0
115.90	614.0
116.90	970.0
117.80	515.0
118.90	790.0
127.90	701.0
128.80	345.0
129.80	513.0
130.70	186.0
134.90	289.0
136.60	165.0
137.00	132.0
140.90	1472.0
142.00	246.0
143.00	2025.0
143.80	180.0
144.80	556.0
145.70	357.0
147.10	155.0
147.80	290.0
148.80	111.0
152.70	115.0
155.00	410.0
156.90	212.0
158.80	190.0
160.90	171.0
167.50	103.0
170.20	191.0
172.00	1384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

173.90	108672.0
175.00	8189.0
175.90	105184.0
177.00	6665.0
178.00	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	1257.0
37.00	5694.0
38.10	4719.0
39.10	2102.0
40.00	319.0
42.00	117.0
42.90	227.0
44.00	937.0
45.00	1013.0
47.00	931.0
47.90	523.0
49.00	4939.0
50.00	21768.0
51.00	6496.0
52.00	489.0
52.90	263.0
55.00	355.0
56.00	1655.0
57.00	3369.0
58.00	153.0
60.00	1147.0
61.00	6307.0
62.00	5830.0
63.00	5121.0
64.10	572.0
65.00	1067.0
65.90	127.0
67.10	468.0
68.00	11759.0
69.00	13143.0
70.00	976.0
70.90	159.0
72.00	787.0
73.00	5460.0
74.00	20584.0
75.00	60992.0
76.00	4953.0
76.90	590.0
78.00	548.0
78.90	3513.0
79.90	1199.0
80.90	3615.0
81.90	978.0
82.90	203.0
85.50	212.0
86.20	154.0
86.90	3600.0
88.00	3589.0
90.80	542.0
92.00	3915.0
93.00	5823.0
94.00	14760.0
95.00	113976.0
96.00	7418.0
97.10	205.0
102.70	121.0
103.90	426.0
104.90	198.0
105.90	604.0
106.80	153.0
109.80	142.0
111.00	115.0
111.90	217.0
112.80	150.0
114.70	125.0
115.80	713.0
116.90	904.0
117.80	476.0
118.80	819.0
127.90	672.0
128.90	294.0
129.80	552.0
130.80	156.0
134.90	273.0
136.60	175.0
140.90	1452.0
142.00	241.0
143.00	1827.0
143.80	176.0
144.80	466.0
145.80	352.0
147.10	110.0
148.00	349.0
152.70	129.0
155.00	359.0
156.80	161.0
157.20	108.0
158.80	145.0
160.90	196.0
167.70	119.0
170.20	242.0
171.00	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

172.00	1310.0
173.90	104352.0
175.00	8190.0
175.90	100552.0
177.00	6546.0
178.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54