

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027050.D
 Acq On : 28 Jul 2022 21:37
 Operator : SY/MD
 Sample : VV0728MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Quant Time: Jul 29 02:11:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	550781	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	533980	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	230795	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	251099	47.920	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.840%		
7) Chloroethane-d5	1.561	69	210033	50.589	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	101.180%		
11) 1,1-Dichloroethene-d2	2.101	63	336139	37.680	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.360%		
21) 2-Butanone-d5	3.889	46	276132	92.418	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.420%		
24) Chloroform-d	4.342	84	463559	49.119	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.240%		
26) 1,2-Dichloroethane-d4	5.027	65	277487	51.796	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.600%		
32) Benzene-d6	5.047	84	958254	51.103	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.200%		
36) 1,2-Dichloropropane-d6	6.066	67	308795	53.804	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	107.600%		
41) Toluene-d8	7.313	98	820590	48.416	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.840%		
43) trans-1,3-Dichloroprop...	7.619	79	124453	49.089	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.180%		
47) 2-Hexanone-d5	8.088	63	247623	100.364	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.360%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	429966	49.687	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.380%		
66) 1,2-Dichlorobenzene-d4	11.622	152	289430	55.786	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.580%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	3618	0.881	ug/L	# 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027050.D
Acq On : 28 Jul 2022 21:37
Operator : SY/MD
Sample : VV0728MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK238

Quant Time: Jul 29 02:11:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

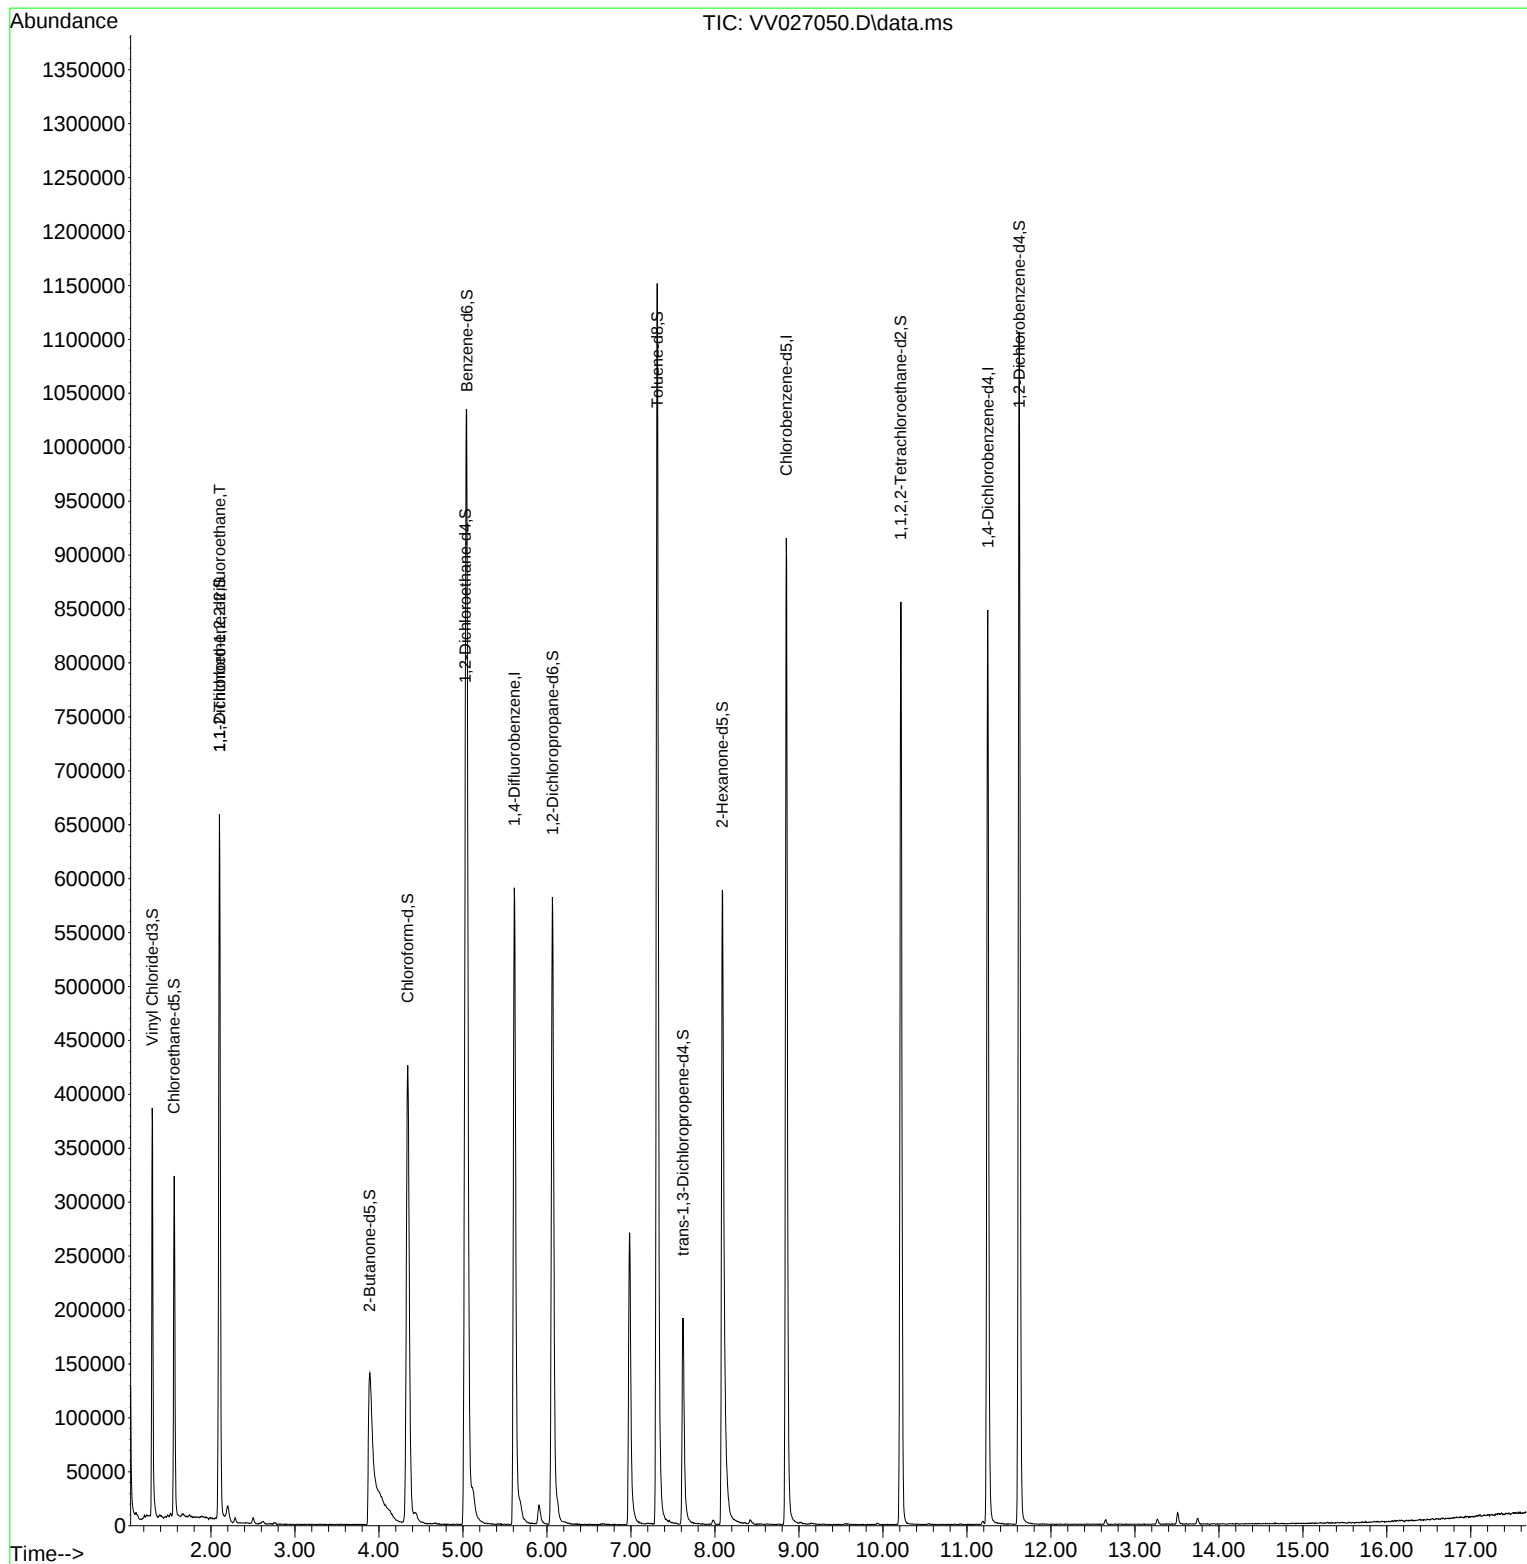

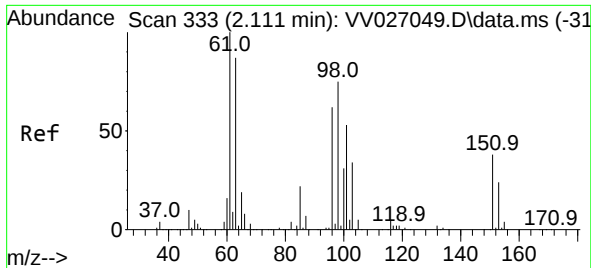

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.881 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV027050.D
 Acq: 28 Jul 2022 21:37

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Tgt Ion:101 Resp: 3618
 Ion Ratio Lower Upper
 101 100
 85 5.0 34.1 51.1#
 151 11.7 57.8 86.8#

