




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027052.D
 Acq On : 28 Jul 2022 22:26
 Operator : SY/MD
 Sample : N3897-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ6

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

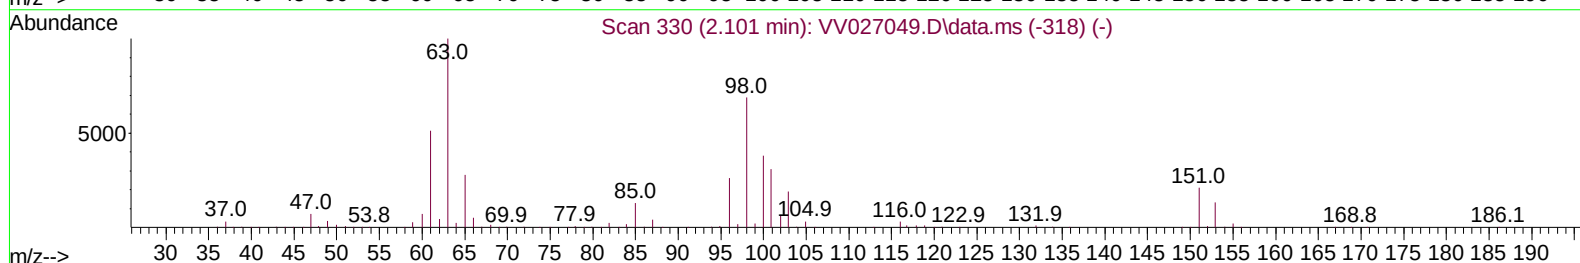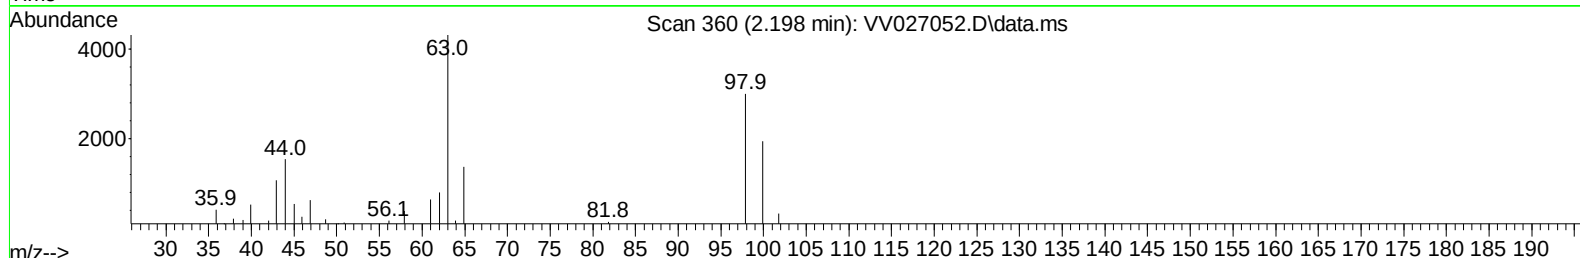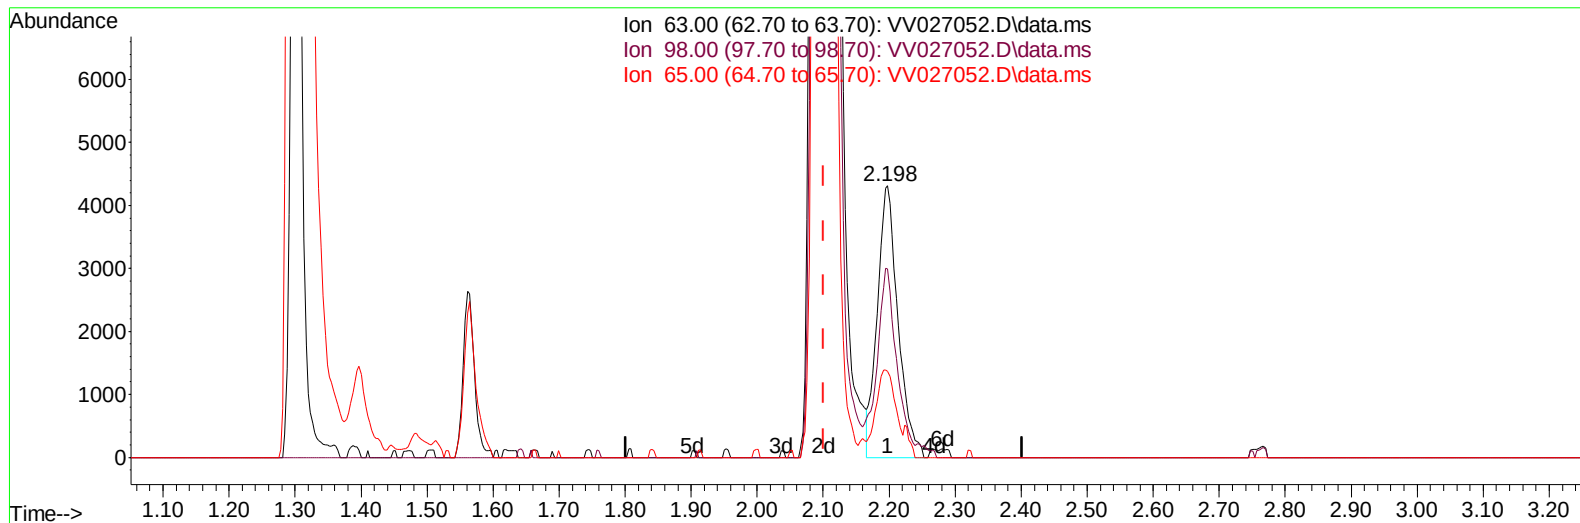

TIC: VV027052.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.198min (+ 0.096) 1.02 ug/L

response 9370

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	59.79
65.00	24.20	30.69
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027052.D
 Acq On : 28 Jul 2022 22:26
 Operator : SY/MD
 Sample : N3897-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 29 05:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

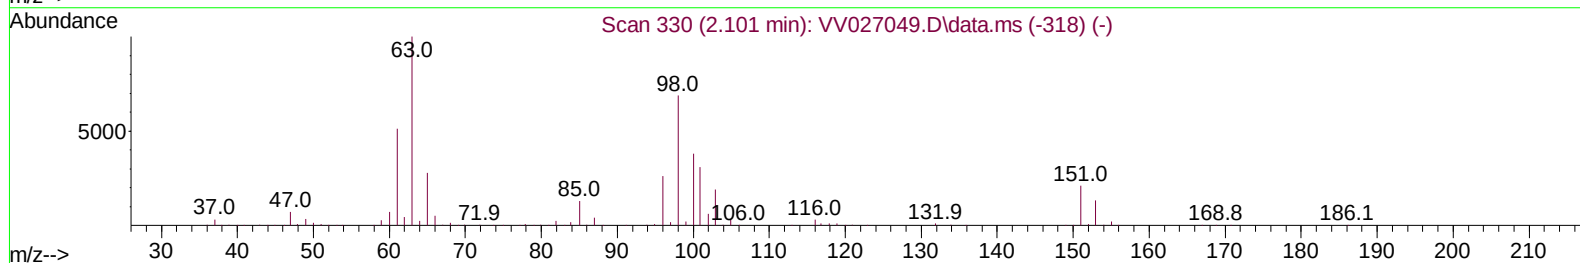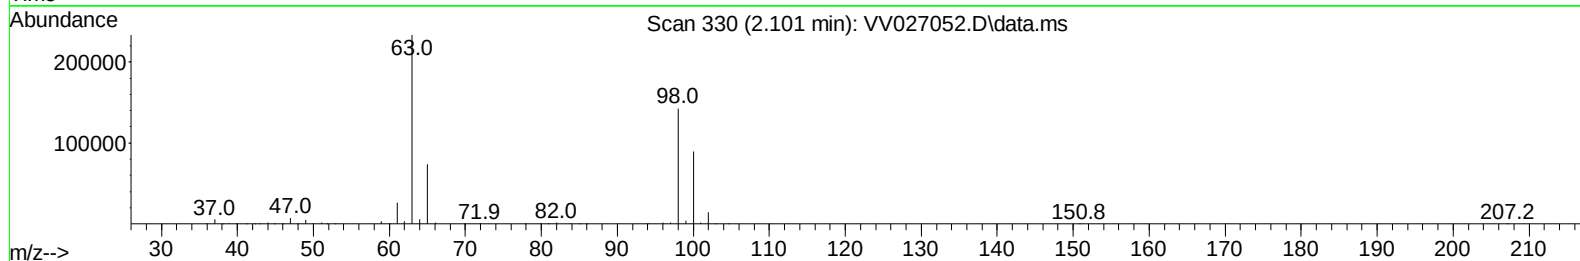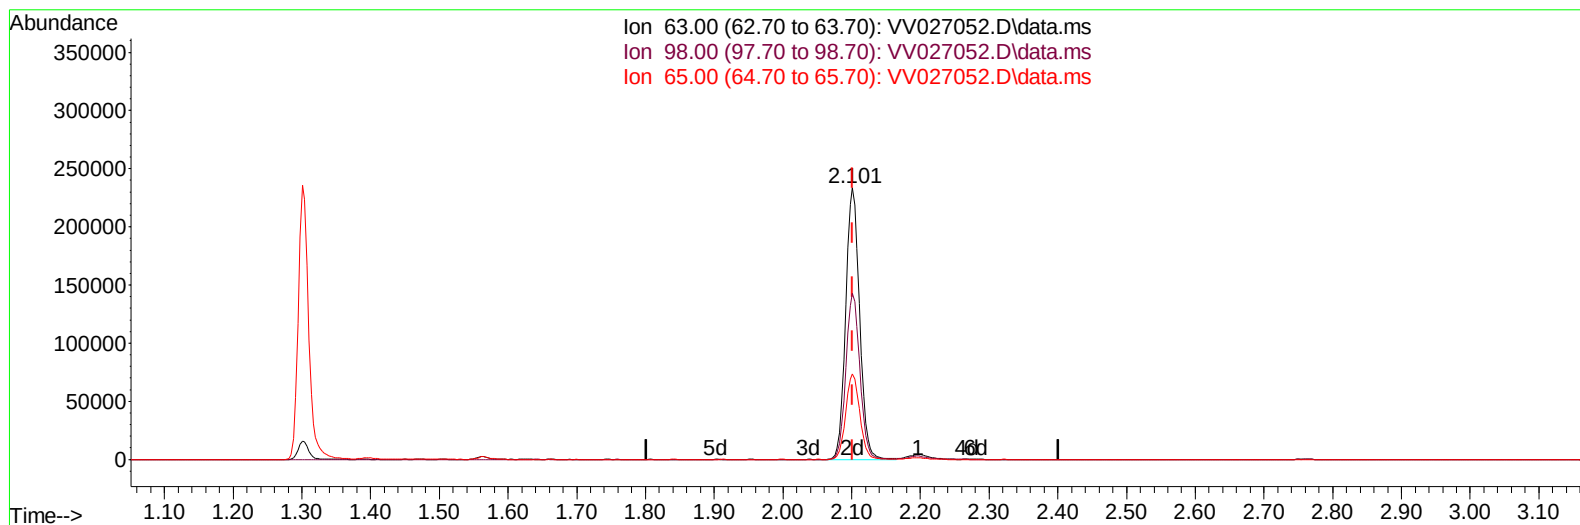

TIC: VV027052.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.000) 35.51 ug/L m

response 327505

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	1.71#
65.00	24.20	0.88#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027052.D
 Acq On : 28 Jul 2022 22:26
 Operator : SY/MD
 Sample : N3897-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUQ6

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	569413	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	565634	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	245255	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	246054	45.421	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	90.840%	
7) Chloroethane-d5	1.564	69	194583	45.335	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	90.660%	
11) 1,1-Dichloroethene-d2	2.101	63	327505m	35.511	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.020%	
21) 2-Butanone-d5	3.886	46	213876	69.239	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	69.240%	
24) Chloroform-d	4.342	84	421172	43.167	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.340%	
26) 1,2-Dichloroethane-d4	5.027	65	249932	45.126	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.260%	
32) Benzene-d6	5.046	84	877797	44.193	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.380%	
36) 1,2-Dichloropropane-d6	6.066	67	279910	46.042	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.080%	
41) Toluene-d8	7.313	98	752797	41.930	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	83.860%	
43) trans-1,3-Dichloroprop...	7.619	79	108525	40.411	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.820%	
47) 2-Hexanone-d5	8.088	63	211546	80.943	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	80.940%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	388494	42.383	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	84.760%	
66) 1,2-Dichlorobenzene-d4	11.622	152	279667	50.726	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	101.460%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027052.D
Acq On : 28 Jul 2022 22:26
Operator : SY/MD
Sample : N3897-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBUQ6

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:13:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

