




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027057.D
 Acq On : 29 Jul 2022 00:29
 Operator : SY/MD
 Sample : N3899-04 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

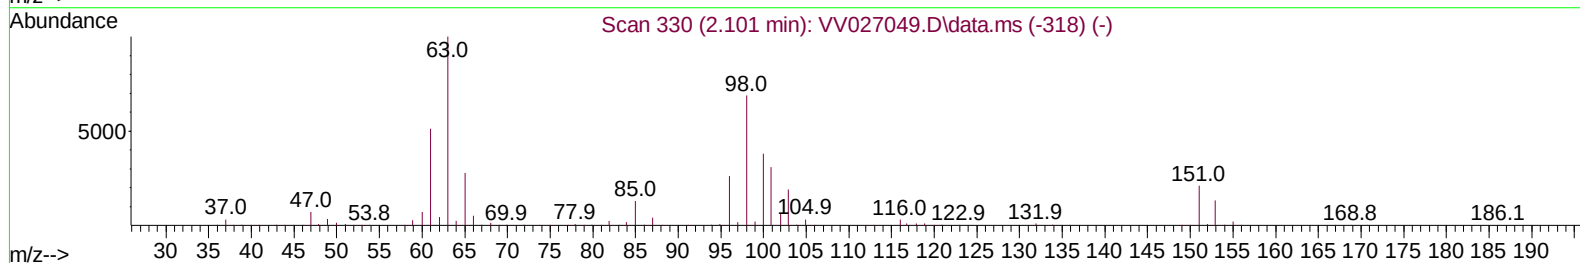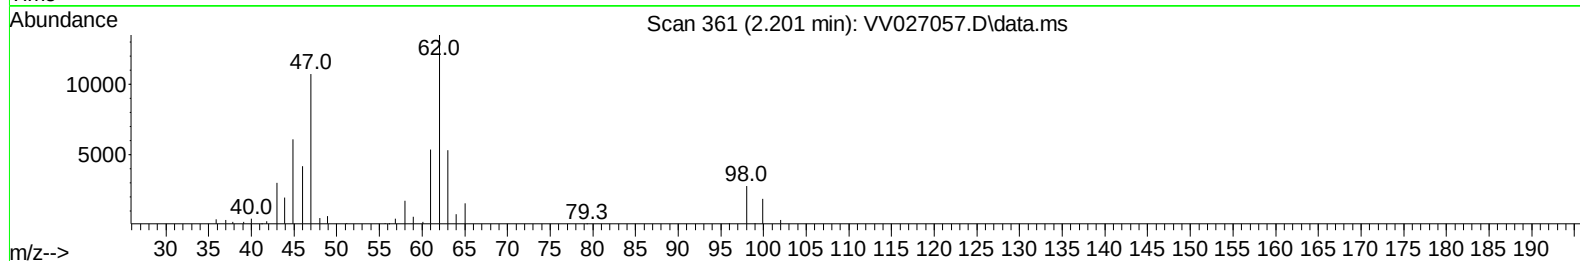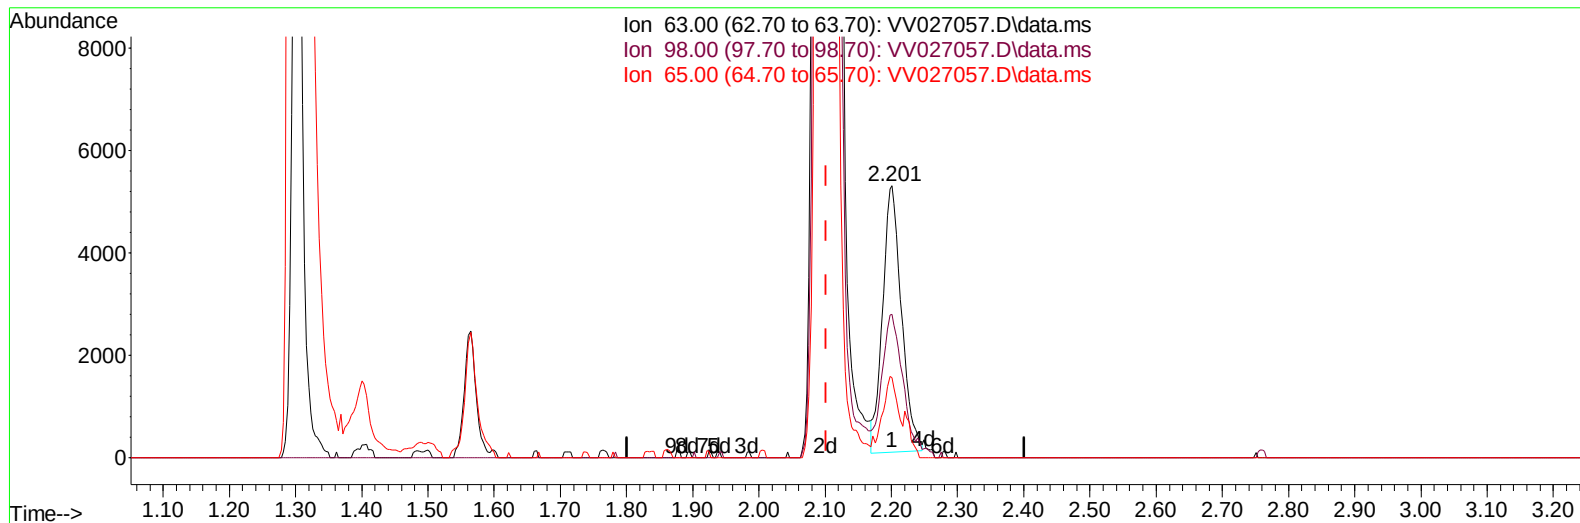

TIC: VV027057.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.201min (+ 0.100) 1.13 ug/L

response 10308

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	57.98
65.00	24.20	24.46
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027057.D
Acq On : 29 Jul 2022 00:29
Operator : SY/MD
Sample : N3899-04 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

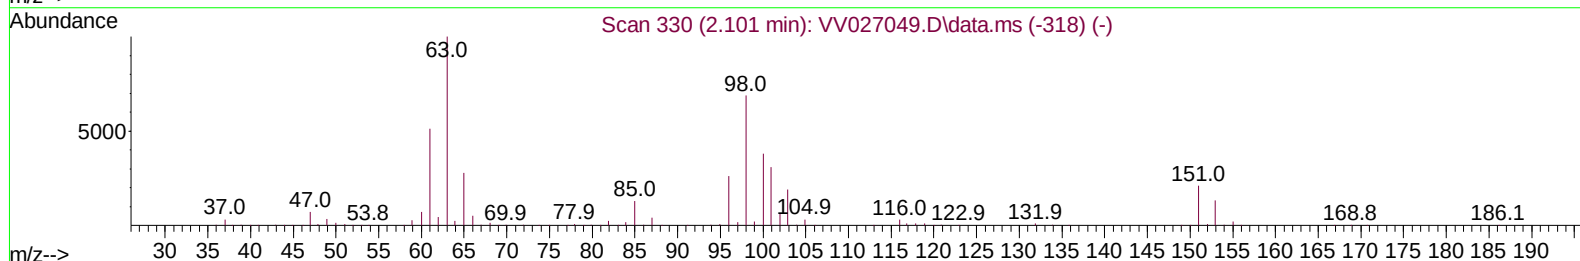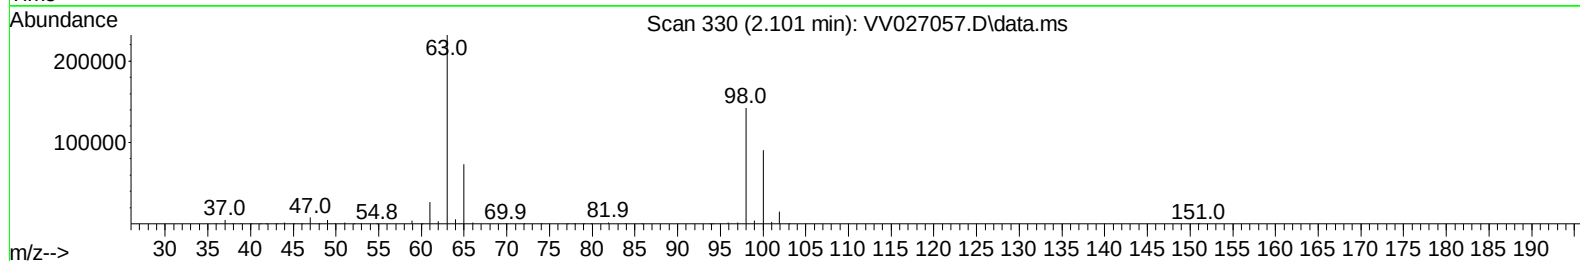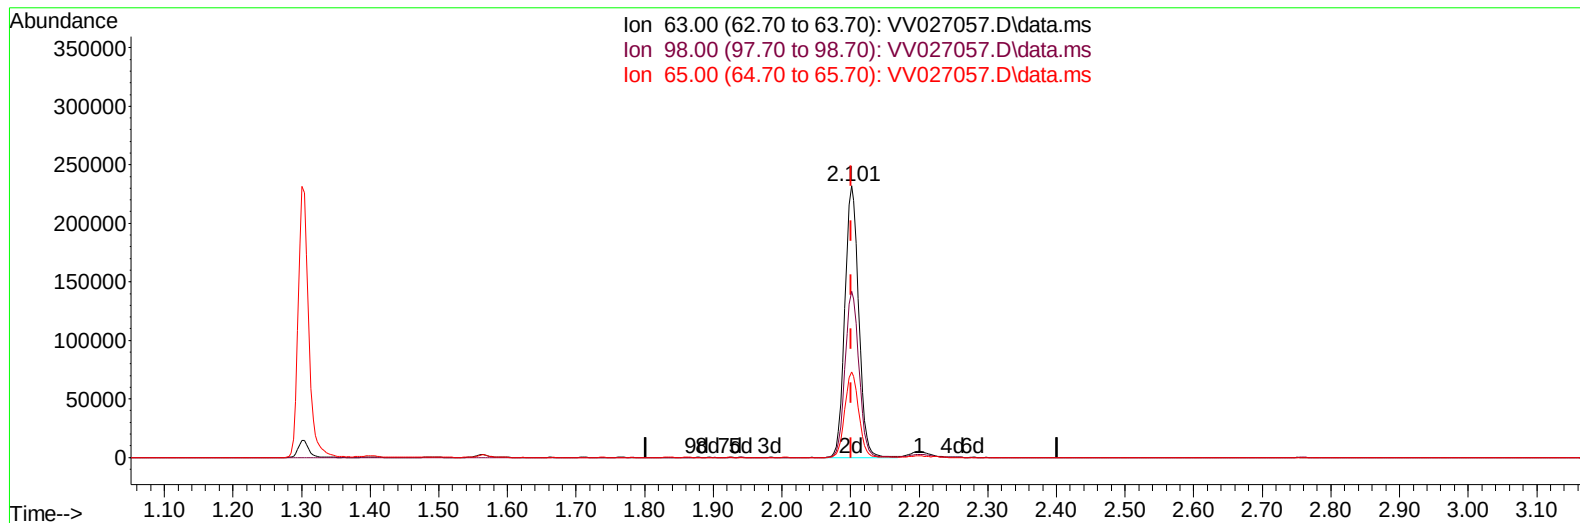

TIC: VV027057.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.000) 35.64 ug/L m

response 323997

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	1.84#
65.00	24.20	0.78#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027057.D
 Acq On : 29 Jul 2022 00:29
 Operator : SY/MD
 Sample : N3899-04 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

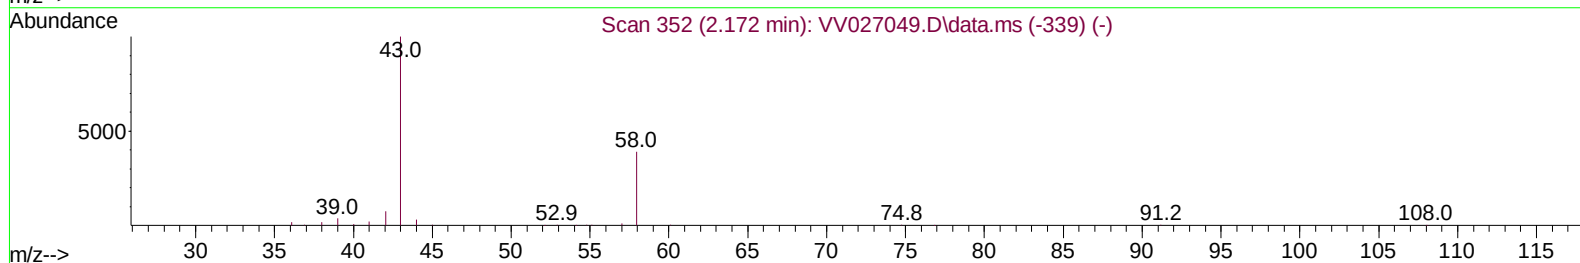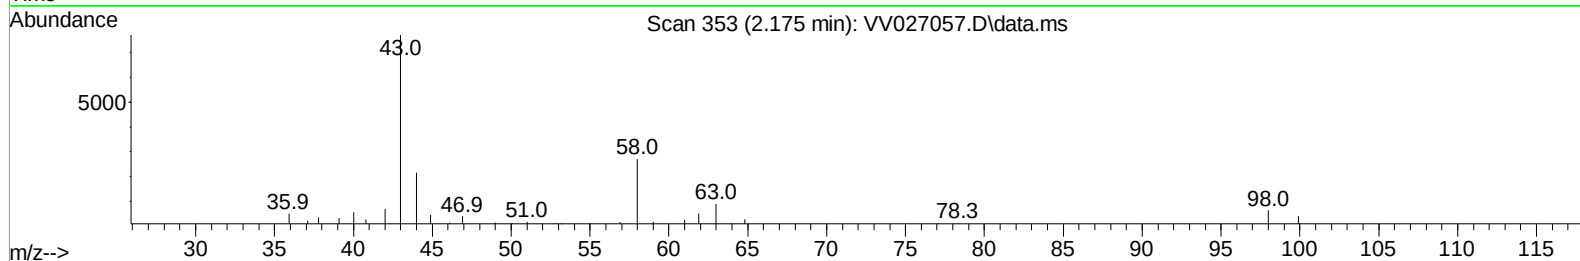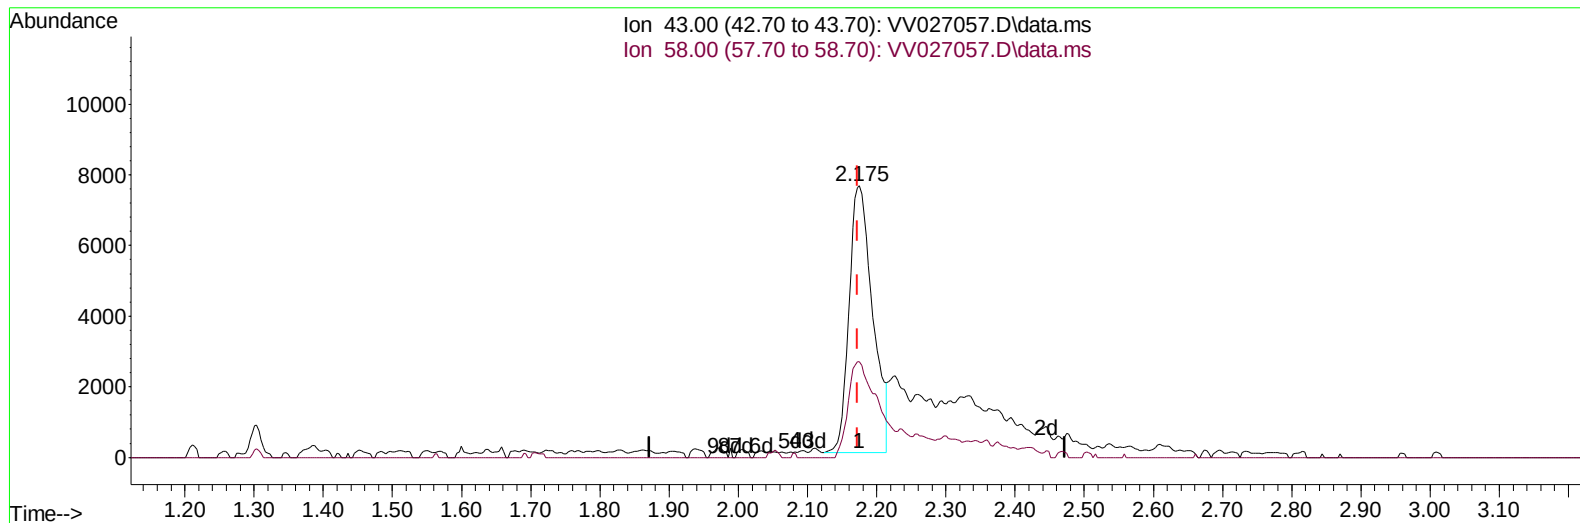

TIC: VV027057.D\data.ms

(13) Acetone (T)

2.175min (+ 0.003) 7.97 ug/L

response 17982

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	24.80	44.99
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027057.D
 Acq On : 29 Jul 2022 00:29
 Operator : SY/MD
 Sample : N3899-04 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

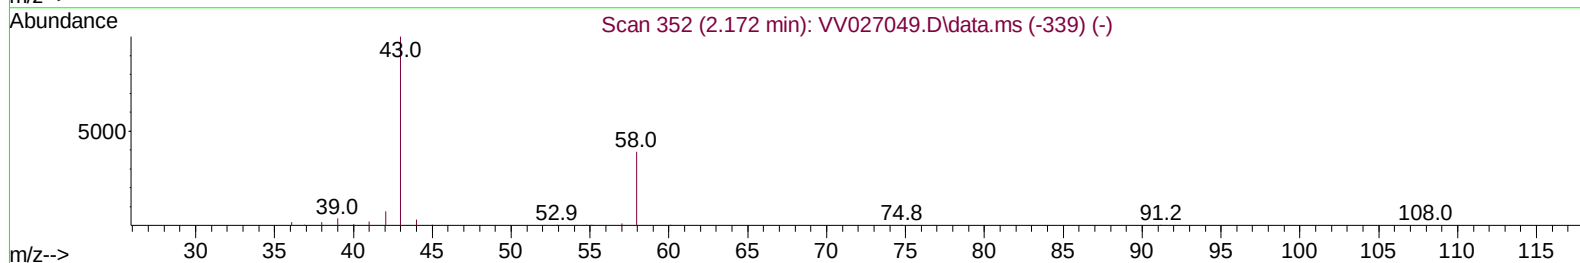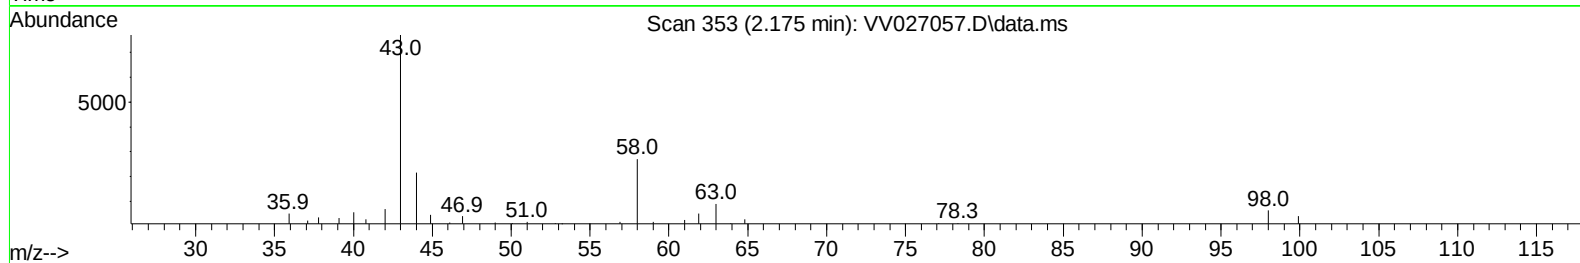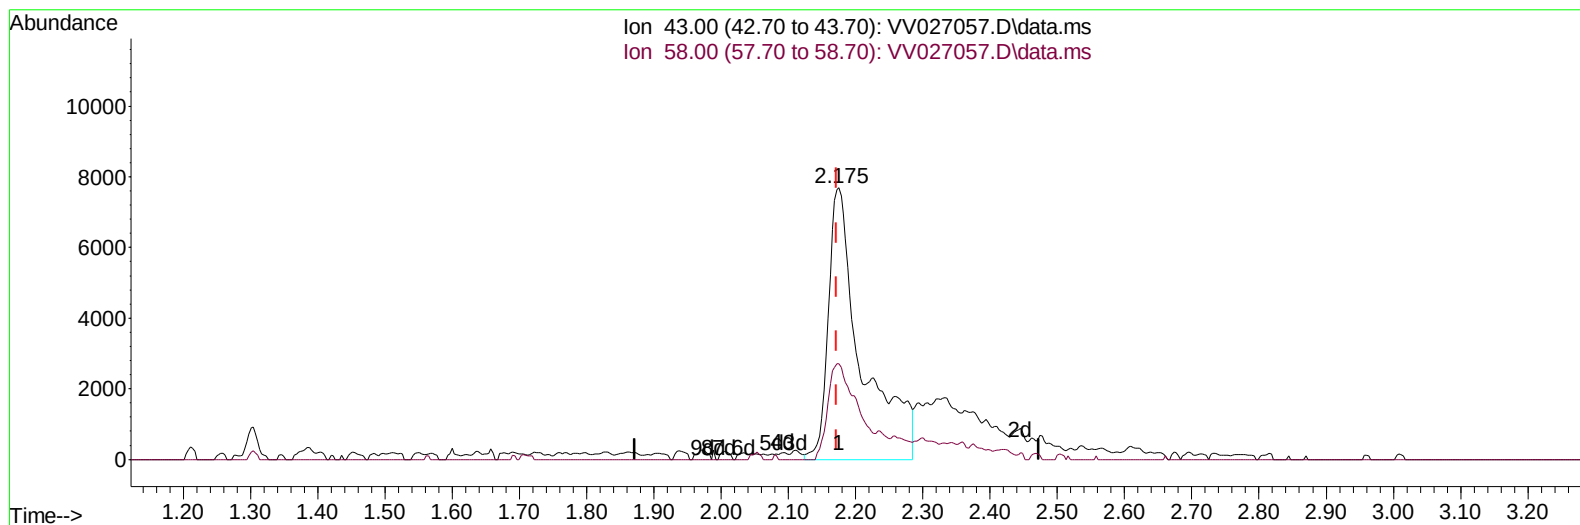

TIC: VV027057.D\data.ms

(13) Acetone (T)

2.175min (+ 0.003) 11.74 ug/L m

response 26473

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	24.80	30.56
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027057.D
 Acq On : 29 Jul 2022 00:29
 Operator : SY/MD
 Sample : N3899-04 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	561311	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	558483	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	249172	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	243497	45.597	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	91.200%	
7) Chloroethane-d5	1.564	69	193176	45.656	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	91.320%	
11) 1,1-Dichloroethene-d2	2.101	63	323997m	35.638	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.280%	
21) 2-Butanone-d5	3.886	46	193871	63.669	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	63.670%	
24) Chloroform-d	4.342	84	418879	43.552	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.100%	
26) 1,2-Dichloroethane-d4	5.027	65	244572	44.795	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.600%	
32) Benzene-d6	5.043	84	856499	43.672	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.340%	
36) 1,2-Dichloropropane-d6	6.066	67	278525	46.401	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.800%	
41) Toluene-d8	7.313	98	744120	41.978	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	83.960%	
43) trans-1,3-Dichloroprop...	7.619	79	106450	40.146	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.300%	
47) 2-Hexanone-d5	8.091	63	203417	78.830	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	78.830%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	383124	42.332	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	84.660%	
66) 1,2-Dichlorobenzene-d4	11.622	152	272077	48.574	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.140%	
Target Compounds						
13) Acetone	2.175	43	26473m	11.738	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027057.D
Acq On : 29 Jul 2022 00:29
Operator : SY/MD
Sample : N3899-04 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR3

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:14:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

