




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027066.D
 Acq On : 29 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3790-13ME
 Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

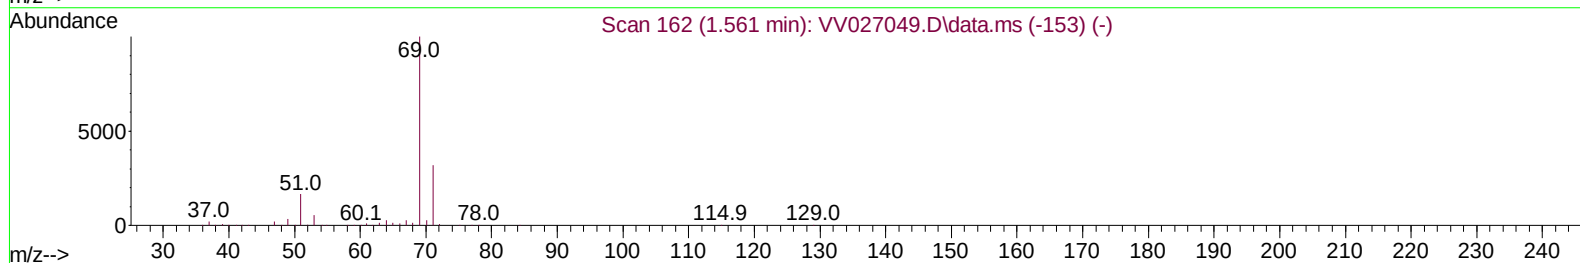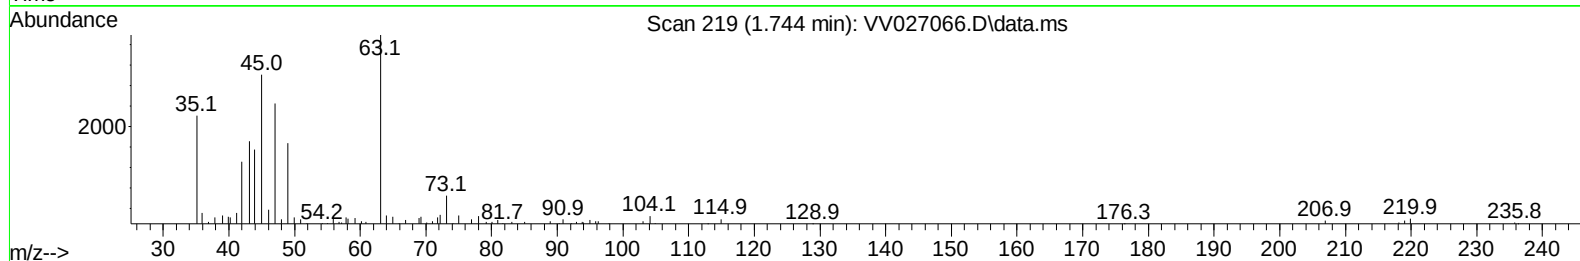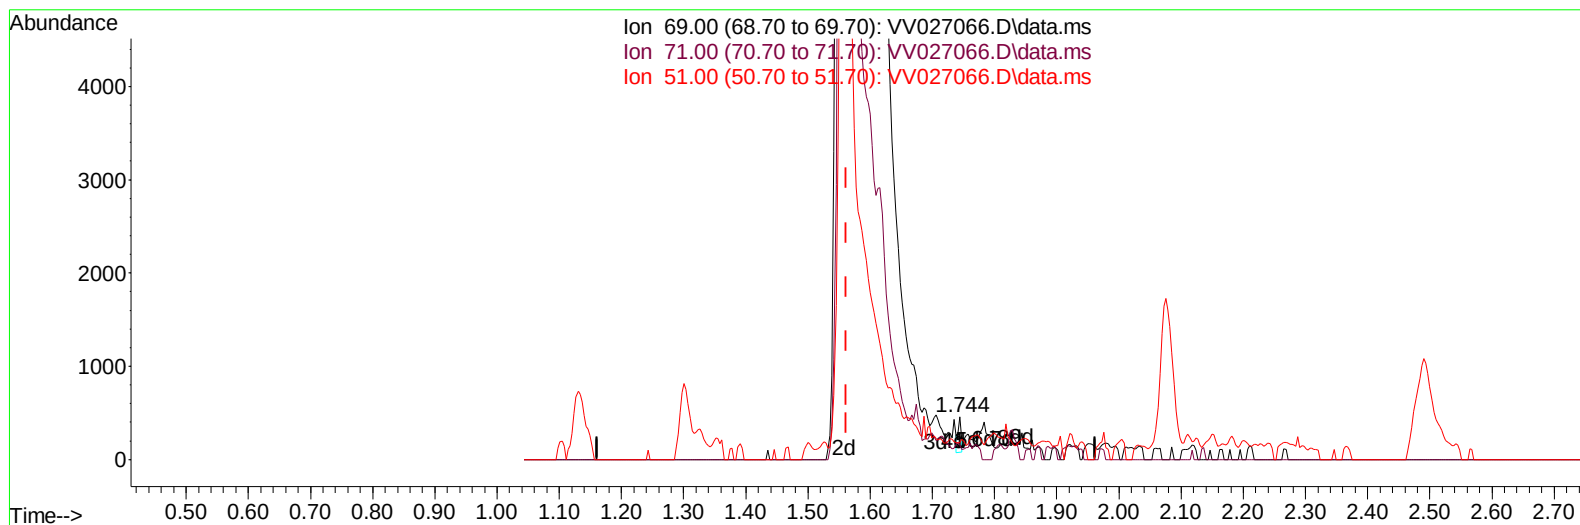

TIC: VV027066.D\data.ms

(7) Chloroethane-d5 (S)

1.744min (+ 0.183) 0.03 ug/L

response 139

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	28.06
51.00	22.80	19.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027066.D
 Acq On : 29 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3790-13ME
 Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

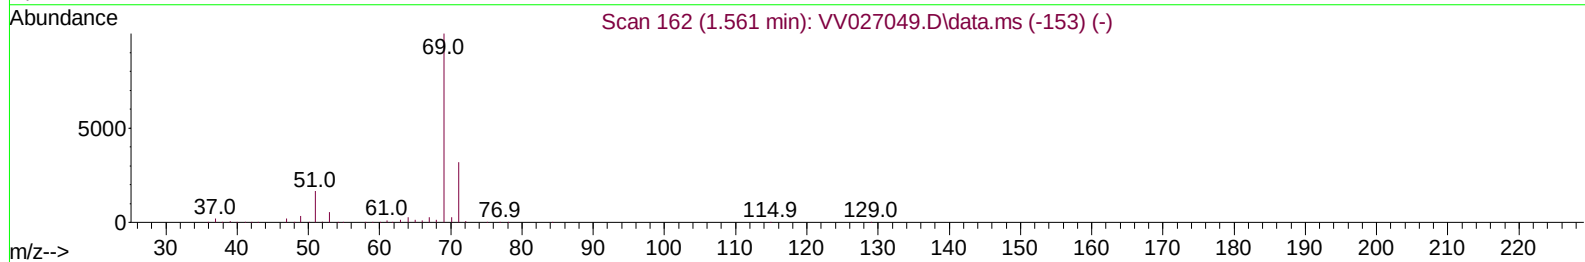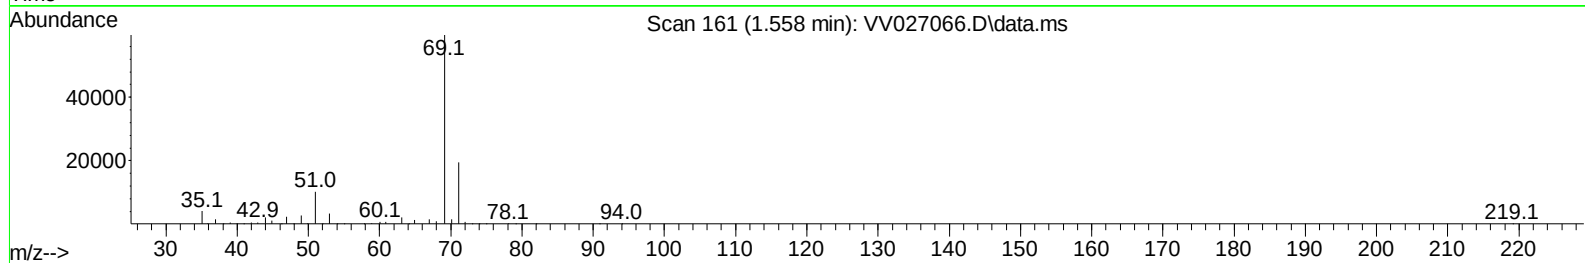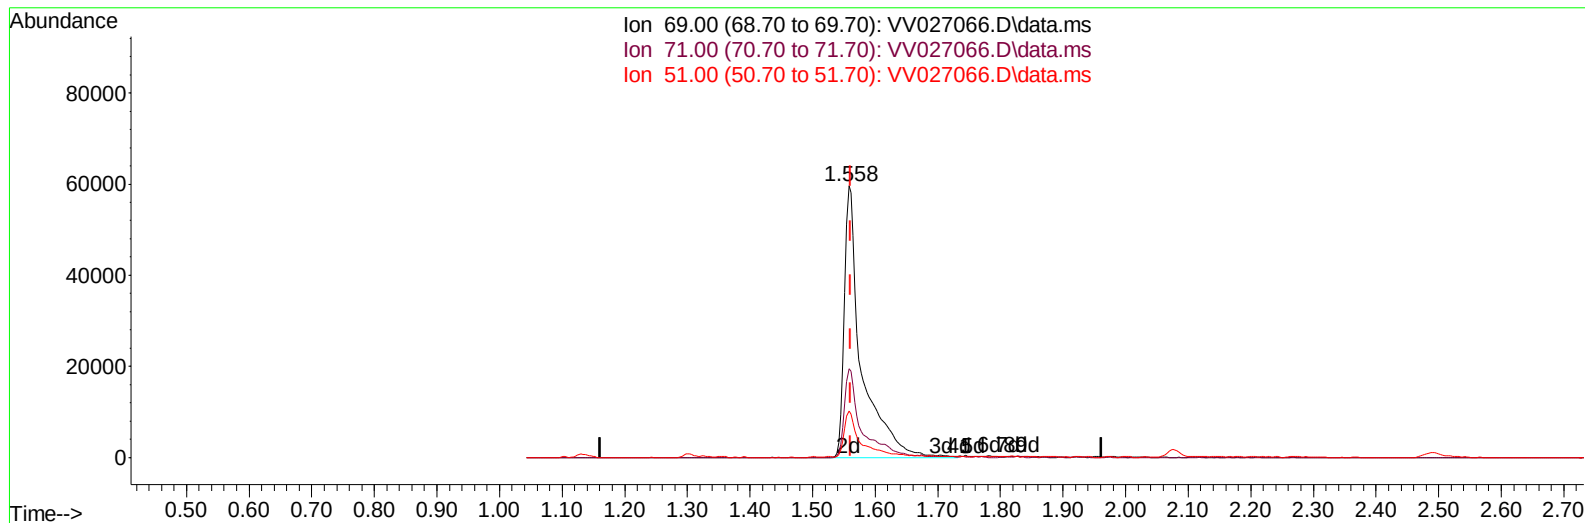

TIC: VV027066.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 25.99 ug/L m

response 113511

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.03#
51.00	22.80	0.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027066.D
 Acq On : 29 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3790-13ME
 Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK7ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 29 05:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

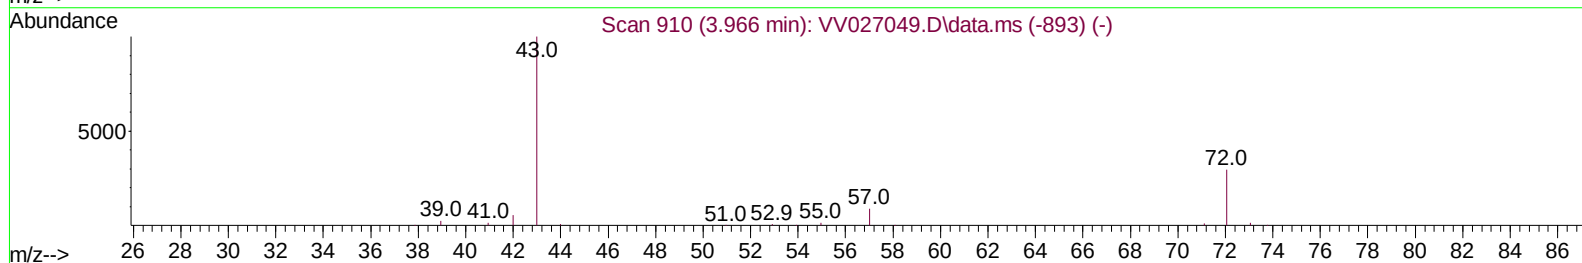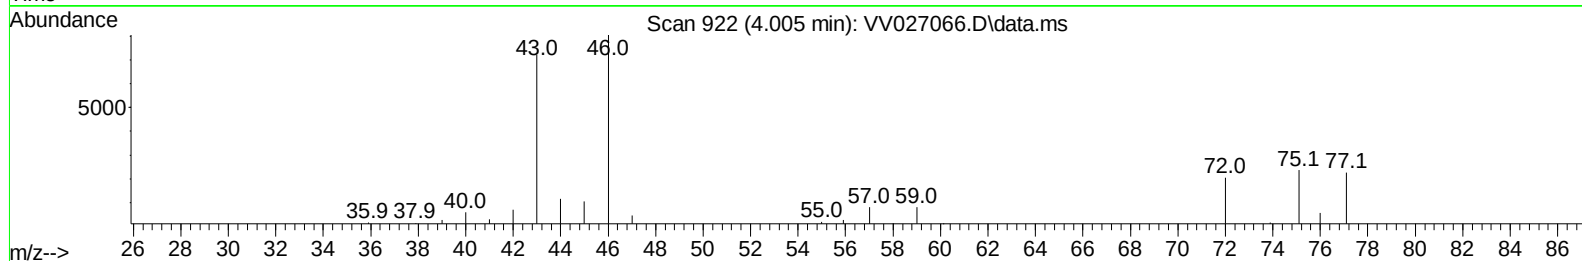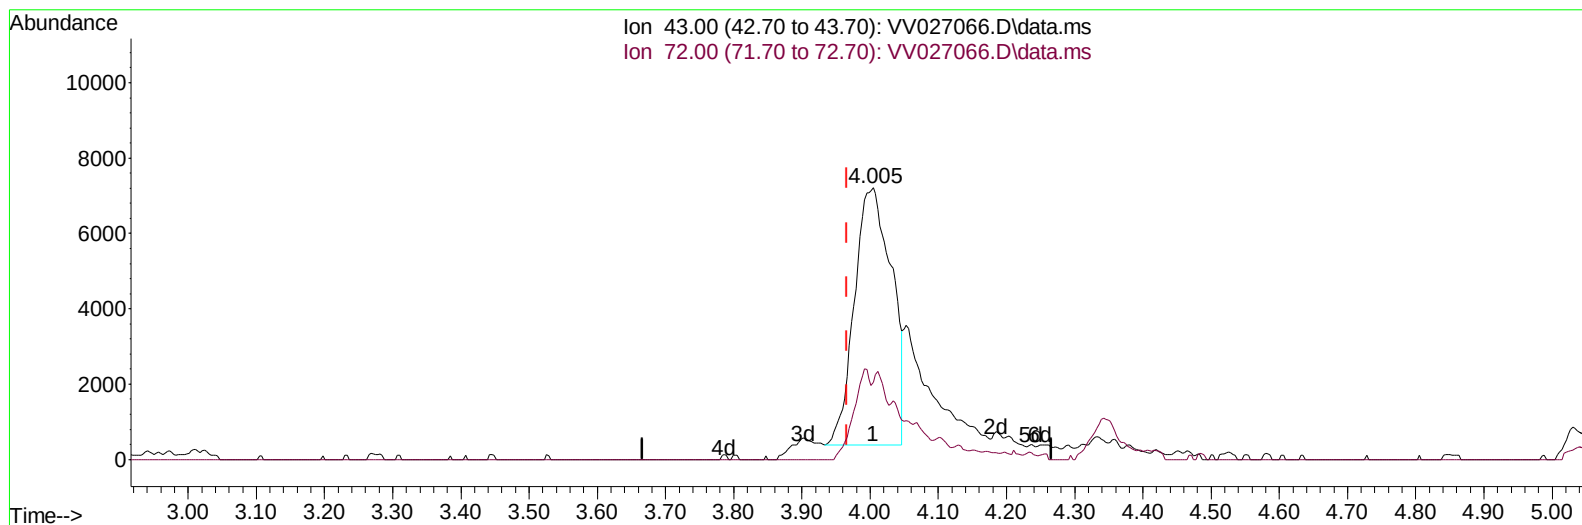

TIC: VV027066.D\data.ms

(22) 2-Butanone (T)

4.005min (+ 0.038) 10.07 ug/L

response 25861

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	15.95
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027066.D
 Acq On : 29 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3790-13ME
 Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

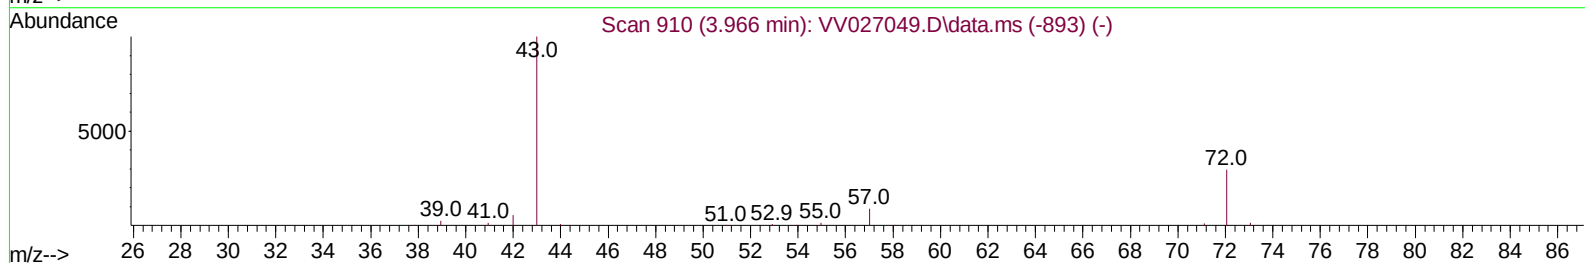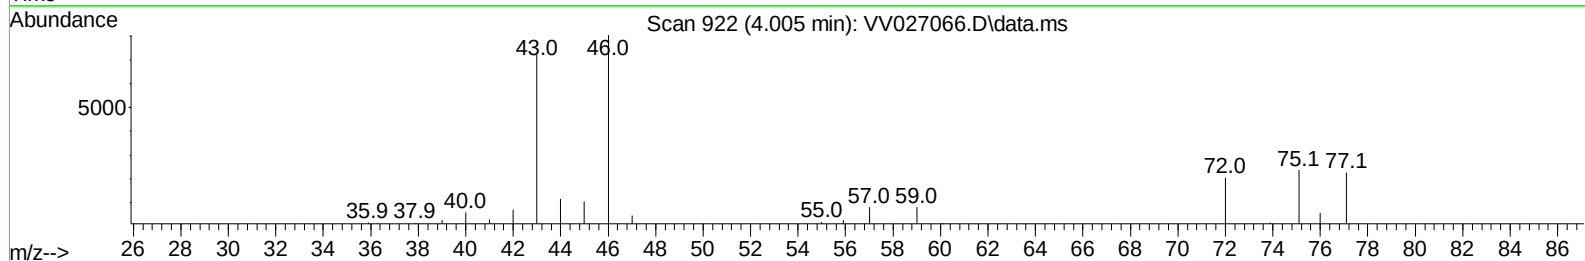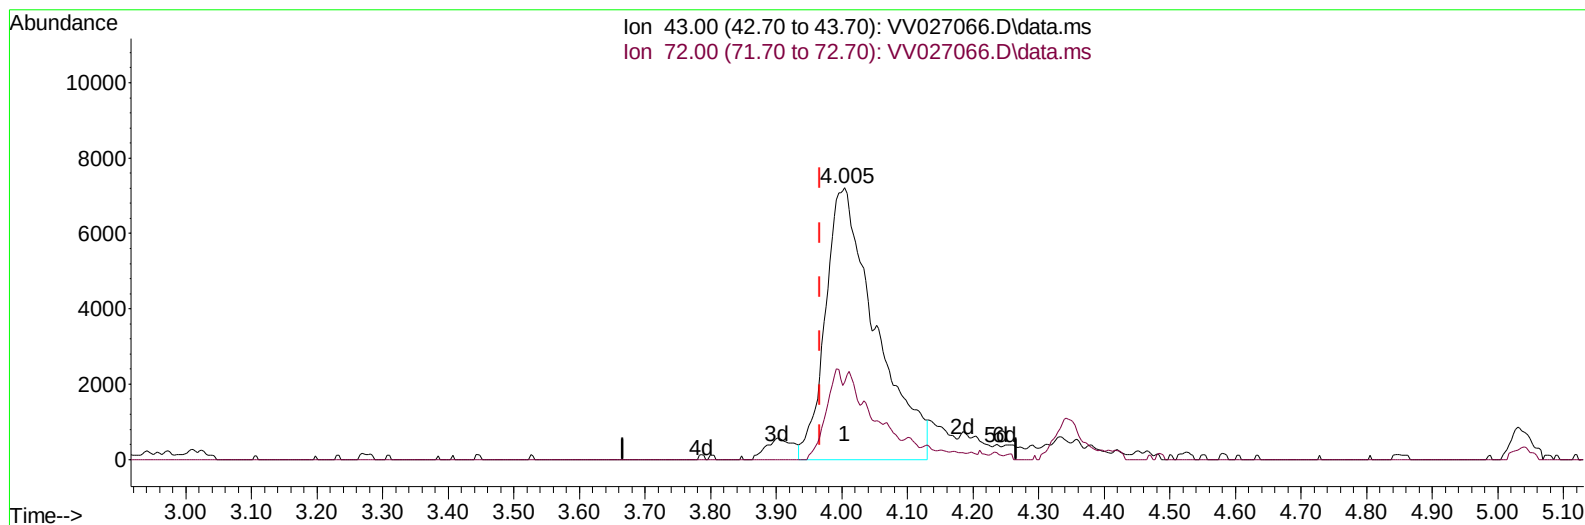

TIC: VV027066.D\data.ms

(22) 2-Butanone (T)

4.005min (+ 0.038) 14.91 ug/L m

response 38306

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	10.77#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027066.D
 Acq On : 29 Jul 2022 04:10
 Operator : SY/MD
 Sample : N3790-13ME
 Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	579420	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	575739	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	247614	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	221413	40.166	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	80.340%	
7) Chloroethane-d5	1.558	69	113511m	25.989	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	51.980%#	
11) 1,1-Dichloroethene-d2	2.076	63	284417	30.307	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	60.620%	
21) 2-Butanone-d5	3.899	46	285526	90.839	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.840%	
24) Chloroform-d	4.339	84	401806	40.471	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	80.940%	
26) 1,2-Dichloroethane-d4	5.024	65	245437	43.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.100%	
32) Benzene-d6	5.037	84	831555	41.130	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	82.260%	
36) 1,2-Dichloropropane-d6	6.063	67	265657	42.930	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	85.860%	
41) Toluene-d8	7.310	98	681945	37.317	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	74.640%#	
43) trans-1,3-Dichloroprop...	7.619	79	100068	36.608	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.220%	
47) 2-Hexanone-d5	8.095	63	185714	69.812	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	69.810%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	351242	37.646	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	75.300%	
66) 1,2-Dichlorobenzene-d4	11.625	152	243629	43.769	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.540%	
Target Compounds						
					Qvalue	
13) Acetone	2.188	43	7690	3.303	ug/L	96
15) Methyl Acetate	2.436	43	21660	5.598	ug/L #	88
22) 2-Butanone	4.005	43	38306m	14.915	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027066.D
Acq On : 29 Jul 2022 04:10
Operator : SY/MD
Sample : N3790-13ME
Misc : 3.18g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUK7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

