




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027067.D
 Acq On : 29 Jul 2022 04:35
 Operator : SY/MD
 Sample : N3790-14ME
 Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK8ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

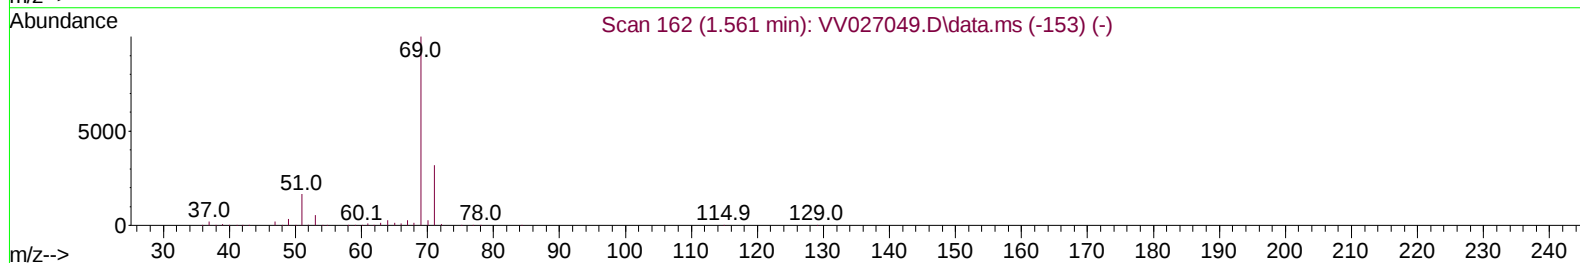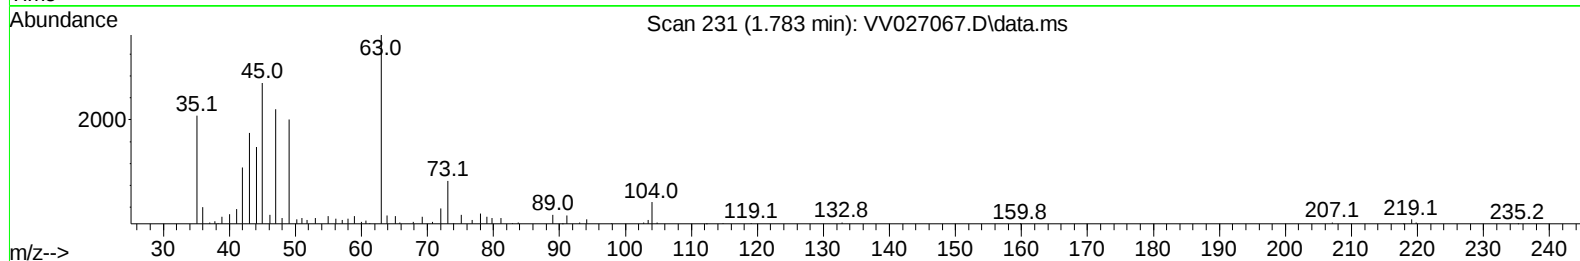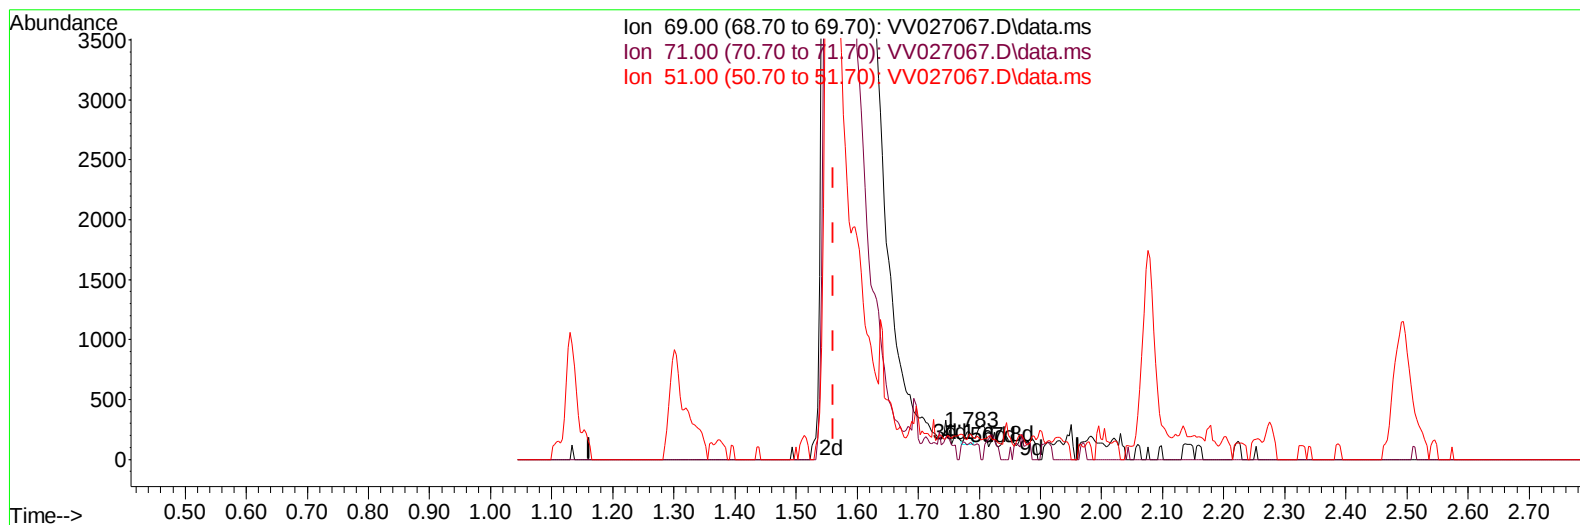

TIC: VV027067.D\data.ms

(7) Chloroethane-d5 (S)

1.783min (+ 0.222) 0.02 ug/L

response 83

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	39.76
51.00	22.80	27.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027067.D
 Acq On : 29 Jul 2022 04:35
 Operator : SY/MD
 Sample : N3790-14ME
 Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK8ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

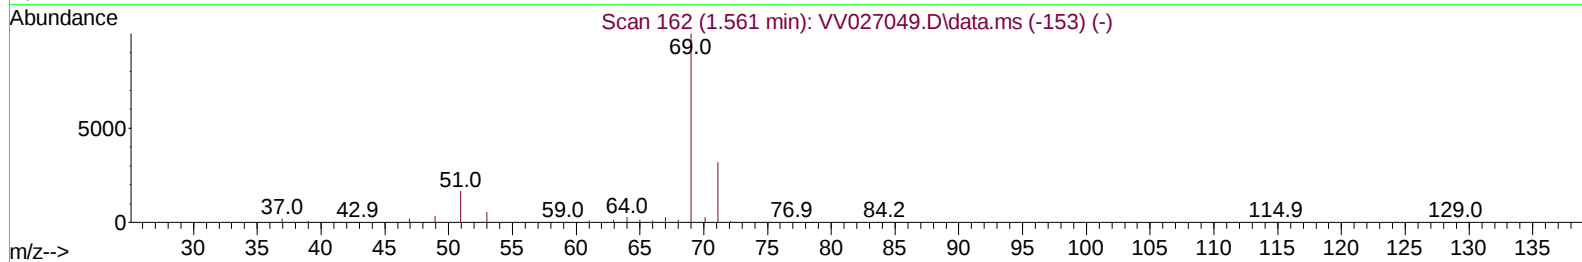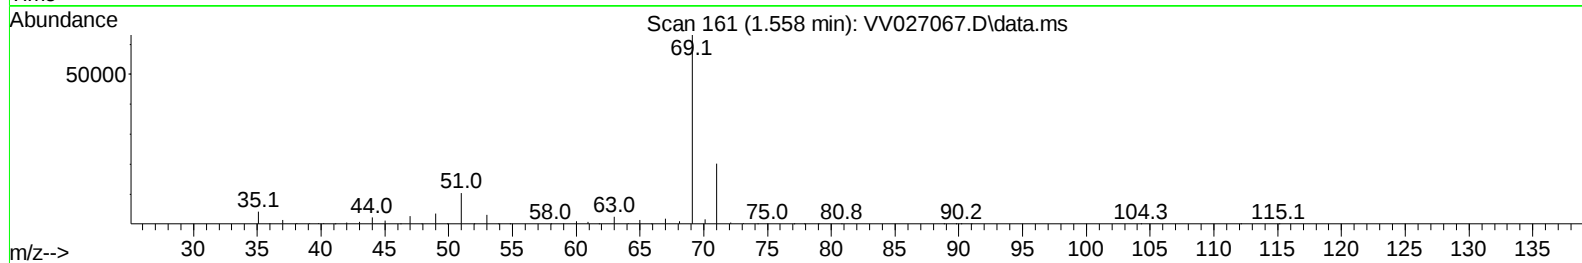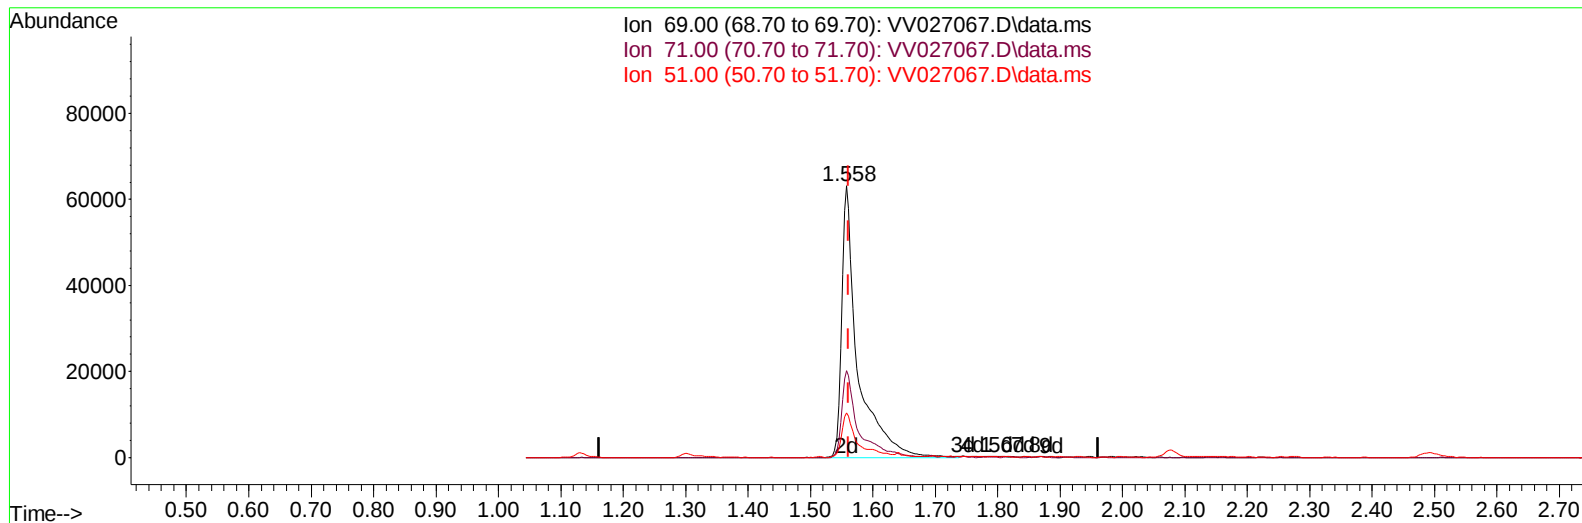

TIC: VV027067.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 24.05 ug/L m

response 113418

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.03#
51.00	22.80	0.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027067.D
 Acq On : 29 Jul 2022 04:35
 Operator : SY/MD
 Sample : N3790-14ME
 Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK8ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 29 05:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

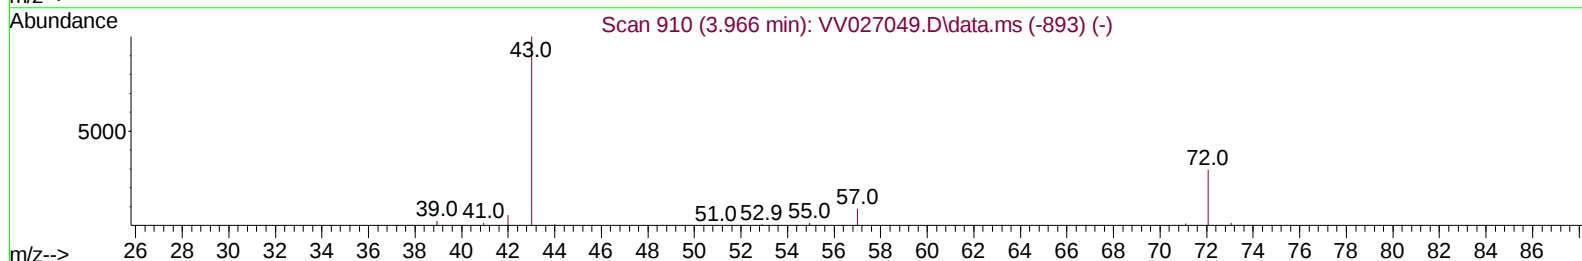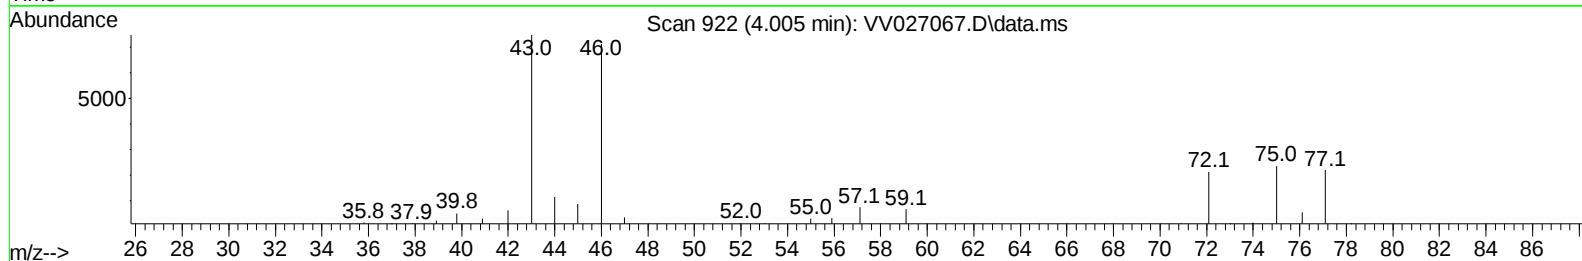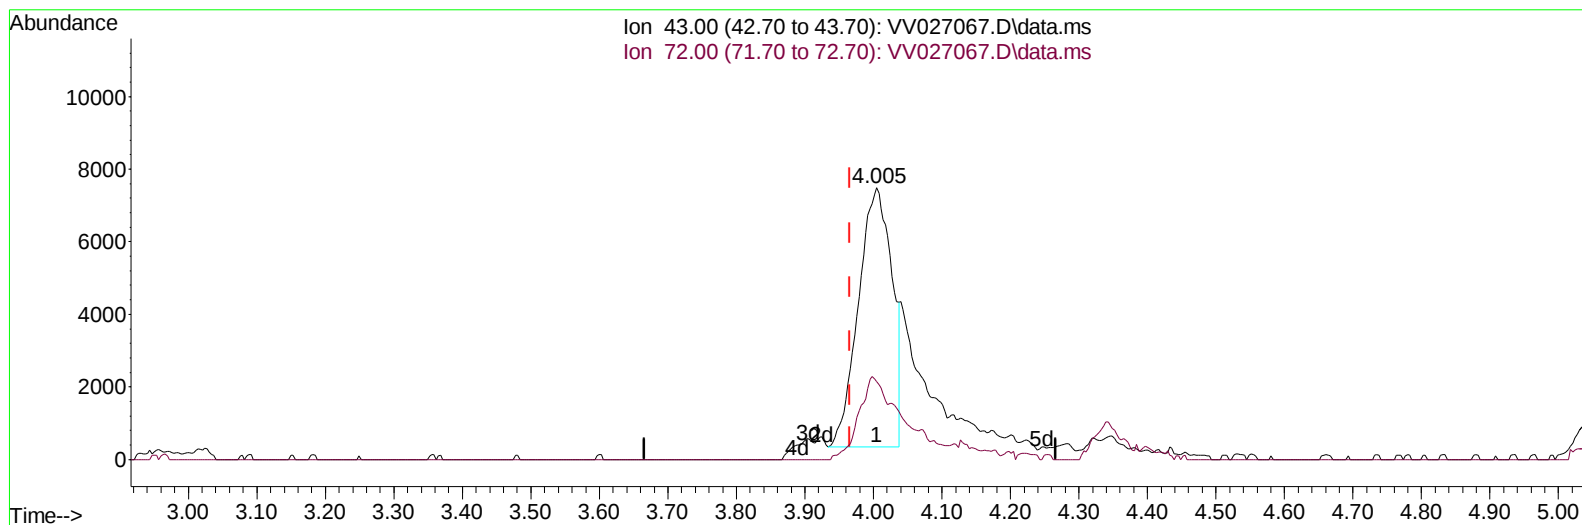

TIC: VV027067.D\data.ms

(22) 2-Butanone (T)

4.005min (+ 0.039) 8.71 ug/L

response 24157

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	22.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027067.D
 Acq On : 29 Jul 2022 04:35
 Operator : SY/MD
 Sample : N3790-14ME
 Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK8ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 29 05:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

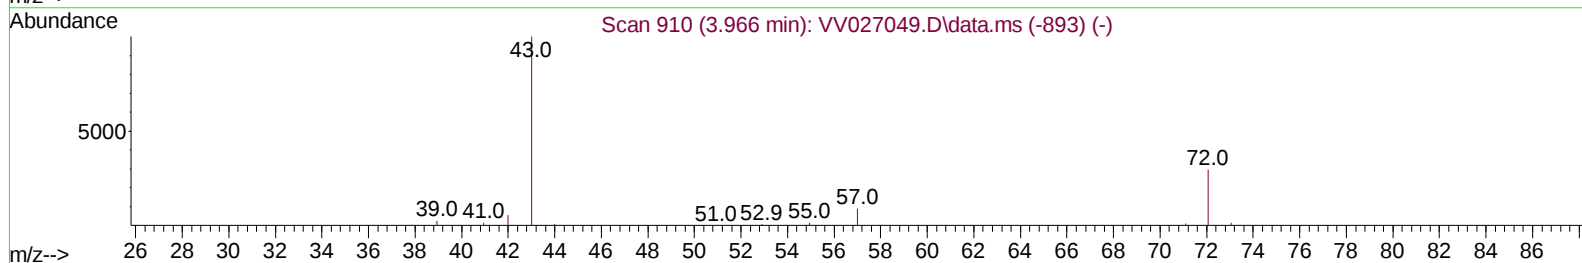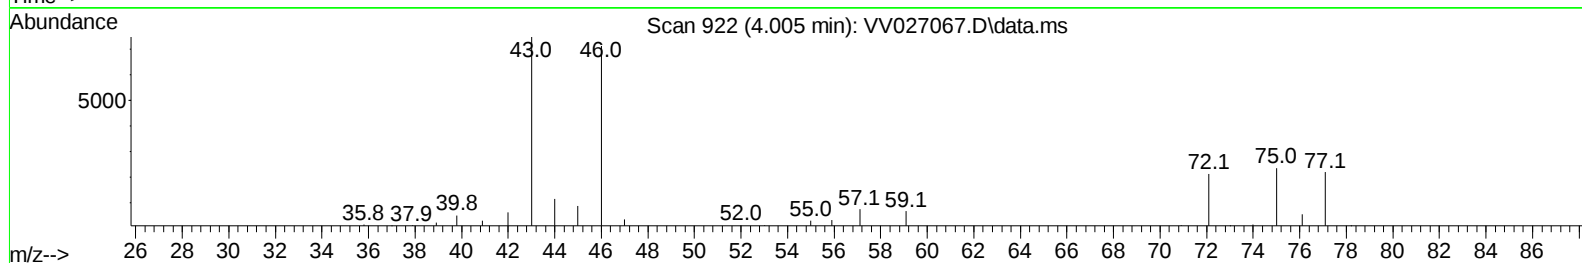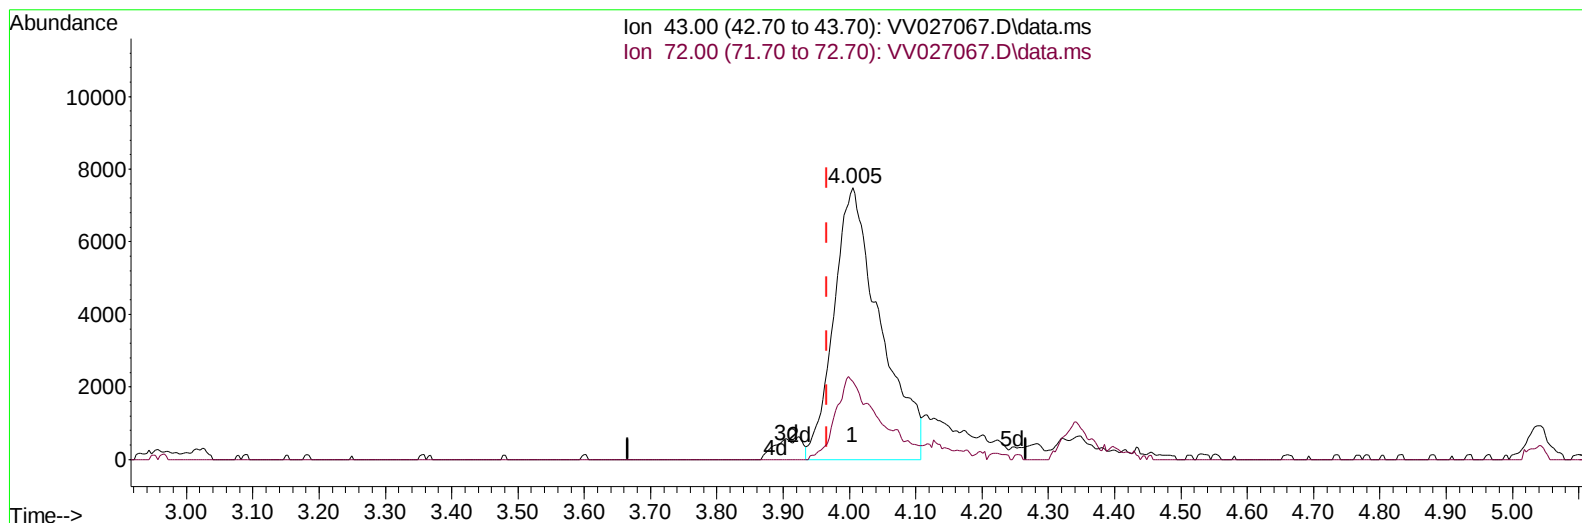

TIC: VV027067.D\data.ms

(22) 2-Butanone (T)

4.005min (+ 0.039) 13.11 ug/L m

response 36344

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	14.70
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027067.D
 Acq On : 29 Jul 2022 04:35
 Operator : SY/MD
 Sample : N3790-14ME
 Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK8ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	625611	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	614361	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	272999	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	229092	38.491	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	76.980%	
7) Chloroethane-d5	1.558	69	113418m	24.051	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	48.100%#	
11) 1,1-Dichloroethene-d2	2.079	63	303754	29.977	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	59.960%#	
21) 2-Butanone-d5	3.899	46	260074	76.632	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	76.630%	
24) Chloroform-d	4.339	84	408410	38.099	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	76.200%	
26) 1,2-Dichloroethane-d4	5.024	65	246931	40.579	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.160%	
32) Benzene-d6	5.037	84	855066	39.634	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.260%	
36) 1,2-Dichloropropane-d6	6.063	67	266843	40.411	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	80.820%	
41) Toluene-d8	7.313	98	716592	36.748	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	73.500%#	
43) trans-1,3-Dichloroprop...	7.619	79	100622	34.496	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	69.000%	
47) 2-Hexanone-d5	8.095	63	179381	63.192	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	63.190%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	348394	34.993	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	69.980%	
66) 1,2-Dichlorobenzene-d4	11.625	152	254555	41.479	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.960%	
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	8672	3.450	ug/L	82
15) Methyl Acetate	2.436	43	28735	6.879	ug/L	93
22) 2-Butanone	4.005	43	36344m	13.106	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027067.D
Acq On : 29 Jul 2022 04:35
Operator : SY/MD
Sample : N3790-14ME
Misc : 3.46g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUK8ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 05:16:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

