




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027068.D
 Acq On : 29 Jul 2022 04:59
 Operator : SY/MD
 Sample : N3790-15ME
 Misc : 5.21g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK9ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 06:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

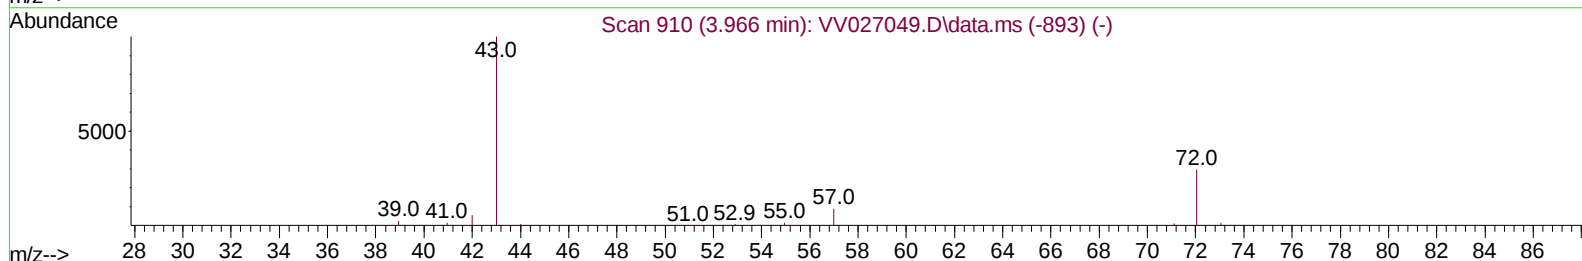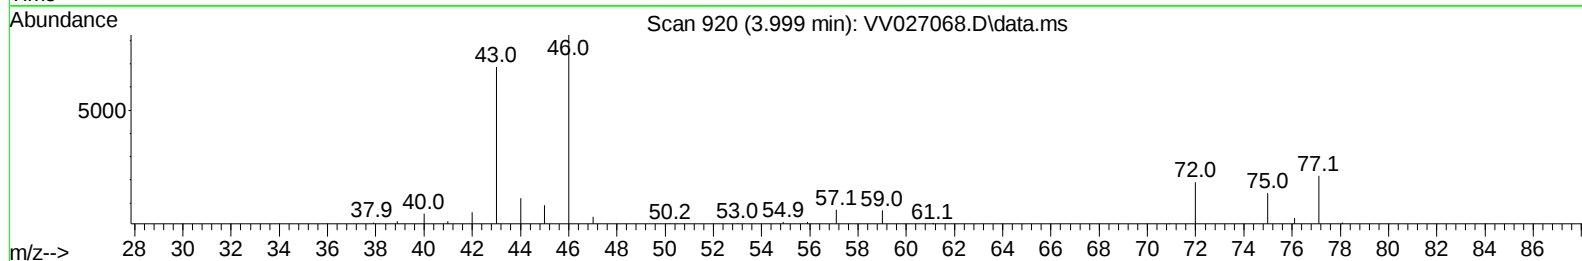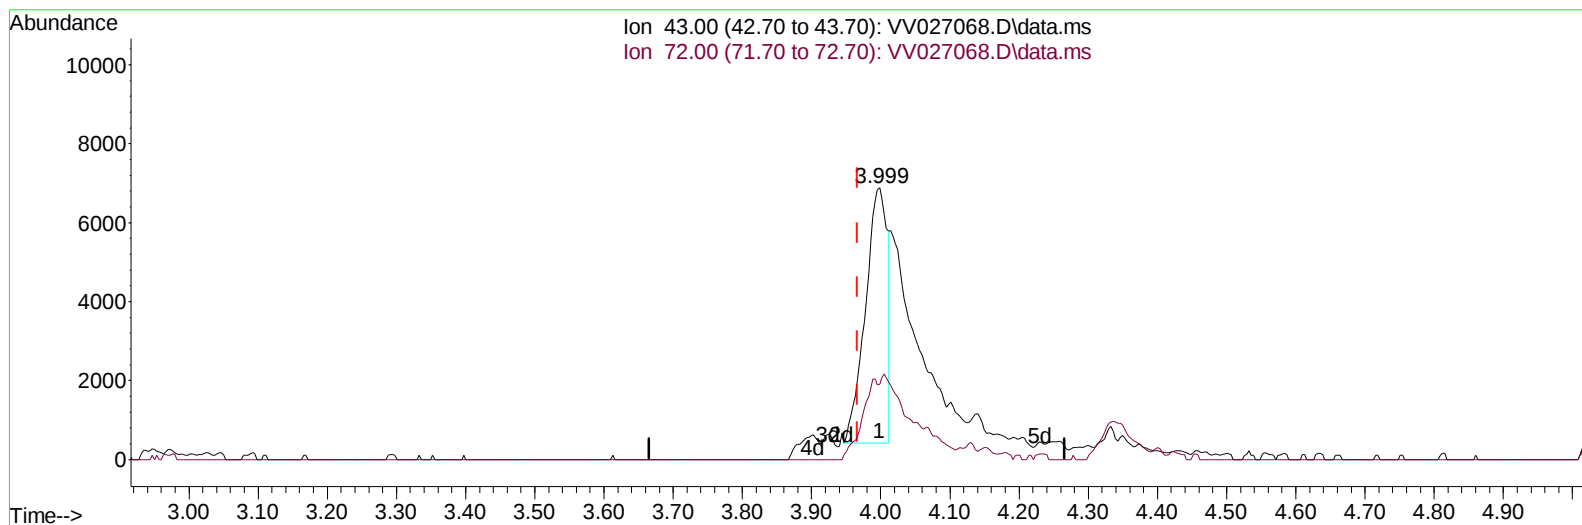

TIC: VV027068.D\data.ms

(22) 2-Butanone (T)

3.999min (+ 0.032) 5.26 ug/L

response 14201

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	22.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027068.D
 Acq On : 29 Jul 2022 04:59
 Operator : SY/MD
 Sample : N3790-15ME
 Misc : 5.21g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK9ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 06:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

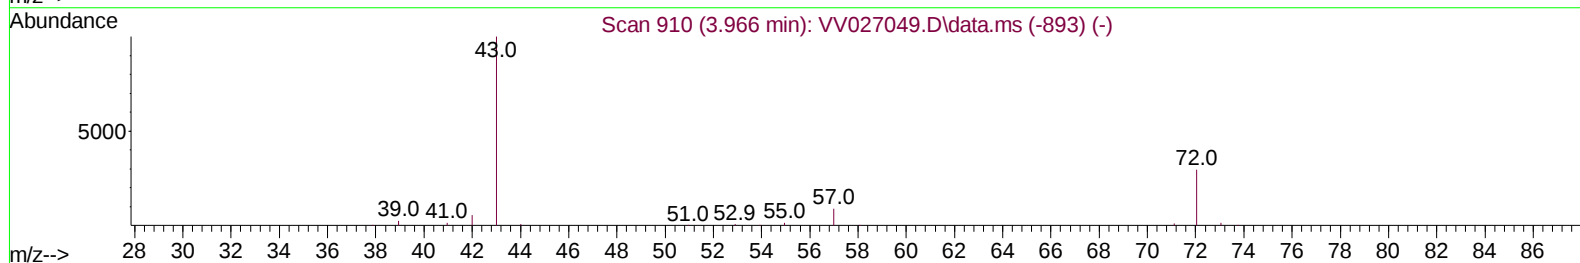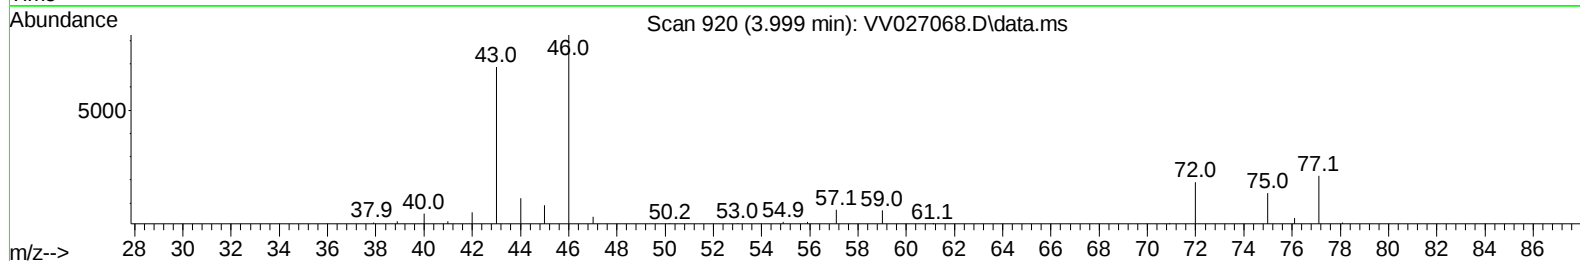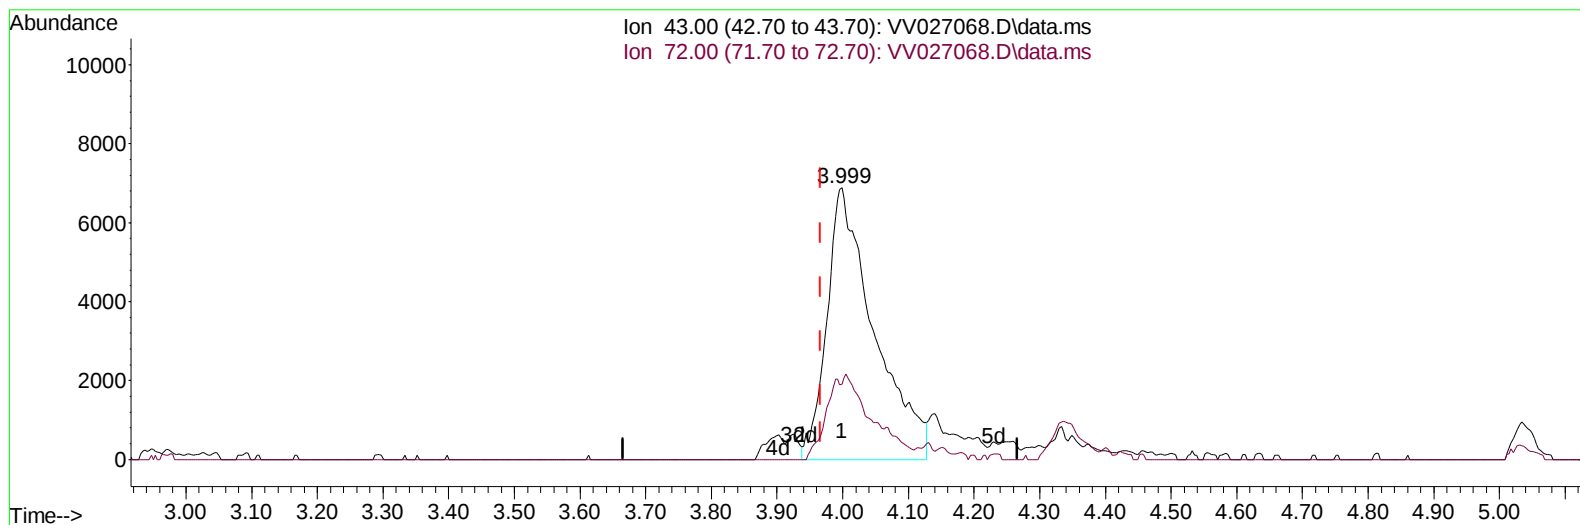

TIC: VV027068.D\data.ms

(22) 2-Butanone (T)

3.999min (+ 0.032) 12.65 ug/L m

response 34169

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.80	9.32#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027068.D
 Acq On : 29 Jul 2022 04:59
 Operator : SY/MD
 Sample : N3790-15ME
 Misc : 5.21g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUK9ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 06:16:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	609403	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	602959	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	286000	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	225782	38.944	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	77.880%	
7) Chloroethane-d5	1.558	69	106838	23.258	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	46.520%#	
11) 1,1-Dichloroethene-d2	2.079	63	304584	30.859	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	61.720%	
21) 2-Butanone-d5	3.899	46	281032	85.010	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	85.010%	
24) Chloroform-d	4.339	84	404501	38.738	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	77.480%	
26) 1,2-Dichloroethane-d4	5.024	65	242387	40.892	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.780%	
32) Benzene-d6	5.037	84	846729	39.990	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.980%	
36) 1,2-Dichloropropane-d6	6.063	67	267047	41.207	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	82.420%	
41) Toluene-d8	7.310	98	707575	36.972	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	73.940%#	
43) trans-1,3-Dichloroprop...	7.619	79	99926	34.906	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	69.820%	
47) 2-Hexanone-d5	8.098	63	186388	66.903	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	66.900%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	358156	36.654	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	73.300%	
66) 1,2-Dichlorobenzene-d4	11.625	152	261792	40.719	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.440%	
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	12004	4.902	ug/L	52
15) Methyl Acetate	2.433	43	38235	9.396	ug/L	90
22) 2-Butanone	3.999	43	34169m	12.649	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027068.D
Acq On : 29 Jul 2022 04:59
Operator : SY/MD
Sample : N3790-15ME
Misc : 5.21g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUK9ME

Manual IntegrationsAPPROVED

Quant Time: Jul 29 06:16:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

