

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027057.D
 Acq On : 29 Jul 2022 00:29
 Operator : SY/MD
 Sample : N3899-04 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 29 05:14:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 29 02:10:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	561311	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	558483	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	249172	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	243497	45.597	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.200%		
7) Chloroethane-d5	1.564	69	193176	45.656	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.320%		
11) 1,1-Dichloroethene-d2	2.101	63	323997m	35.638	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.280%		
21) 2-Butanone-d5	3.886	46	193871	63.669	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	63.670%		
24) Chloroform-d	4.342	84	418879	43.552	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.100%		
26) 1,2-Dichloroethane-d4	5.027	65	244572	44.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.600%		
32) Benzene-d6	5.043	84	856499	43.672	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.340%		
36) 1,2-Dichloropropane-d6	6.066	67	278525	46.401	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.800%		
41) Toluene-d8	7.313	98	744120	41.978	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.960%		
43) trans-1,3-Dichloroprop...	7.619	79	106450	40.146	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.300%		
47) 2-Hexanone-d5	8.091	63	203417	78.830	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.830%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	383124	42.332	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.660%		
66) 1,2-Dichlorobenzene-d4	11.622	152	272077	48.574	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.140%		
Target Compounds					Qvalue	
13) Acetone	2.175	43	26473m	11.738	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027057.D
Acq On : 29 Jul 2022 00:29
Operator : SY/MD
Sample : N3899-04 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBUR3

Quant Time: Jul 29 05:14:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 29 02:10:37 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/29/2022
Supervised By :Mahesh Dadoda 08/01/2022

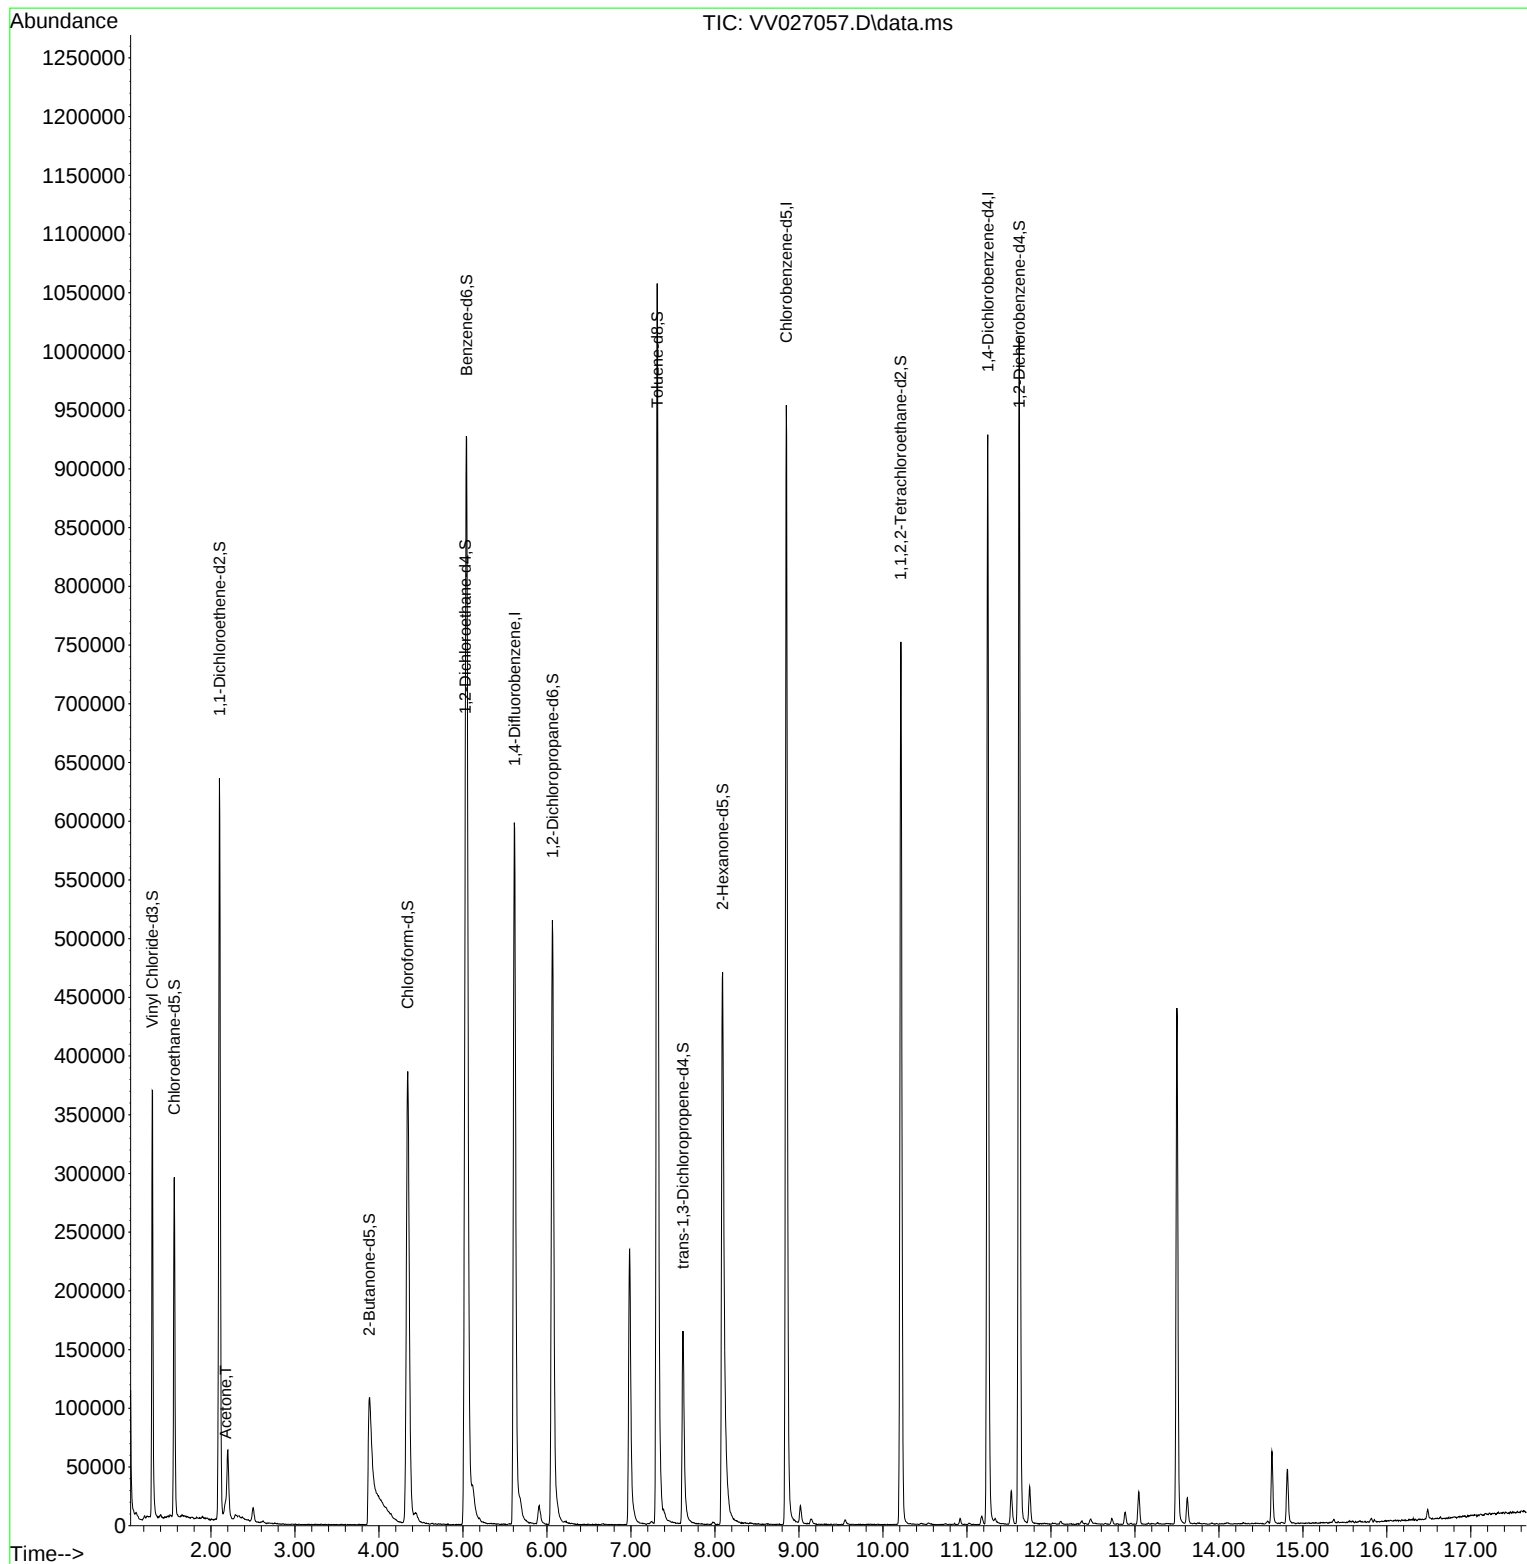

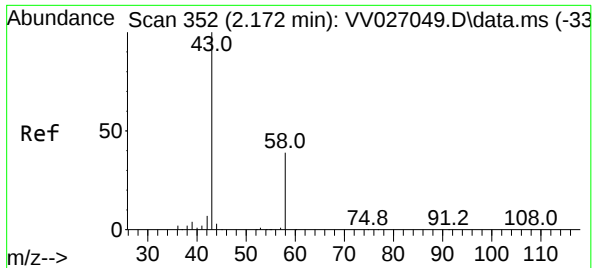

#13
 Acetone
 Concen: 11.738 ug/L m
 RT: 2.175 min Scan# 30
 Delta R.T. 0.003 min
 Lab File: VV027057.D
 Acq: 29 Jul 2022 00:29

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR3

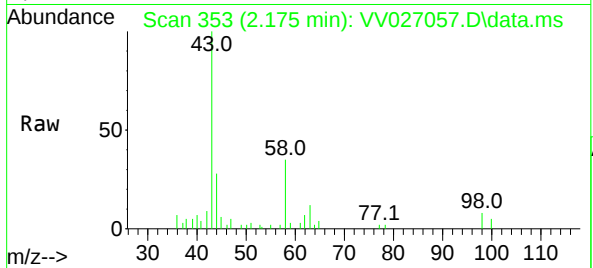

Tgt Ion: 43 Resp: 2647
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 49.6

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/29/2022
 Supervised By :Mahesh Dadoda 08/01/2022

